
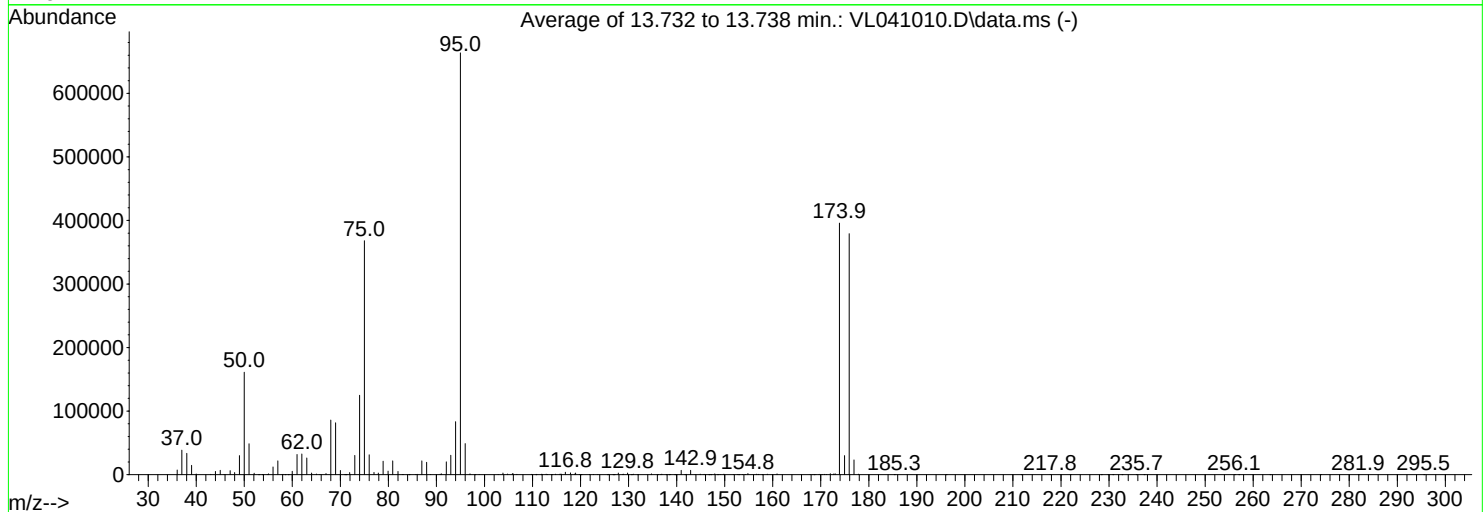


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012424\
Data File : VL041010.D
Acq On : 24 Jan 2024 10:42
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL012324AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jan 25 03:13:06 2024

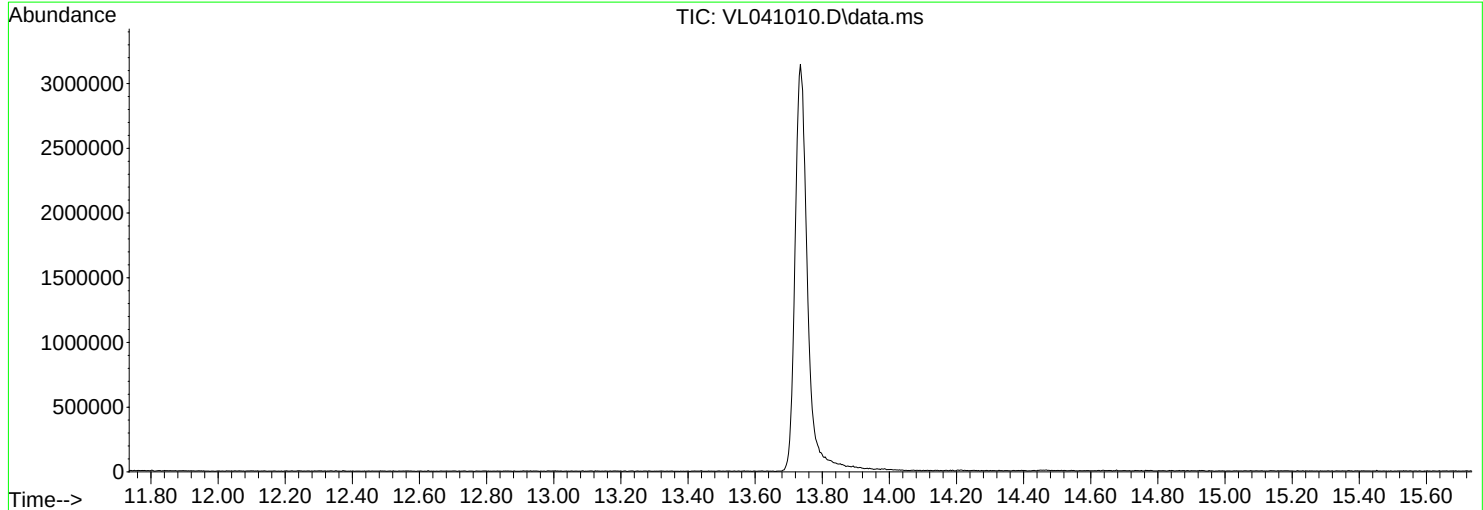

AutoFind: Scans 3461, 3462, 3463; Background Corrected with Scan 3432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	161173	PASS
75	95	30	66	55.5	368147	PASS
95	95	100	100	100.0	663765	PASS
96	95	5	9	7.4	48867	PASS
173	174	0.00	2	0.4	1481	PASS
174	95	50	120	59.6	395861	PASS
175	174	4	9	7.6	29933	PASS
176	174	93	101	95.8	379072	PASS
177	176	5	9	6.1	23149	PASS

Average of 13.732 to 13.738 min.: VL041010.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7371	48.00	3300	57.00	21608	65.75	261
37.00	38451	49.00	30024	57.90	357	67.00	184
38.05	33403	50.00	161173	58.05	557	68.00	8597
39.05	14697	51.00	48563	58.50	71	69.00	8172
40.00	1016	52.05	2196	59.15	155	70.00	6455
43.05	522	53.00	64	60.00	5316	70.90	84
44.00	5106	53.80	111	61.00	31661	71.20	65
45.00	6912	54.00	325	62.00	32467	71.95	3231
45.80	318	54.80	368	63.00	26165	73.00	30275
46.00	319	55.05	1341	64.00	2601	74.00	124896
47.05	6321	56.00	12117	65.00	937	75.00	368147

Average of 13.732 to 13.738 min.: VL041010.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	31200	86.00	467	97.00	1325	110.85	520
77.00	3495	86.95	21659	98.00	63	111.80	134
77.90	2431	87.95	19387	98.90	220	111.95	752
78.90	21104	88.80	235	102.85	326	112.85	856
79.95	5472	90.80	770	103.85	2542	113.10	173
80.90	21536	91.05	1236	104.80	932	113.95	151
82.00	4931	92.05	20165	105.80	1638	114.80	777
82.90	410	93.00	30490	105.95	1528	115.70	699
83.10	246	94.00	83469	106.75	637	115.95	1035
84.30	94	95.00	663765	109.85	469	116.85	3917
85.70	253	96.00	48867	110.70	152	117.90	2731

Average of 13.732 to 13.738 min.: VL041010.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.80	909	127.85	2502	137.80	79	145.70	480
118.95	2511	128.80	452	138.40	155	146.00	290
119.75	208	128.95	766	138.75	220	146.70	159
120.10	156	129.80	2401	139.60	129	146.90	280
121.85	287	130.60	138	140.05	362	147.10	55
122.70	338	131.00	799	140.95	6710	147.95	1244
123.60	239	131.90	58	141.70	135	148.50	143
125.60	57	134.75	1325	142.00	572	149.05	402
125.90	499	136.00	62	142.90	6927	149.85	725
126.75	146	136.70	323	143.85	370	151.80	270
127.00	108	136.90	888	144.90	672	152.70	266

Average of 13.732 to 13.738 min.: VL041010.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.90	118	168.60	50	175.90	379072	232.70	69
153.75	302	169.00	296	176.90	23149	235.70	144
154.30	179	169.65	476	177.85	840	237.30	103
154.85	1858	170.30	160	185.30	78	256.10	131
156.65	645	170.80	583	196.10	54	257.00	84
157.05	510	171.20	218	211.70	66	263.50	53
157.80	136	172.00	1583	217.75	184	274.00	84
158.85	715	172.70	1105	221.90	93	281.90	154
160.90	1233	173.00	1481	228.40	74	295.50	85
167.80	276	173.90	395861	229.80	67		
168.35	160	174.95	29933	230.80	55		