


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012524\
Data File : VL041023.D
Acq On : 25 Jan 2024 9:10
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL012324AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Jan 26 01:06:47 2024

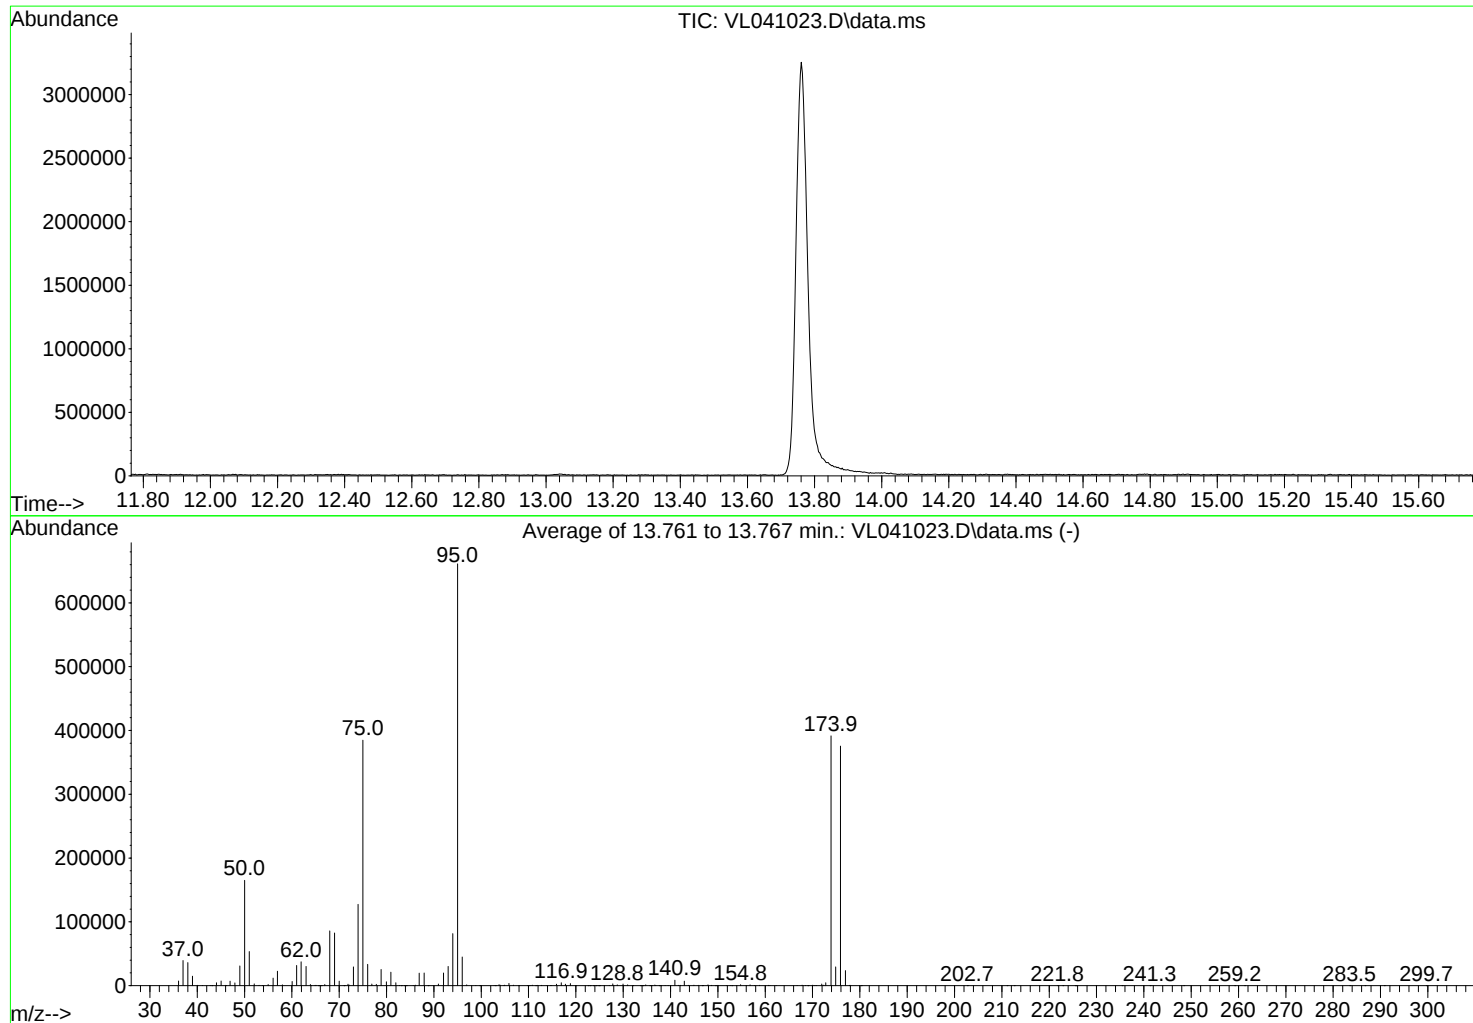

AutoFind: Scans 3470, 3471, 3472; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	165141	PASS
75	95	30	66	58.2	384704	PASS
95	95	100	100	100.0	661205	PASS
96	95	5	9	6.8	44829	PASS
173	174	0.00	2	1.1	4450	PASS
174	95	50	120	59.2	391637	PASS
175	174	4	9	7.5	29256	PASS
176	174	93	101	95.8	375360	PASS
177	176	5	9	6.3	23656	PASS

Average of 13.761 to 13.767 min.: VL041023.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7193	46.20	289	56.95	22677	65.90	101
37.00	39267	46.95	7060	58.00	1206	66.20	101
38.00	36040	47.95	4238	60.05	6487	66.95	168
39.00	14766	49.00	30770	61.00	31619	68.00	8581
40.10	467	50.00	165141	61.95	37312	69.00	82563
41.10	220	51.00	53437	63.00	30037	70.00	6952
42.75	333	52.05	2759	63.90	1811	71.00	103
43.10	55	53.05	474	64.10	388	71.20	248
44.05	4577	53.80	257	64.90	557	71.85	2280
45.05	7280	55.00	1801	65.10	581	72.10	1127
46.00	449	56.05	11852	65.60	126	73.00	29253

Average of 13.761 to 13.767 min.: VL041023.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	127344	83.80	51	95.00	661205	105.85	3469
75.00	384704	84.15	142	96.00	44829	106.80	862
76.00	33493	85.65	298	96.95	1177	107.90	60
76.90	2520	86.10	673	98.85	207	109.80	414
77.85	2052	86.90	19606	99.70	60	110.00	79
78.85	25248	87.95	19768	102.70	308	110.50	191
79.95	5934	88.80	114	103.00	102	110.80	735
80.90	21115	90.95	2521	103.75	1547	111.50	71
81.95	4582	92.05	19853	104.00	879	111.95	471
82.75	331	93.00	30131	104.80	324	112.75	611
83.10	98	94.00	81595	104.95	882	113.90	160

Average of 13.761 to 13.767 min.: VL041023.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.65	218	124.30	149	133.90	65	140.00	368
114.90	226	124.80	150	134.20	137	140.90	8500
115.90	2296	125.00	51	134.75	1359	141.70	548
116.90	4618	126.00	264	135.60	115	142.10	557
117.80	2251	127.05	273	135.90	107	142.90	7039
118.85	3370	127.80	2727	136.70	1068	143.80	511
119.90	80	128.75	1300	136.90	353	144.95	679
122.60	56	129.95	2607	137.60	57	145.85	586
123.00	87	130.95	1187	137.90	119	146.70	132
123.70	148	132.00	76	138.85	278	146.90	409
124.00	348	133.60	138	139.50	201	147.90	1380

Average of 13.761 to 13.767 min.: VL041023.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.65	583	158.80	632	170.80	390	202.70	137
149.50	101	160.70	424	171.95	2422	211.10	51
150.00	593	161.00	239	172.40	870	212.60	55
151.90	329	162.30	199	172.80	4450	221.80	59
152.60	224	166.75	302	173.90	391637	222.90	59
152.95	134	167.80	645	174.90	29256	225.50	55
153.95	214	168.50	296	175.90	375360	225.70	51
154.80	1457	169.00	116	176.95	23656	235.40	106
156.00	190	169.20	296	177.80	445	241.30	125
156.80	1354	170.05	824	178.05	421	248.40	68
157.75	403	170.50	178	180.30	55	259.20	87

Average of 13.761 to 13.767 min.: VL041023.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
261.30	57						
283.50	65						
286.70	50						
290.80	76						
299.70	107						