


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL012622\
 Data File : VL038283.D
 Acq On : 26 Jan 2022 10:11
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jan 24 14:12:48 2022
 Last Update : Mon Jan 24 14:12:48 2022

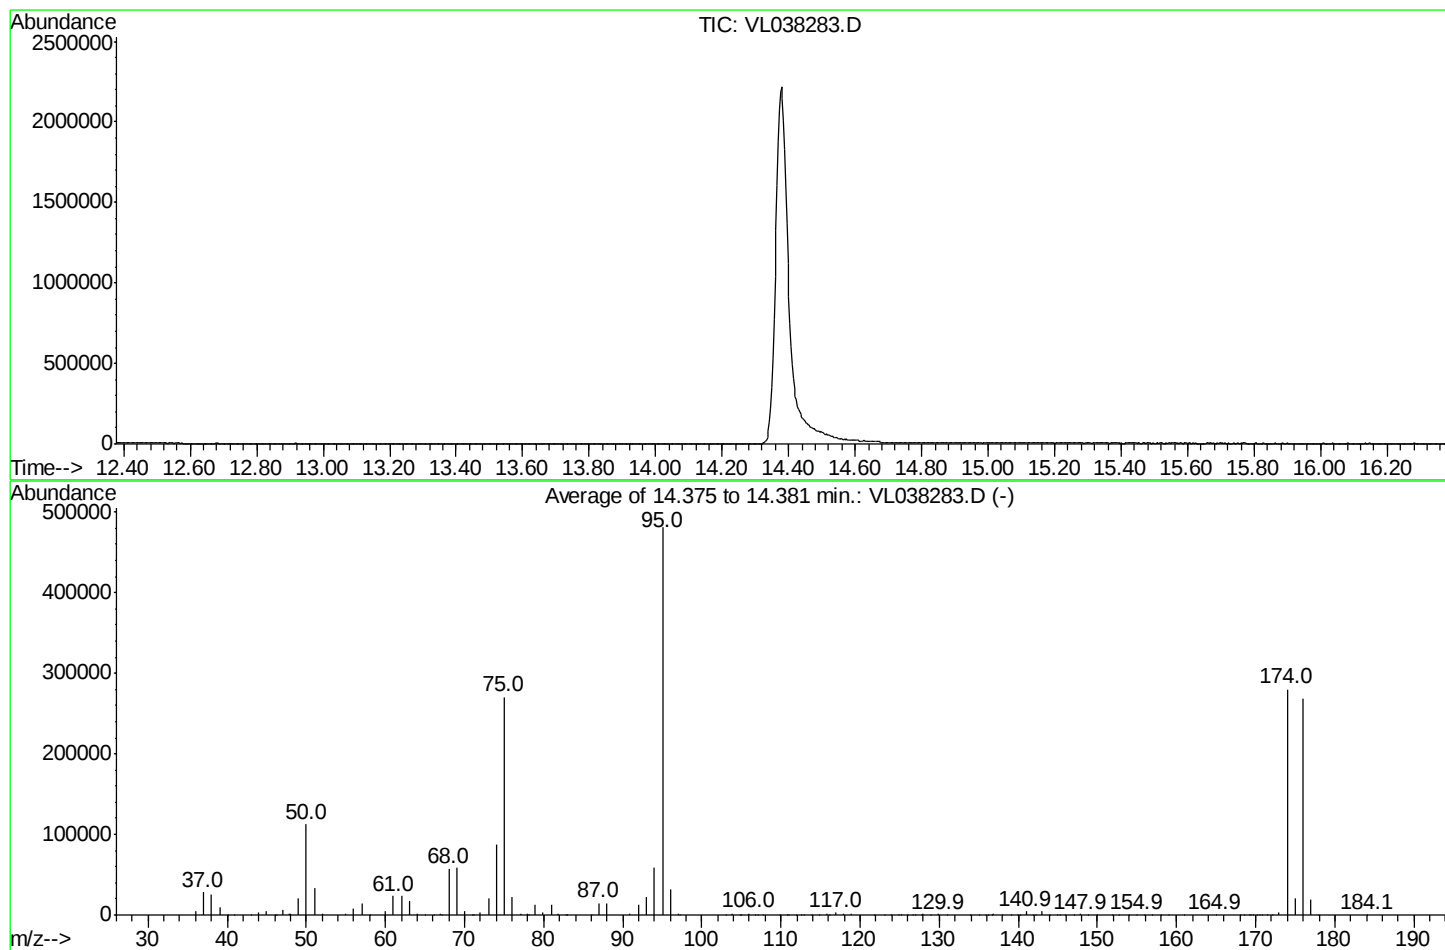

AutoFind: Scans 3604, 3605, 3606; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	112730	PASS
75	95	30	66	56.3	270762	PASS
95	95	100	100	100.0	480981	PASS
96	95	5	9	6.5	31456	PASS
173	174	0.00	2	1.3	3672	PASS
174	95	50	120	58.2	279850	PASS
175	174	4	9	7.5	21109	PASS
176	174	93	101	95.9	268437	PASS
177	176	5	9	6.9	18602	PASS