


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL012720\
 Data File : VL034556.D
 Acq On : 27 Jan 2020 9:53
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL123019AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 09 03:01:19 2020
 Last Update : Thu Jan 09 03:01:19 2020

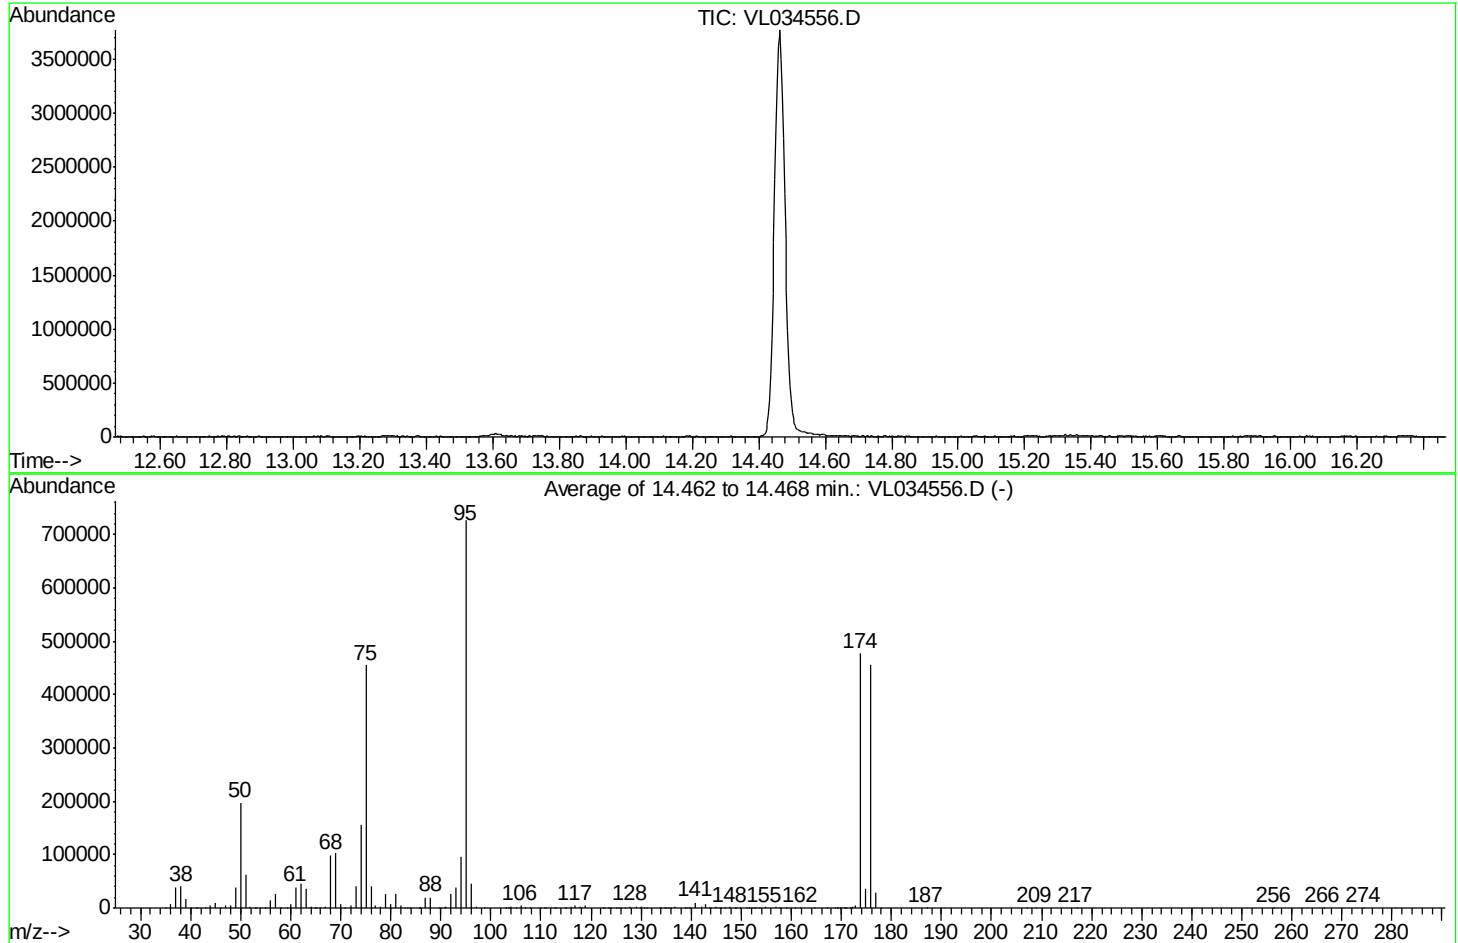

AutoFind: Scans 3631, 3632, 3633; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.2	198144	PASS
75	95	30	66	62.7	455957	PASS
95	95	100	100	100.0	727146	PASS
96	95	5	9	6.3	45719	PASS
173	174	0.00	2	0.8	3828	PASS
174	95	50	120	65.6	477333	PASS
175	174	4	9	7.7	36589	PASS
176	174	93	101	95.6	456490	PASS
177	176	5	9	6.5	29848	PASS