


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012722\
 Data File : VL038296.D
 Acq On : 27 Jan 2022 13:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jan 24 14:12:48 2022
 Last Update : Mon Jan 24 14:12:48 2022

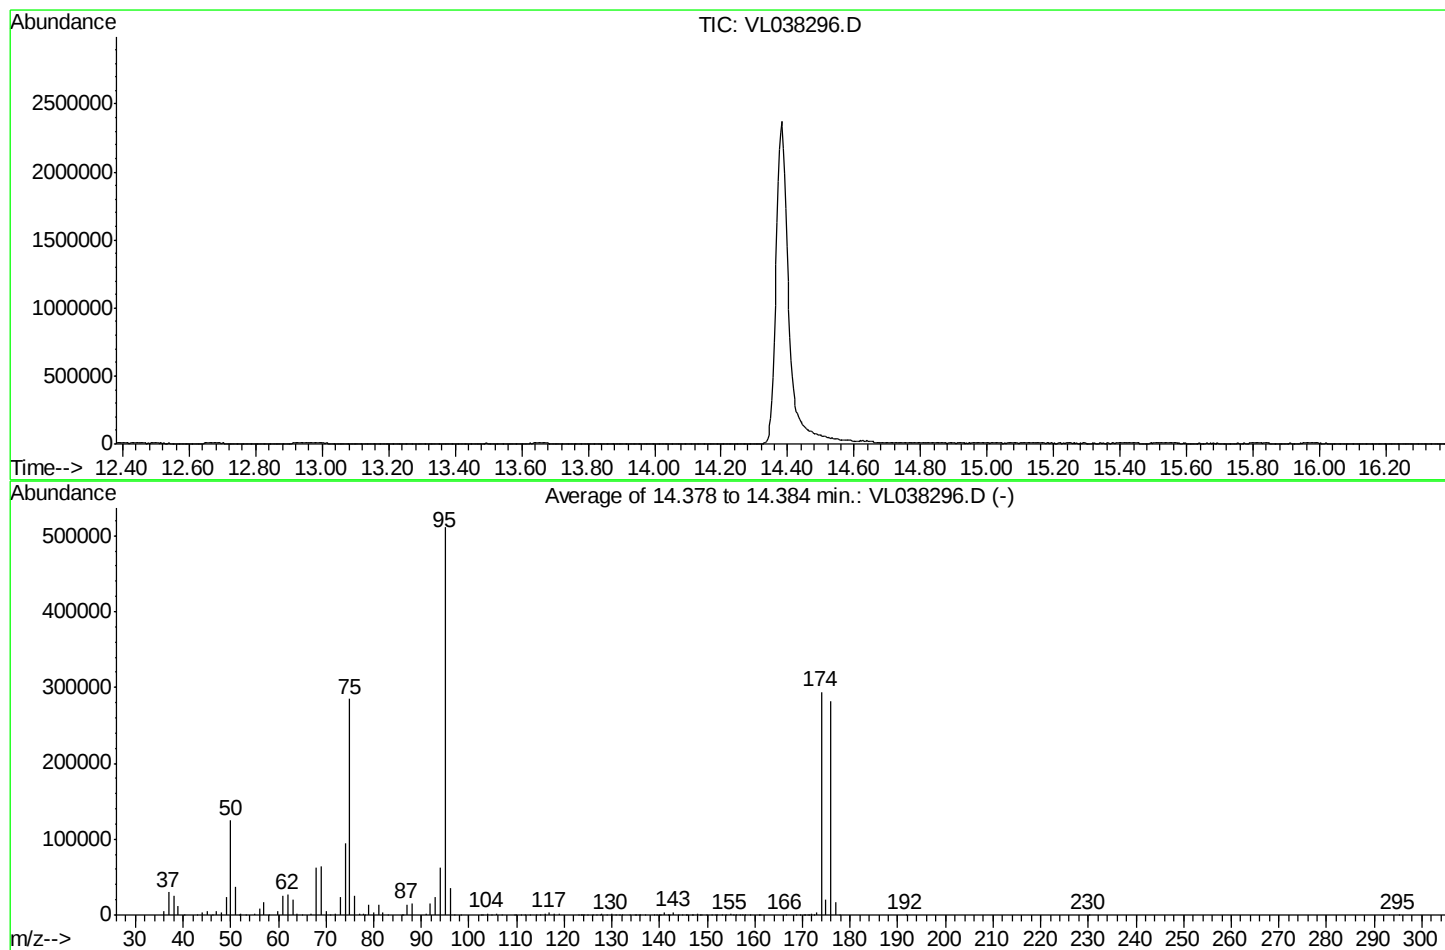

AutoFind: Scans 3605, 3606, 3607; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	124890	PASS
75	95	30	66	55.7	284928	PASS
95	95	100	100	100.0	511168	PASS
96	95	5	9	6.8	34682	PASS
173	174	0.00	2	1.2	3429	PASS
174	95	50	120	57.5	293930	PASS
175	174	4	9	7.2	21018	PASS
176	174	93	101	95.7	281429	PASS
177	176	5	9	6.1	17151	PASS