


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012819\
Data File : VL033113.D
Acq On : 28 Jan 2019 15:02
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012819AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jan 04 16:09:05 2019
Last Update : Fri Jan 04 16:09:05 2019

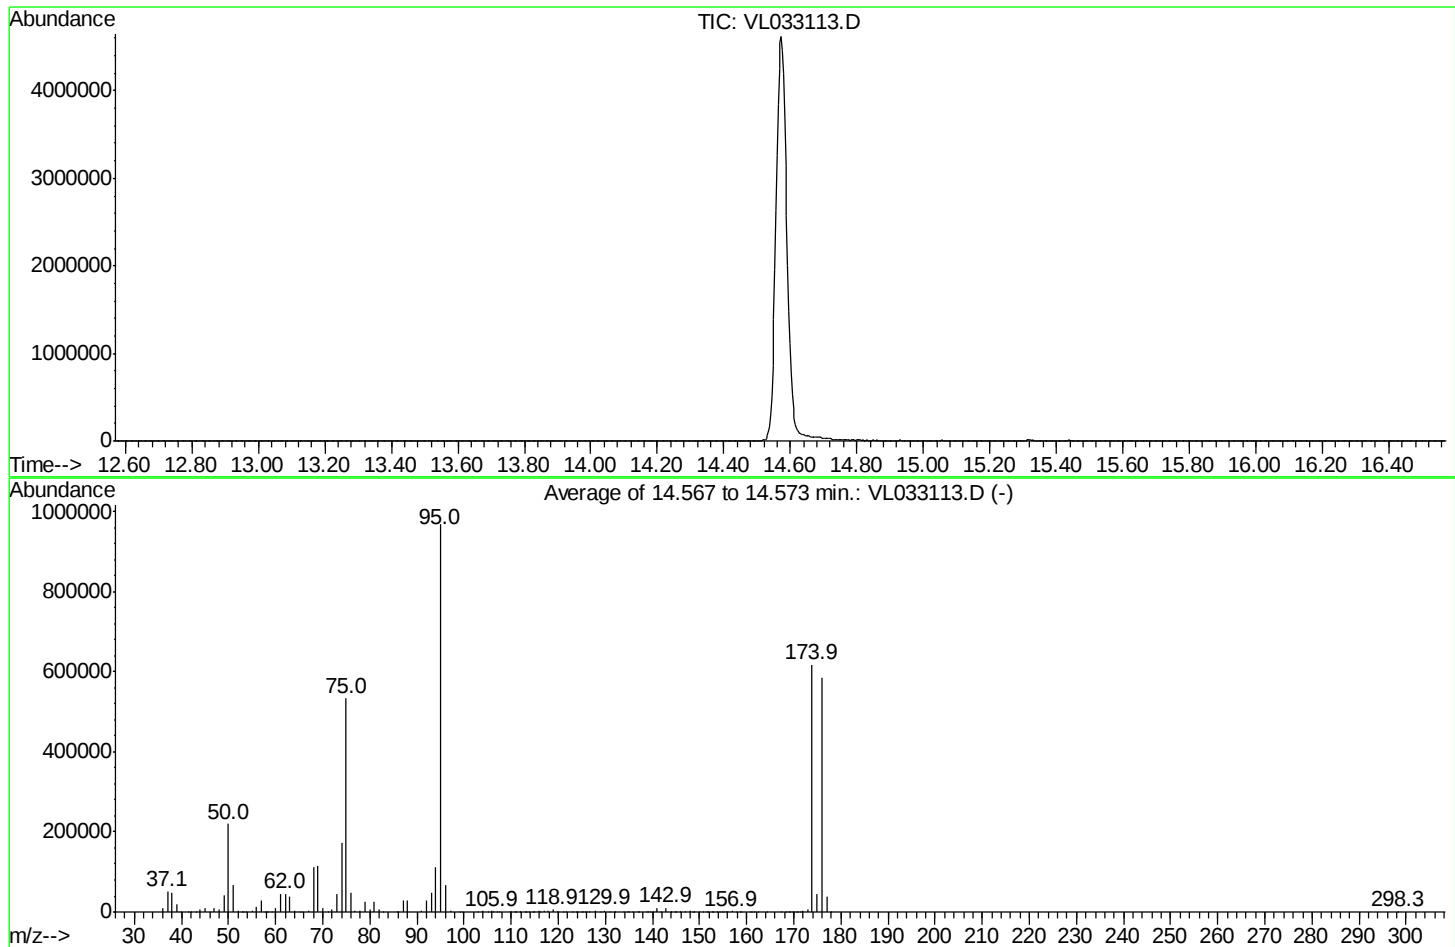

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	219264	PASS
75	95	30	66	55.1	533162	PASS
95	95	100	100	100.0	967786	PASS
96	95	5	9	7.0	67389	PASS
173	174	0.00	2	1.2	7157	PASS
174	95	50	120	63.8	617024	PASS
175	174	4	9	7.4	45512	PASS
176	174	93	101	95.0	586304	PASS
177	176	5	9	6.7	39514	PASS