


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL013020\
 Data File : VL034567.D
 Acq On : 30 Jan 2020 11:27
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL013020AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 30 11:35:42 2020
 Last Update : Thu Jan 30 11:35:42 2020

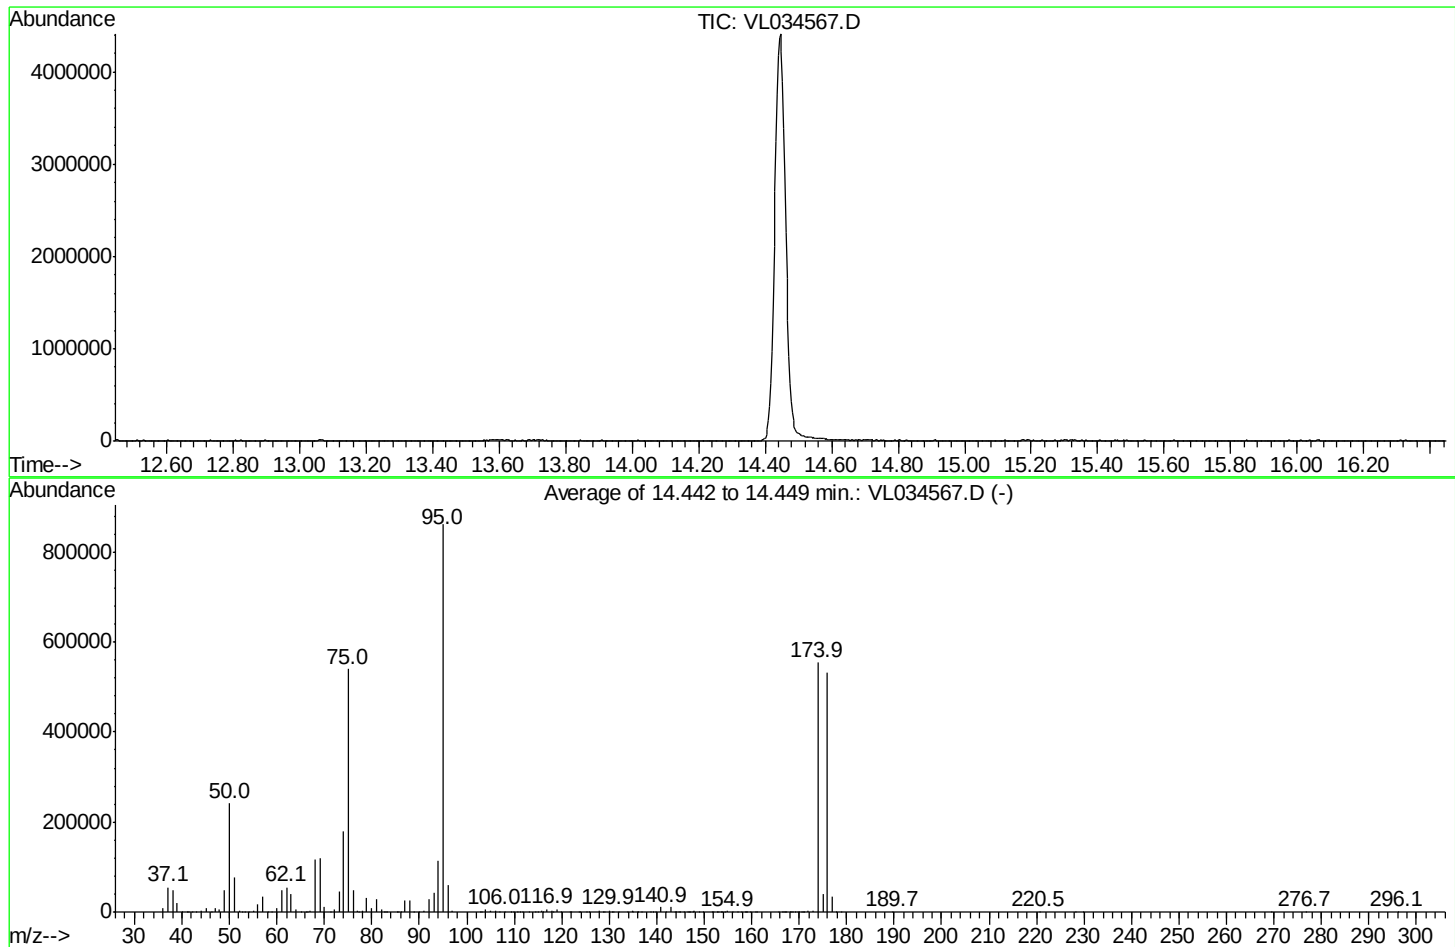

AutoFind: Scans 3625, 3626, 3627; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	28.1	241814	PASS
75	95	30	66	62.6	539541	PASS
95	95	100	100	100.0	861589	PASS
96	95	5	9	7.1	60957	PASS
173	174	0.00	2	0.7	4117	PASS
174	95	50	120	64.3	553728	PASS
175	174	4	9	7.4	41178	PASS
176	174	93	101	96.0	531456	PASS
177	176	5	9	6.4	34176	PASS