


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL013023\
 Data File : VL040127.D
 Acq On : 30 Jan 2023 10:26
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Jan 31 05:24:57 2023

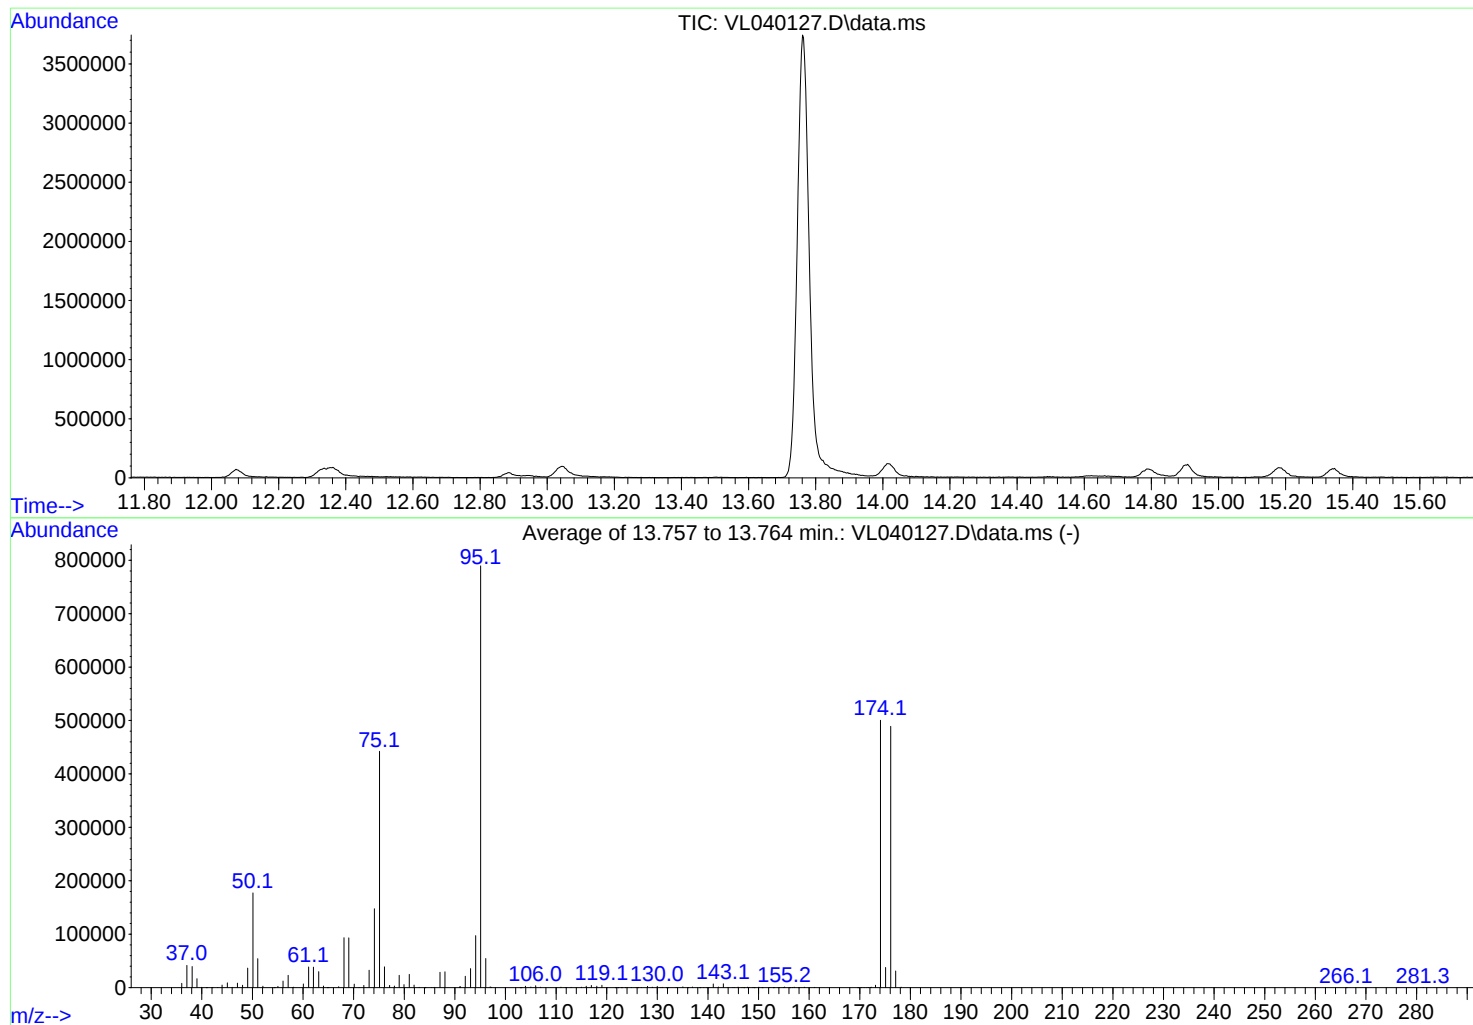

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.5	177429	PASS
75	95	30	66	56.0	442219	PASS
95	95	100	100	100.0	789504	PASS
96	95	5	9	6.9	54565	PASS
173	174	0.00	2	0.9	4525	PASS
174	95	50	120	63.4	500395	PASS
175	174	4	9	7.5	37685	PASS
176	174	93	101	97.7	488939	PASS
177	176	5	9	6.3	31011	PASS

Average of 13.757 to 13.764 min.: VL040127.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8233	47.05	8544	58.15	933	70.10	6511
37.05	41707	48.05	4425	60.05	7070	71.05	366
38.10	39539	49.05	36531	61.10	38608	72.00	422
39.05	16806	50.10	177429	62.05	38360	73.05	3264
40.00	644	51.05	54253	63.10	30040	74.10	147733
40.90	61	52.05	2788	64.05	3103	75.10	442219
42.00	58	54.30	51	64.80	137	76.10	38869
43.15	173	55.05	2305	65.10	390	77.10	4079
44.00	4896	56.05	12355	67.05	1879	78.05	3013
45.05	8935	57.05	23205	68.10	93509	79.00	23059
46.00	524	57.90	322	69.05	93265	79.95	5818

Average of 13.757 to 13.764 min.: VL040127.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.00	24800	93.10	35653	106.95	830	120.05	174
81.95	4727	94.10	97317	110.05	397	121.70	98
82.95	744	95.10	789504	110.95	801	121.95	228
84.10	54	96.10	54565	111.80	264	122.20	53
85.45	429	97.00	1520	112.05	239	122.90	53
85.90	692	97.20	483	112.95	550	123.70	243
87.05	28709	102.90	131	115.00	1047	124.05	229
88.05	29749	103.10	78	115.95	2610	124.85	164
90.90	1568	103.95	2845	116.95	4229	125.80	242
91.10	1786	105.00	1212	118.05	2639	126.10	69
92.05	21416	105.95	3456	119.05	4465	126.85	287

Average of 13.757 to 13.764 min.: VL040127.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.05	2496	136.95	1343	145.95	882	153.15	434
129.00	1049	138.40	55	146.75	233	153.85	435
130.00	2419	139.20	420	147.10	128	154.10	225
130.70	365	139.80	337	147.85	887	154.90	476
131.05	599	140.00	129	148.10	640	155.15	1315
131.80	111	141.05	6931	148.90	601	156.10	89
132.10	114	142.05	1116	149.10	117	156.70	235
133.70	254	143.05	7161	150.05	802	157.05	1014
133.95	186	143.95	545	150.70	132	157.90	61
135.05	1435	144.95	390	152.20	433	159.05	904
136.00	87	145.20	253	152.90	110	161.05	762

Average of 13.757 to 13.764 min.: VL040127.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.60	98	177.10	31011				
170.35	190	178.15	1082				
170.85	362	266.10	63				
171.40	167	281.30	201				
171.70	294						
172.10	462						
172.25	780						
173.10	4525						
174.10	500395						
175.10	37685						
176.10	488939						