

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041962.D
 Acq On : 03 Feb 2025 13:57
 Operator : SY/MD
 Sample : Q1222-01 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/04/2025
 Supervised By :Mahesh Dadoda 02/04/2025

Quant Time: Feb 04 02:35:35 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 23:15:42 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Bromochloromethane	2.793	49	159297	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.968	114	441984	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	404852	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.383	95	312689	9.806	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.100%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.499	85	2951	0.136	ppbv #	79
4) Chloromethane	1.534	50	1179	0.144	ppbv	96
9) Propene	1.486	41	30351	3.241	ppbv	89
10) Heptane	4.985	43	12032m	0.481	ppbv	
13) Ethanol	1.725	45	107420	156.617	ppbv	87
15) Acetone	1.839	43	39507	2.065	ppbv	99
19) Isopropyl Alcohol	1.890	45	108933	9.602	ppbv #	34
20) Methylene Chloride	2.065	84	11774	1.557	ppbv #	78
26) Hexane	2.832	57	67384	3.302	ppbv #	39
27) Carbon Disulfide	2.153	76	21096	1.045	ppbv #	1
29) Chloroform	2.855	83	3627	0.112	ppbv #	83
30) Cyclohexane	3.861	84	2131m	0.120	ppbv	
34) 2-Butanone	2.570	43	8793	0.313	ppbv	94
36) Benzene	3.667	78	8790	0.217	ppbv #	95
38) Trichloroethene	4.561	130	542m	0.034	ppbv	
41) Tetrahydrofuran	3.078	42	2353m	0.154	ppbv	
52) Tetrachloroethene	8.234	164	32706	2.327	ppbv	93
53) Toluene	6.949	91	14795	0.335	ppbv	94
58) Ethyl Benzene	9.364	91	10216	0.161	ppbv	89
59) m/p-Xylene	9.532	91	18053m	0.356	ppbv	
60) o-Xylene	9.969	91	11076m	0.220	ppbv	
62) Isopropylbenzene	10.545	105	14191	0.182	ppbv #	87
67) sec-Butylbenzene	11.775	105	10079m	0.103	ppbv	
73) 1,3,5-Trimethylbenzene	11.209	105	9214	0.173	ppbv #	85
74) 1,2,4-Trimethylbenzene	11.542	105	14454	0.251	ppbv #	49
78) Hexachloro-1,3-Butadiene	13.646	225	21171m	0.763	ppbv	
79) Naphthalene	13.118	128	98033m	1.691	ppbv	
80) Naphthalene,2-methyl-	14.309	142	37363m	1.359	ppbv	
81) 1,2,4-Trichlorobenzene	13.047	180	51438m	1.818	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
Data File : VL041962.D
Acq On : 03 Feb 2025 13:57
Operator : SY/MD
Sample : Q1222-01 4X
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SV1

Quant Time: Feb 04 02:35:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jan 14 23:15:42 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 02/04/2025
Supervised By : Mahesh Dadoda 02/04/2025

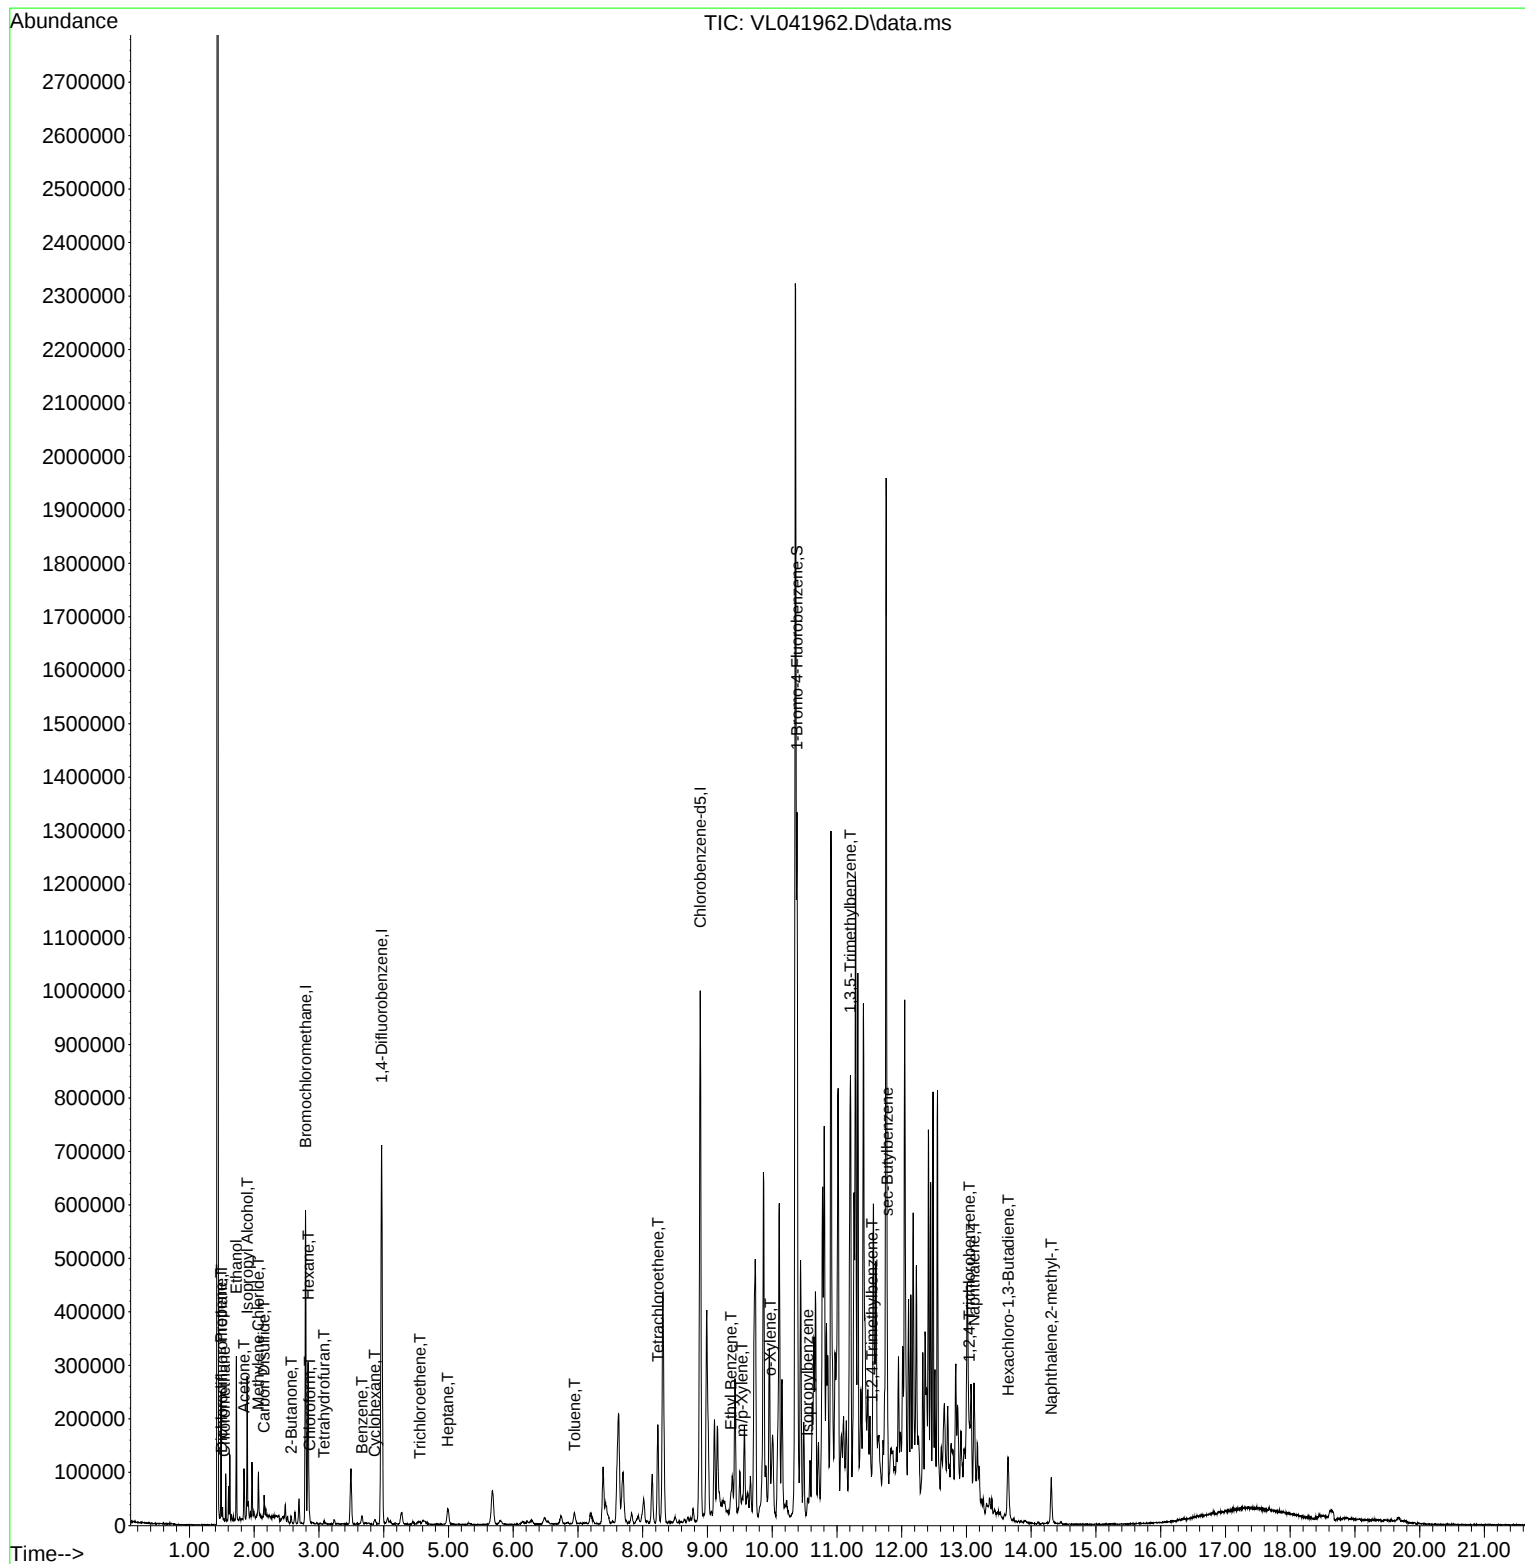







#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.793 min Scan# 81
Delta R.T. -0.004 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 49 Resp: 15929
Ion Ratio Lower Upper
49 100
128 47.7 24.3 73.0
130 61.4 31.1 93.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

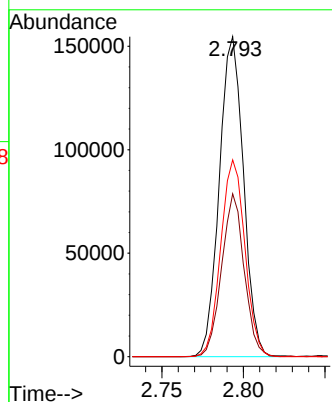

#2
Dichlorodifluoromethane
Concen: 0.136 ppbv
RT: 1.499 min Scan# 436
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion: 85 Resp: 2951
Ion Ratio Lower Upper
85 100
87 42.8 24.9 37.3#

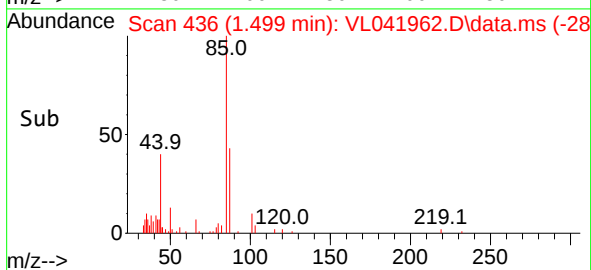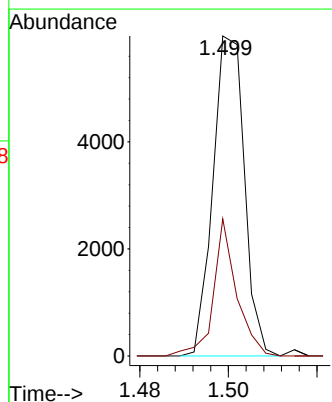



#4
Chloromethane
Concen: 0.144 ppbv
RT: 1.534 min Scan# 447
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 50 Resp: 1179
Ion Ratio Lower Upper
50 100
52 32.7 24.6 36.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

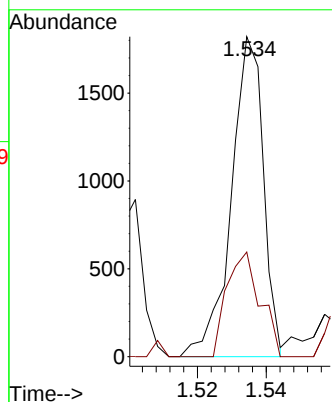

#9
Propene
Concen: 3.241 ppbv
RT: 1.486 min Scan# 432
Delta R.T. 0.000 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion: 41 Resp: 30351
Ion Ratio Lower Upper
41 100
42 56.3 52.0 78.0

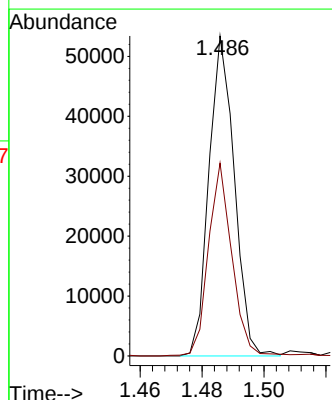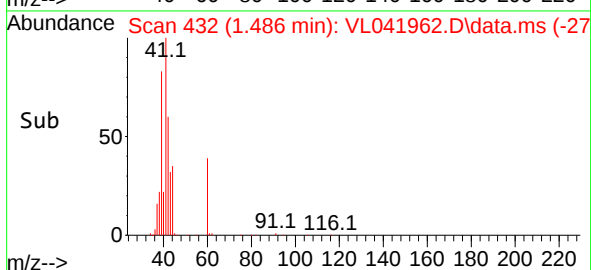



#10
Heptane
Concen: 0.481 ppbv m
RT: 4.985 min Scan# 11
Delta R.T. -0.016 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 43 Resp: 1203
Ion Ratio Lower Upper
43 100
57 49.8 41.0 61.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

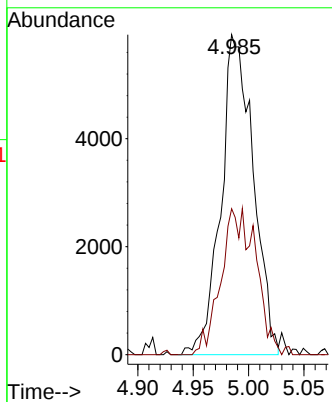

#13
Ethanol
Concen: 156.617 ppbv
RT: 1.725 min Scan# 506
Delta R.T. -0.000 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion: 45 Resp: 107420
Ion Ratio Lower Upper
45 100
46 36.8 18.1 72.5

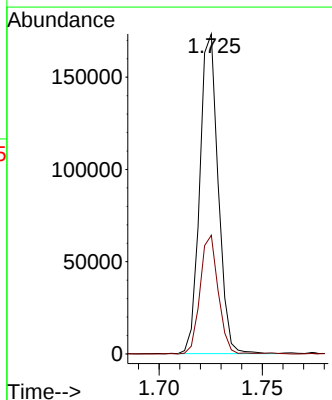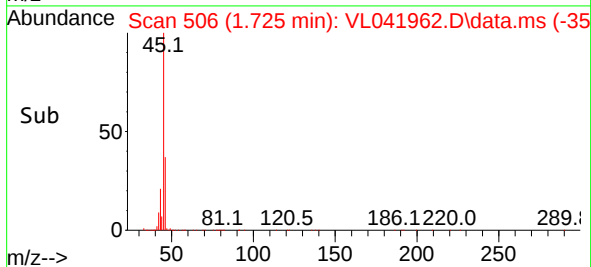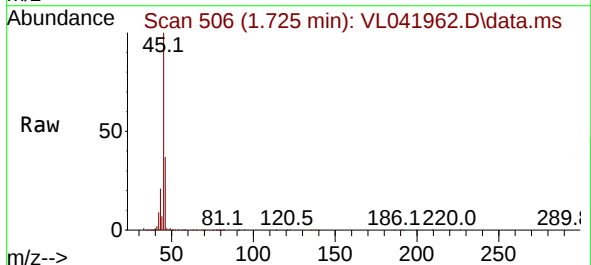



#15
Acetone
Concen: 2.065 ppbv
RT: 1.839 min Scan# 541
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion: 43 Resp: 39507
Ion Ratio Lower Upper
43 100
58 26.8 21.9 32.9

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

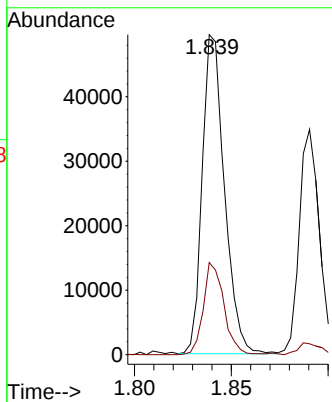


#19
Isopropyl Alcohol
Concen: 9.602 ppbv
RT: 1.890 min Scan# 557
Delta R.T. -0.000 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

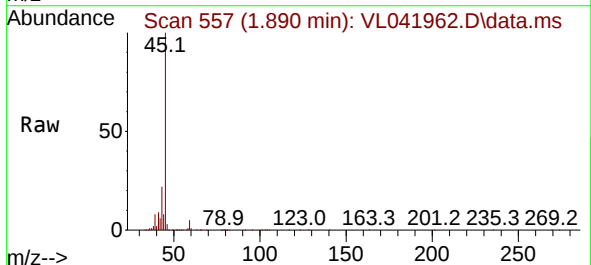


Tgt Ion: 45 Resp: 108933
Ion Ratio Lower Upper
45 100
58 1.4 35.0 52.6#

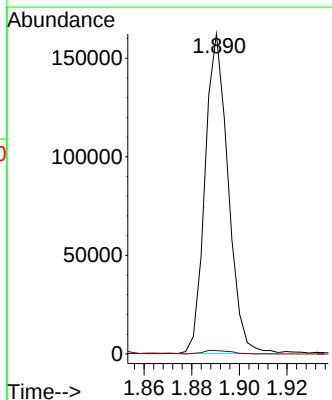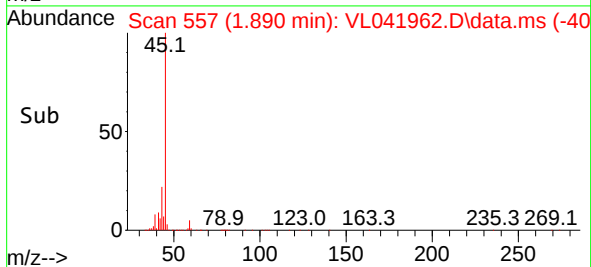



#20
Methylene Chloride
Concen: 1.557 ppbv
RT: 2.065 min Scan# 611
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1

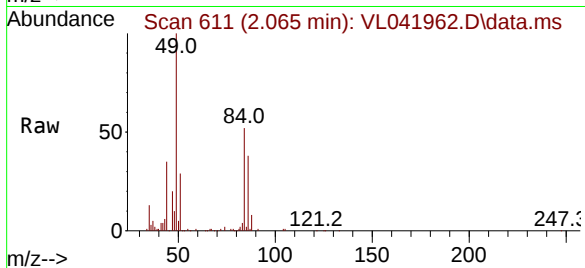


Tgt Ion: 84 Resp: 11774
Ion Ratio Lower Upper
84 100
49 192.8 123.1 184.7
51 53.4 35.8 53.8
86 73.5 53.7 80.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025




#26
Hexane
Concen: 3.302 ppbv
RT: 2.832 min Scan# 848
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

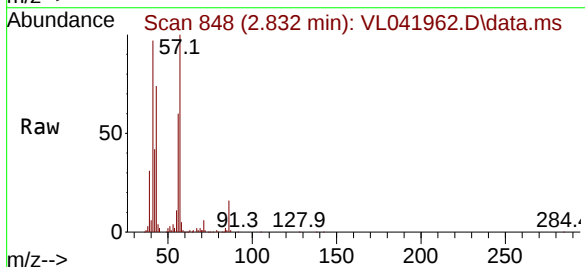


Tgt Ion: 57 Resp: 67384
Ion Ratio Lower Upper
57 100
41 98.1 73.8 110.8
43 85.3 197.3 295.9#
56 58.3 42.7 64.1

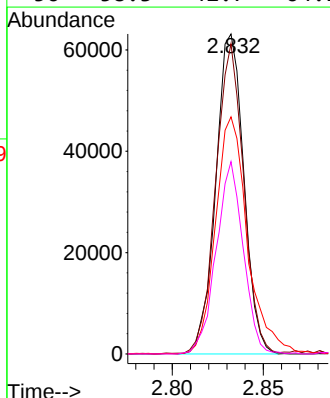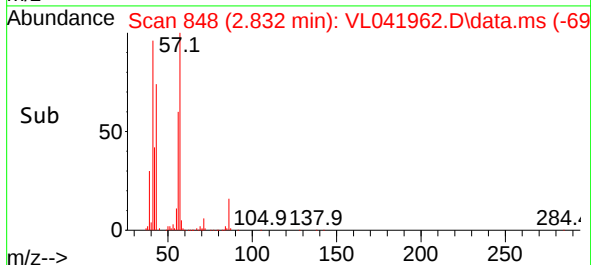



#27
Carbon Disulfide
Concen: 1.045 ppbv
RT: 2.153 min Scan# 61
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 76 Resp: 21090
Ion Ratio Lower Upper
76 100
44 109.1 15.4 23.0
78 11.0 9.3 13.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

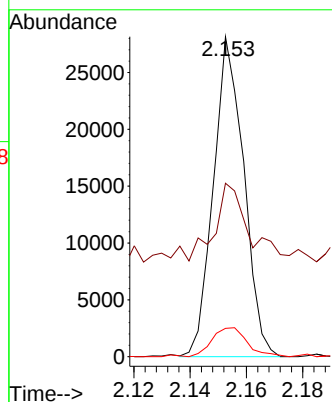

#29
Chloroform
Concen: 0.112 ppbv
RT: 2.855 min Scan# 855
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion: 83 Resp: 3627
Ion Ratio Lower Upper
83 100
85 49.5 50.1 75.1#

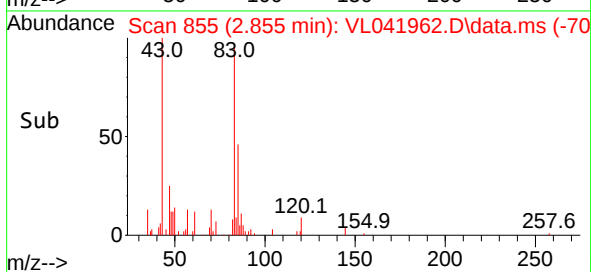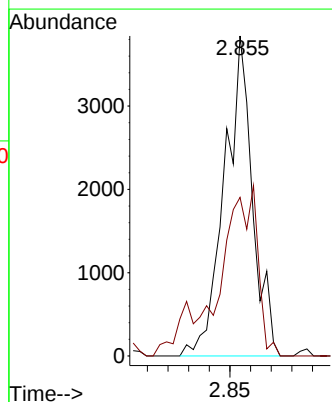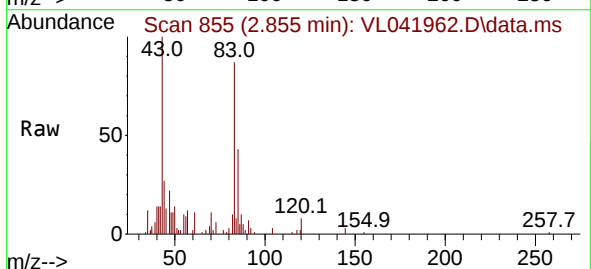



#30
Cyclohexane
Concen: 0.120 ppbv m
RT: 3.861 min Scan# 1166
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 84 Resp: 213
Ion Ratio Lower Upper
84 100
56 118.2 99.3 148.9
41 114.1 64.3 96.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

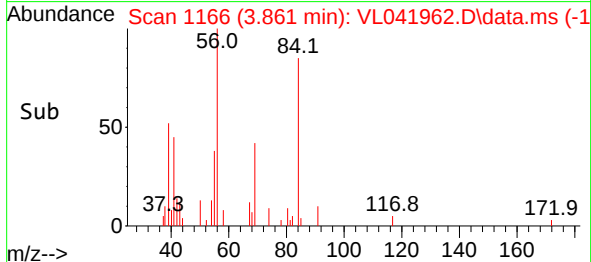

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.968 min Scan# 1199
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion:114 Resp: 441984
Ion Ratio Lower Upper
114 100
63 24.1 19.8 29.6
88 17.7 14.4 21.6

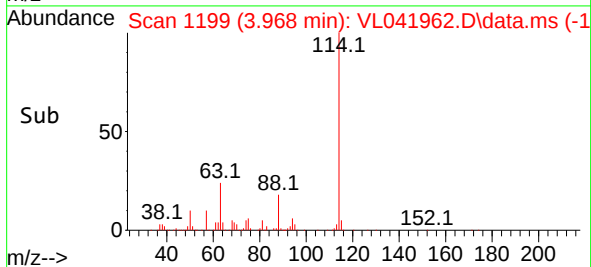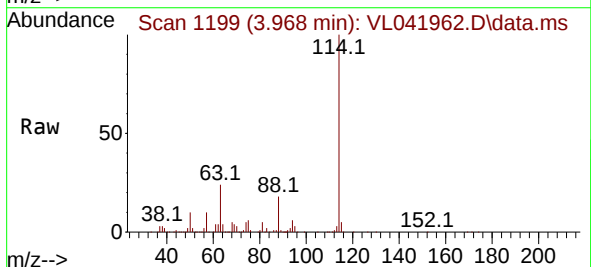



#34
2-Butanone
Concen: 0.313 ppbv
RT: 2.570 min Scan# 70
Delta R.T. 0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion: 43 Resp: 8790
Ion Ratio Lower Upper
43 100
72 26.4 18.6 28.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025



#36
Benzene
Concen: 0.217 ppbv
RT: 3.667 min Scan# 1106
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion: 78 Resp: 8790
Ion Ratio Lower Upper
78 100
77 23.0 18.1 27.1
50 14.9 15.2 22.8#

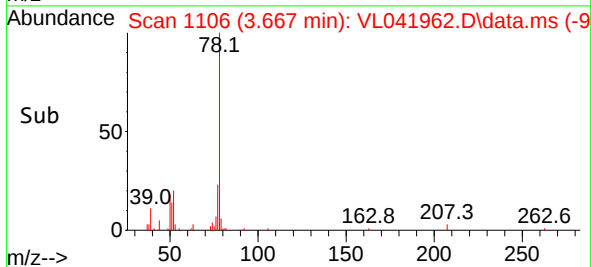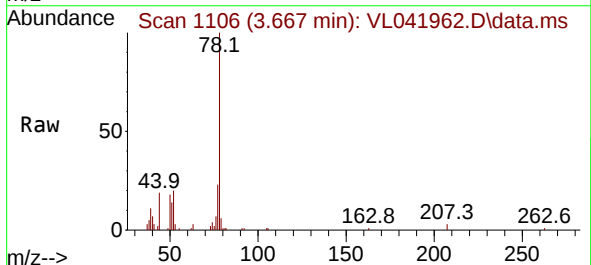



#38
 Trichloroethene
 Concen: 0.034 ppbv m
 RT: 4.561 min Scan# 1382
 Delta R.T. -0.003 min
 Lab File: VL041962.D
 Acq: 03 Feb 2025 13:57




Instrument : MSVOA_L
 ClientSampleId : SV1



Tgt Ion:130 Resp: 542
 Ion Ratio Lower Upper
 130 100
 95 148.9 85.8 128.8#
 132 130.6 76.5 114.7#
 97 58.2 56.8 85.2




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
 Supervised By :Mahesh Dadoda 02/04/2025



#41
 Tetrahydrofuran
 Concen: 0.154 ppbv m
 RT: 3.078 min Scan# 924
 Delta R.T. 0.013 min
 Lab File: VL041962.D
 Acq: 03 Feb 2025 13:57


Tgt Ion: 42 Resp: 2353
 Ion Ratio Lower Upper
 42 100
 72 28.0 32.3 48.5#
 71 0.0 29.9 44.9#

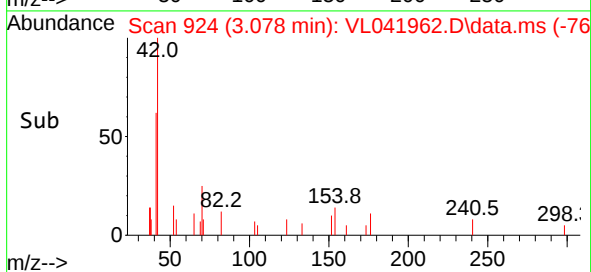



#52
Tetrachloroethene
Concen: 2.327 ppbv
RT: 8.234 min Scan# 2120
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1



Tgt Ion:164 Resp: 32700
Ion Ratio Lower Upper
164 100
166 118.1 100.8 151.2
129 91.5 82.0 123.0
131 96.4 80.2 120.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

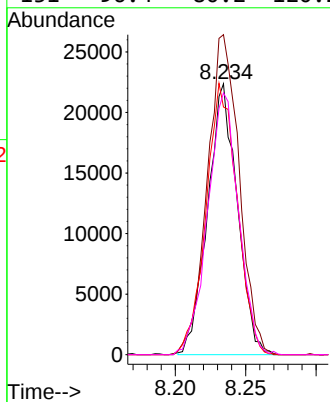

#53
Toluene
Concen: 0.335 ppbv
RT: 6.949 min Scan# 2120
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Tgt Ion: 91 Resp: 14795
Ion Ratio Lower Upper
91 100
92 63.6 47.4 71.0

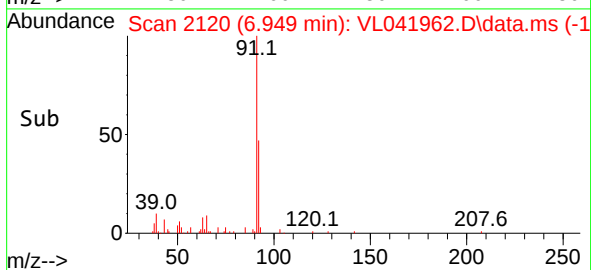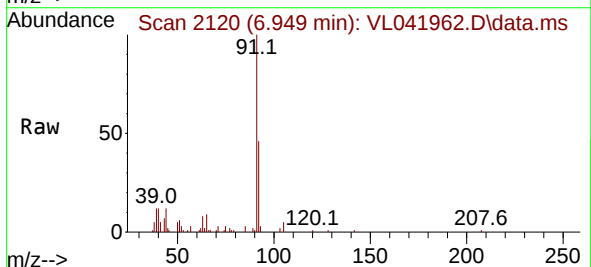







#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.888 min Scan# 2719
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion:117 Resp: 404852
Ion Ratio Lower Upper
117 100
82 63.9 54.2 81.4
119 32.3 25.0 37.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

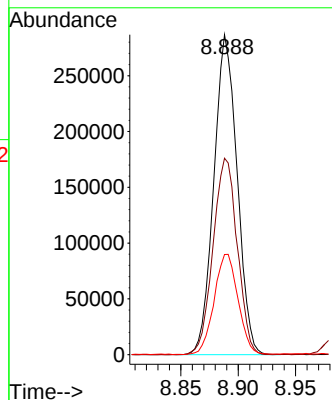

#58
Ethyl Benzene
Concen: 0.161 ppbv
RT: 9.364 min Scan# 2866
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Tgt Ion: 91 Resp: 10216
Ion Ratio Lower Upper
91 100
106 23.2 23.1 34.7

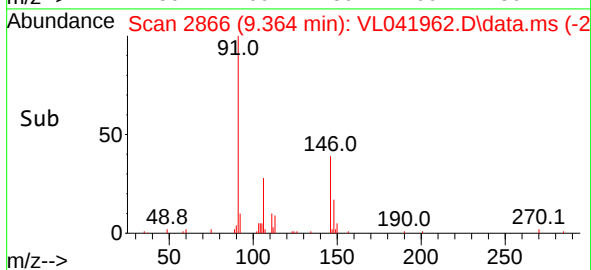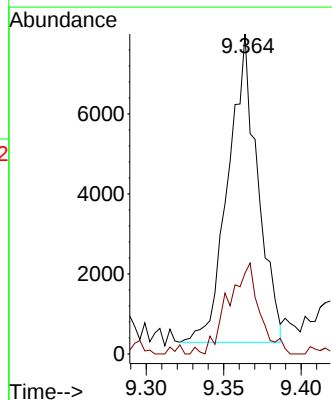







#59
m/p-Xylene
Concen: 0.356 ppbv m
RT: 9.532 min Scan# 2918
Delta R.T. -0.032 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 91 Resp: 1805
Ion Ratio Lower Upper
91 100
106 0.0 36.0 54.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

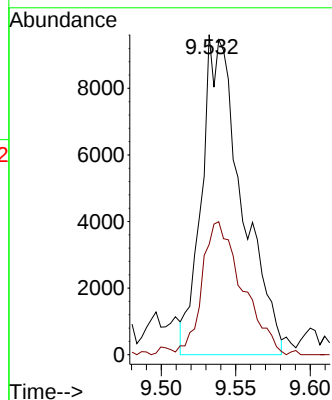

#60
o-Xylene
Concen: 0.220 ppbv m
RT: 9.969 min Scan# 3053
Delta R.T. -0.010 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57


Tgt Ion: 91 Resp: 11076
Ion Ratio Lower Upper
91 100
106 2.3 21.3 63.9

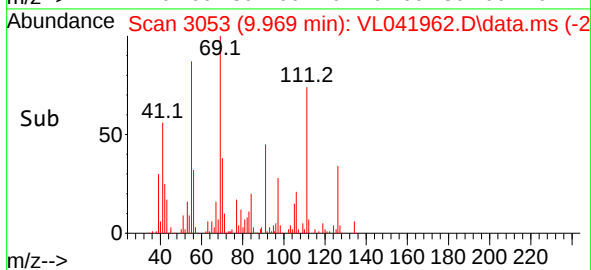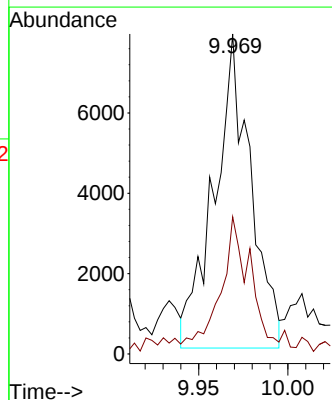

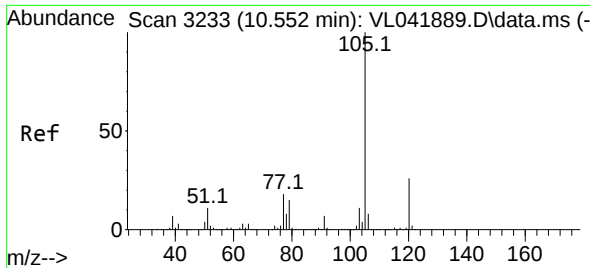

#62
Isopropylbenzene
Concen: 0.182 ppbv
RT: 10.545 min Scan# 31
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1

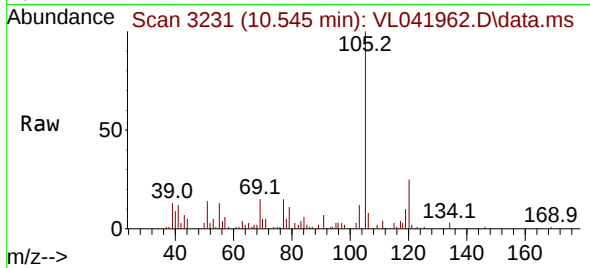

Tgt Ion:105 Resp: 1419
Ion Ratio Lower Upper
105 100
120 32.2 20.3 30.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

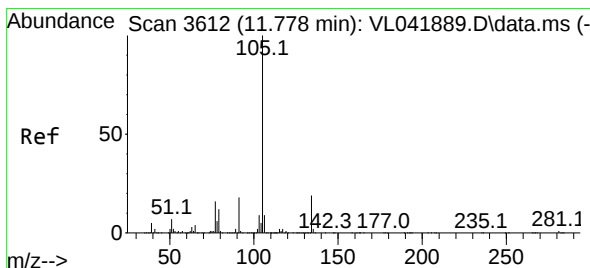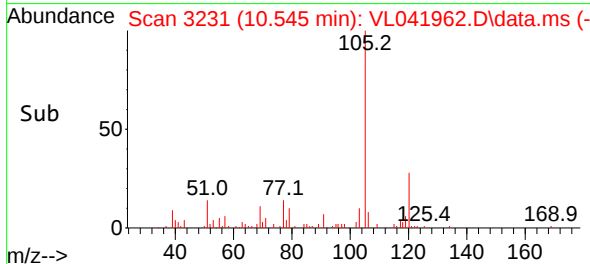

#67
sec-Butylbenzene
Concen: 0.103 ppbv m
RT: 11.775 min Scan# 3611
Delta R.T. -0.003 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Tgt Ion:105 Resp: 10079
Ion Ratio Lower Upper
105 100
134 1.7 15.1 22.7#

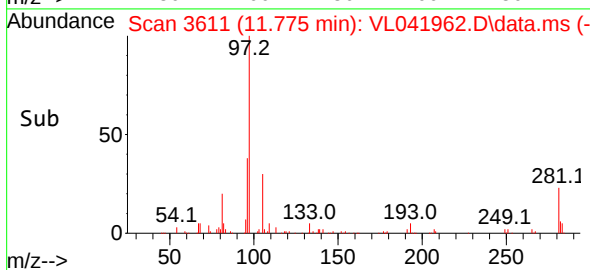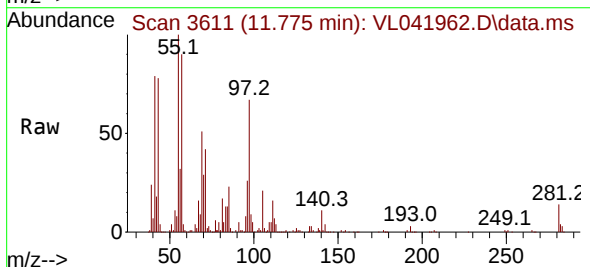

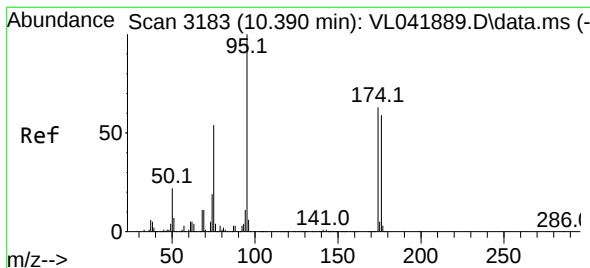





#68
1-Bromo-4-Fluorobenzene
Concen: 9.806 ppbv
RT: 10.383 min Scan# 3183
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion: 95 Resp: 312689
Ion Ratio Lower Upper
95 100
174 60.5 49.0 73.4
175 4.9 3.8 5.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

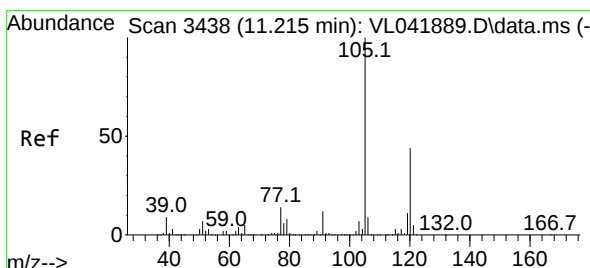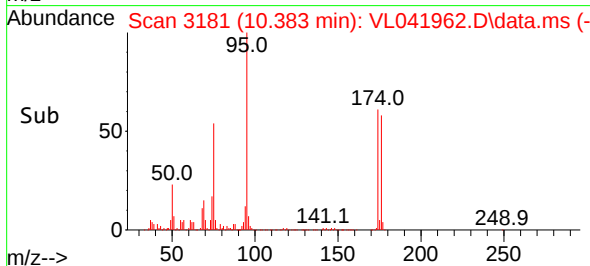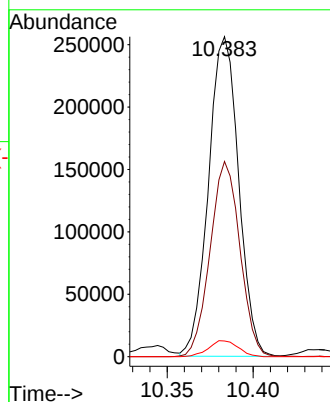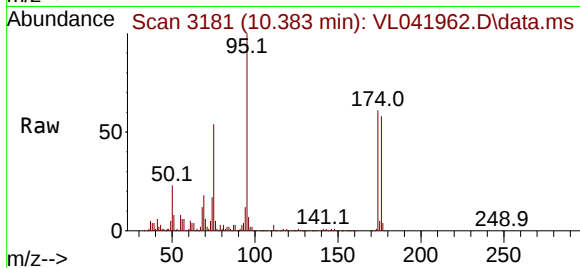

#73
1,3,5-Trimethylbenzene
Concen: 0.173 ppbv
RT: 11.209 min Scan# 3436
Delta R.T. -0.006 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Tgt Ion:105 Resp: 9214
Ion Ratio Lower Upper
105 100
120 34.3 35.4 53.2#

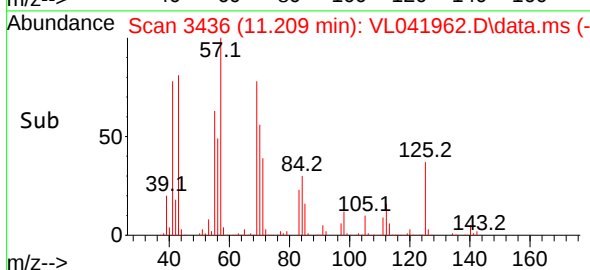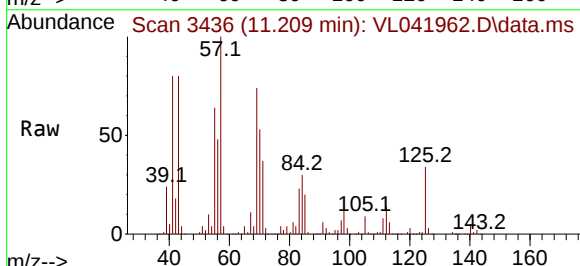

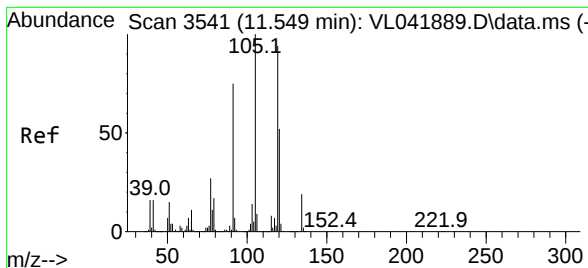

#74

1,2,4-Trimethylbenzene

Concen: 0.251 ppbv

RT: 11.542 min Scan# 31

Delta R.T. -0.006 min

Lab File: VL041962.D

Acq: 03 Feb 2025 13:57

Instrument :

MSVOA_L

ClientSampleId :

SV1

Tgt Ion:105 Resp: 14454





Ion	Ratio	Lower	Upper
105	100		
120	37.7	41.4	62.2
91	6.4	60.2	90.2
77	12.3	22.0	33.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/04/2025

Supervised By :Mahesh Dadoda 02/04/2025

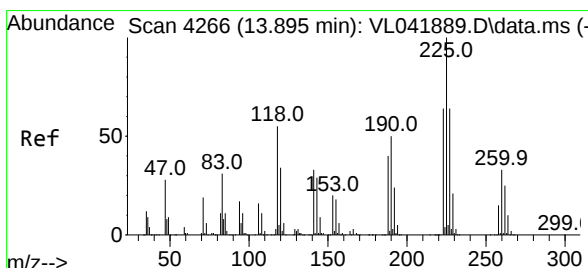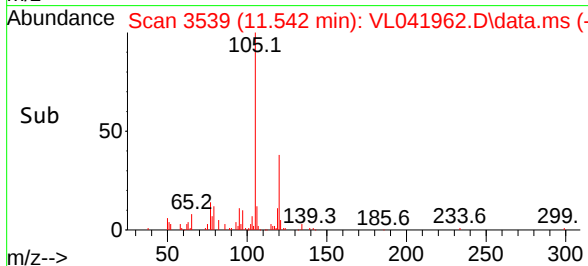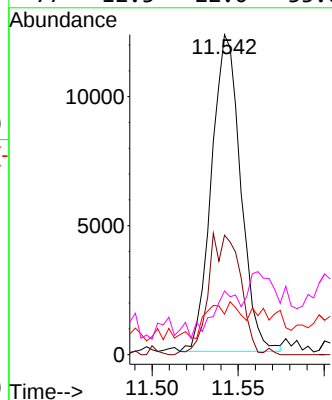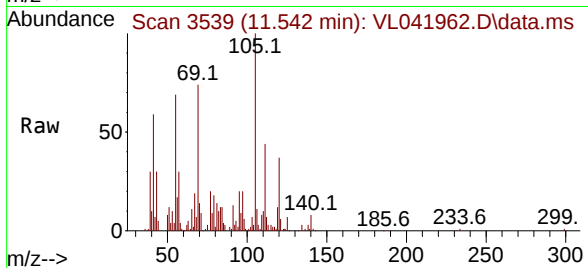

#78

Hexachloro-1,3-Butadiene

Concen: 0.763 ppbv m

RT: 13.646 min Scan# 4189




Delta R.T. -0.249 min


Lab File: VL041962.D

Acq: 03 Feb 2025 13:57

Tgt Ion:225 Resp: 21171


Ion	Ratio	Lower	Upper
225	100		
223	0.0	50.8	76.2
227	0.0	50.3	75.5

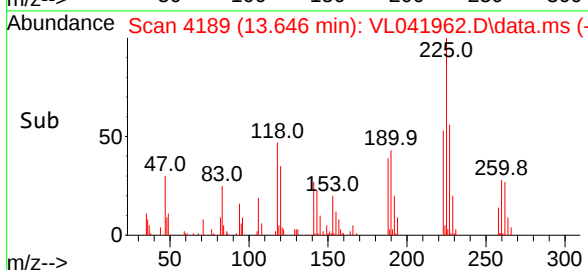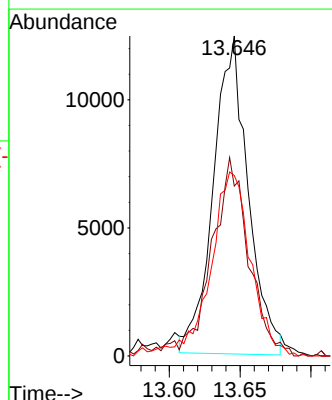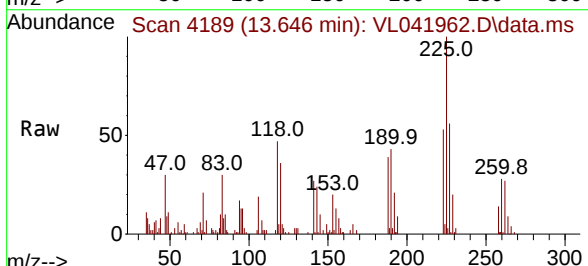



#79
Naphthalene
Concen: 1.691 ppbv m
RT: 13.118 min Scan# 4026
Delta R.T. -0.408 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57




Instrument :
MSVOA_L
ClientSampleId :
SV1




Tgt Ion:128 Resp: 9803
Ion Ratio Lower Upper
128 100
127 15.3 10.2 15.4
129 10.1 9.1 13.7

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

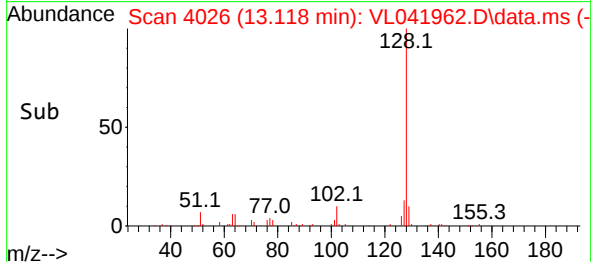


#80
Naphthalene,2-methyl-
Concen: 1.359 ppbv m
RT: 14.309 min Scan# 4394
Delta R.T. -0.162 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

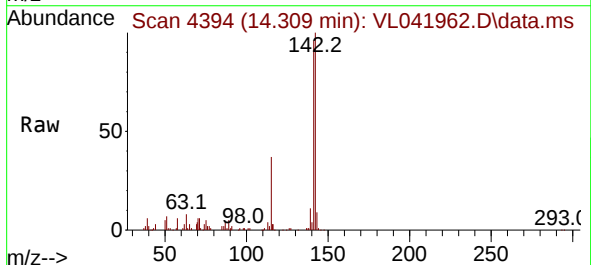

Tgt Ion:142 Resp: 37363
Ion Ratio Lower Upper
142 100
141 0.0 68.1 102.1#
115 0.0 31.7 47.5#

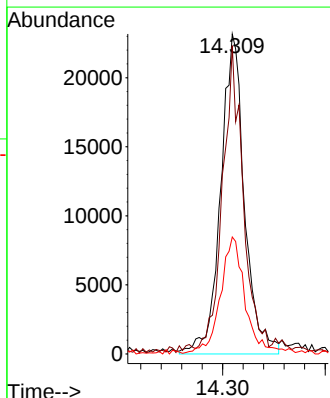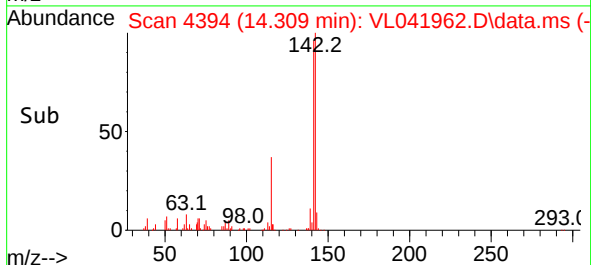

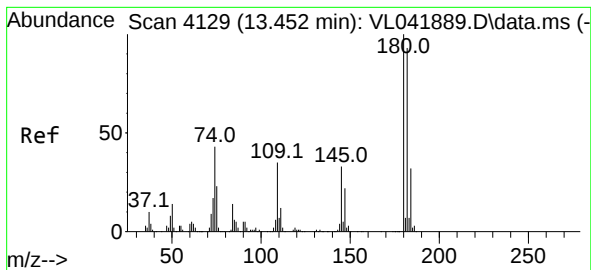

#81
1,2,4-Trichlorobenzene
Concen: 1.818 ppbv m
RT: 13.047 min Scan# 4004
Delta R.T. -0.405 min
Lab File: VL041962.D
Acq: 03 Feb 2025 13:57

Instrument :
MSVOA_L
ClientSampleId :
SV1

Tgt Ion:180 Resp: 51438
Ion Ratio Lower Upper
180 100
182 0.0 77.0 115.6
184 0.0 24.9 37.3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 02/04/2025
Supervised By :Mahesh Dadoda 02/04/2025

