


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL020420\
 Data File : VL034576.D
 Acq On : 4 Feb 2020 11:03
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL013020AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 30 17:16:44 2020
 Last Update : Thu Jan 30 17:16:44 2020

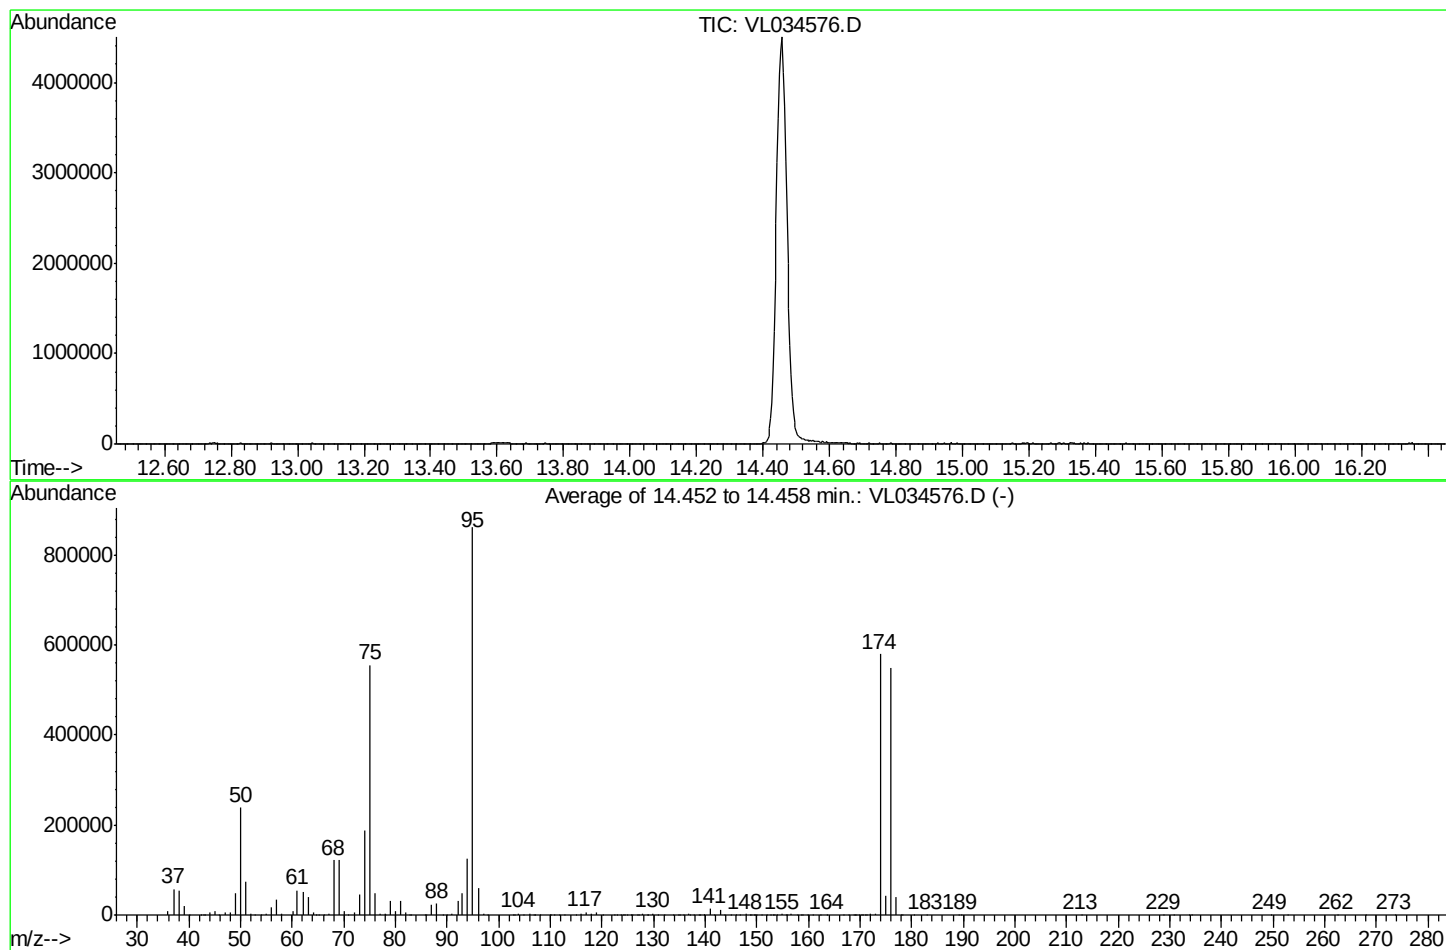

AutoFind: Scans 3628, 3629, 3630; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.6	237930	PASS
75	95	30	66	64.4	554666	PASS
95	95	100	100	100.0	861418	PASS
96	95	5	9	7.0	60629	PASS
173	174	0.00	2	0.6	3444	PASS
174	95	50	120	67.3	579584	PASS
175	174	4	9	7.3	42456	PASS
176	174	93	101	94.7	548693	PASS
177	176	5	9	7.1	38757	PASS