

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL020519\
 Data File : VL033182.D
 Acq On : 6 Feb 2019 17:54
 Operator : SY/AP
 Sample : K1289-01DL 2X
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 1000DL

Quant Time: Feb 20 06:51:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL020519AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Feb 20 06:00:52 2019
 QLast Update : Wed Feb 20 06:00:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	960160	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.29	114	2376399	10.00	ppbv	-0.01
55) Chlorobenzene-d5	12.24	117	2489478	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.58	95	2245173	11.57	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	115.70%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Vinyl Chloride	3.29	62	513146	8.050	ppbv	99
9) Propene	3.04	41	388778	6.961	ppbv	100
18) 1,1-Dichloroethene	4.35	96	372805	8.086	ppbv	95
24) 1,1-Dichloroethane	5.09	63	1578560	11.904	ppbv	99
26) Hexane	5.78	57	1456344	12.755	ppbv #	42
47) 1,1,2-Trichloroethane	9.61	97	820621	8.320	ppbv	98
48) Dibromochloromethane	10.45	129	1185421	7.628	ppbv	100
53) Toluene	9.95	91	1835486	6.436	ppbv	99
54) 1,2-Dibromoethane	10.76	107	1236898	7.991	ppbv	97
57) Chlorobenzene	12.30	112	1932489	8.773	ppbv	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL020519\
Data File : VL033182.D
Acq On : 6 Feb 2019 17:54
Operator : SY/AP
Sample : K1289-01DL 2X
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
1000DL

Quant Time: Feb 20 06:51:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL020519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Feb 20 06:00:52 2019
QLast Update : Wed Feb 20 06:00:52 2019
Response via : Initial Calibration

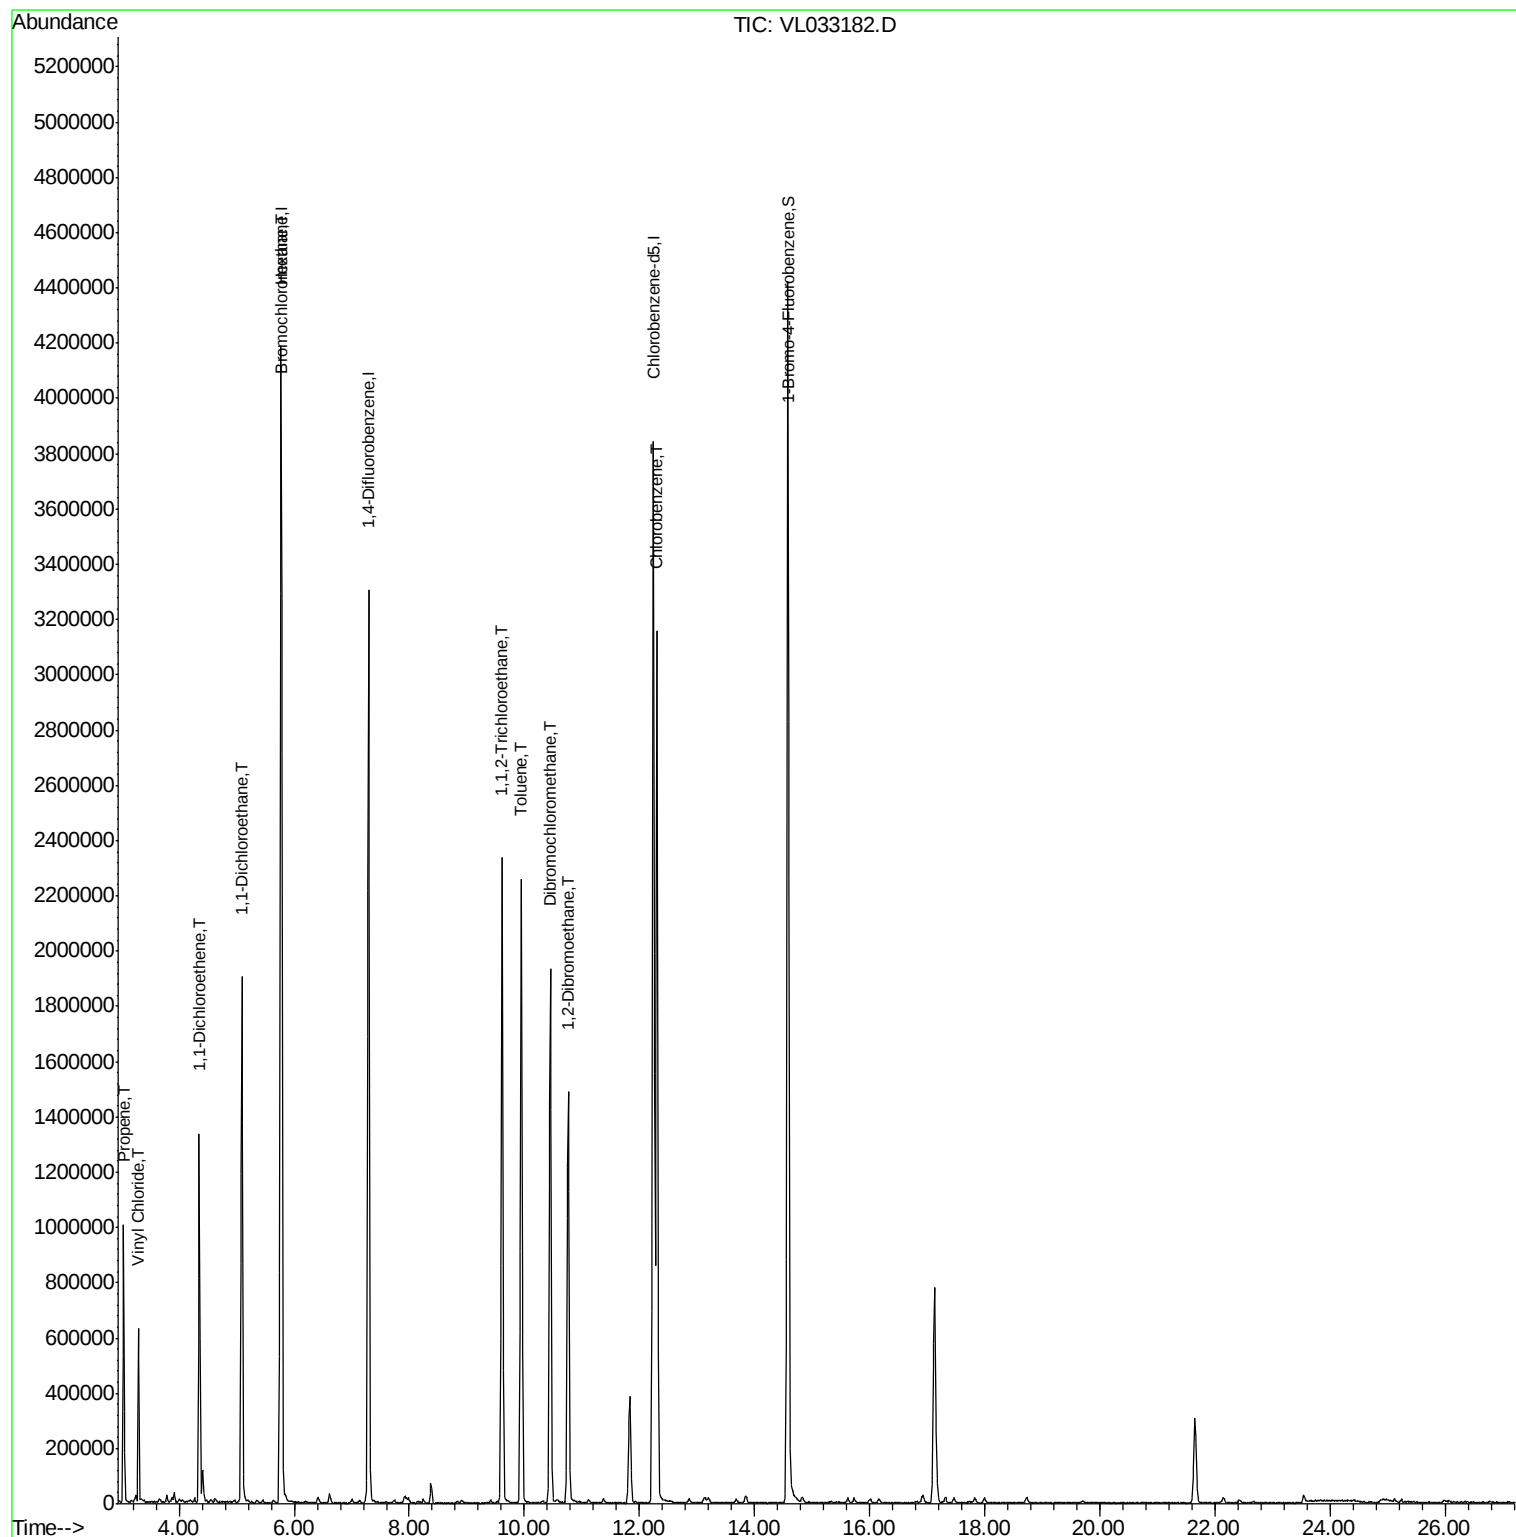

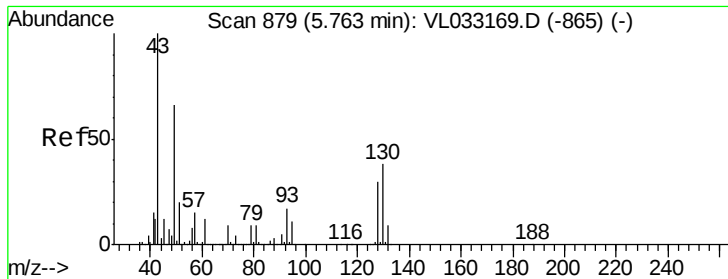

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 878

Delta R.T. -0.00 min

Lab File: VL033182.D

Acq: 6 Feb 2019 17:54

Instrument :

MSVOA_L

ClientSampleId :

1000DL


Tgt Ion: 49 Resp: 960160

Ion Ratio Lower Upper

49 100

128 45.7 23.6 71.0




130 59.1 30.3 91.0

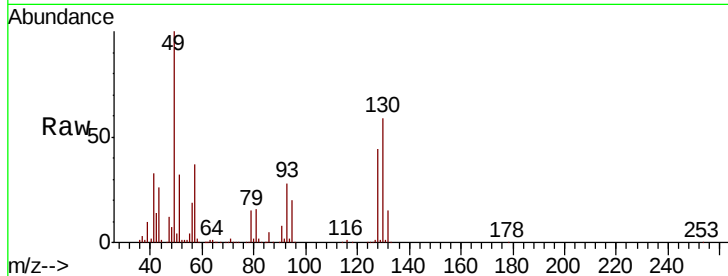

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

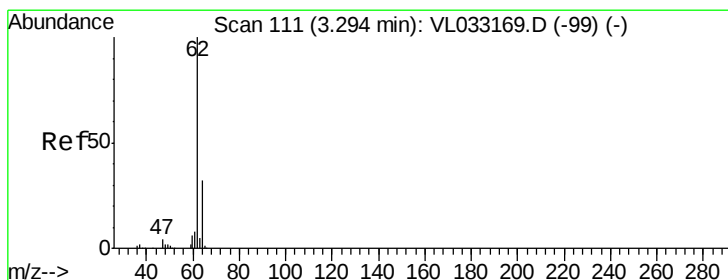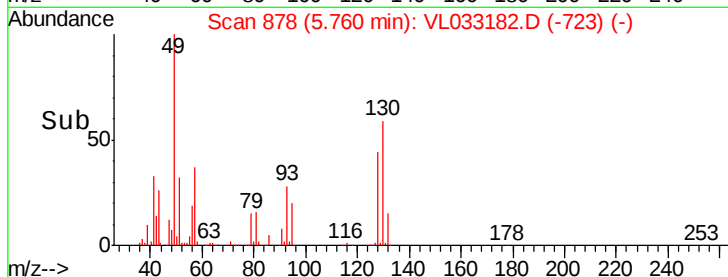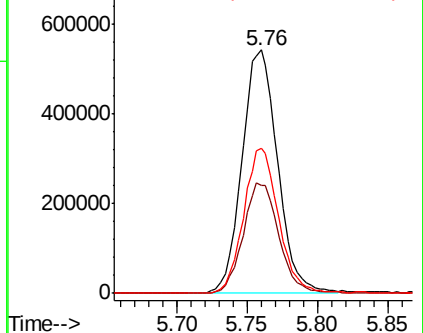

#5

Vinyl Chloride

Concen: 8.050 ppbv

RT: 3.29 min Scan# 110

Delta R.T. -0.00 min

Lab File: VL033182.D


Acq: 6 Feb 2019 17:54

Tgt Ion: 62 Resp: 513146

Ion Ratio Lower Upper



62 100


64 32.5 25.6 38.4

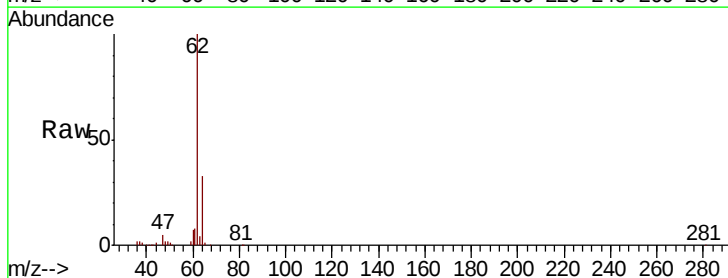

Abundance Ion 62.10 (61.80 to 62.80): VL0

Ion 64.10 (63.80 to 64.80): VL0

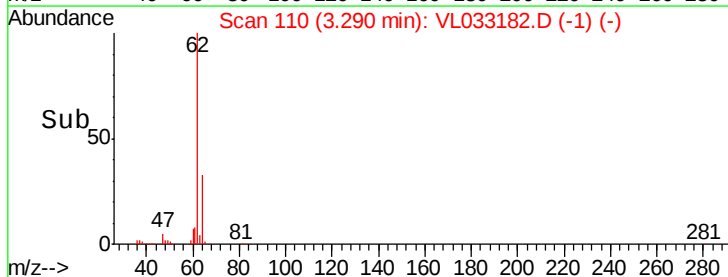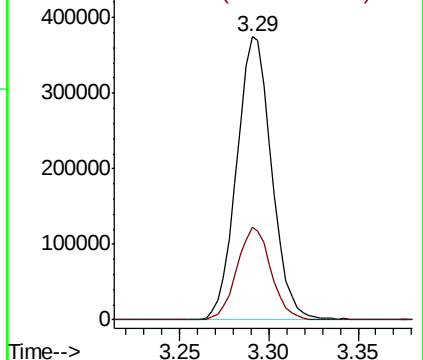

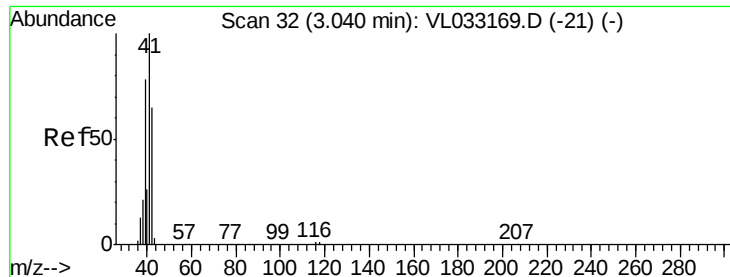

#9

Propene

Concen: 6.961 ppbv

RT: 3.04 min Scan# 31

Delta R.T. -0.00 min

Lab File: VL033182.D

Acq: 6 Feb 2019 17:54

Instrument :

MSVOA_L

ClientSampleId :


1000DL

Tgt Ion: 41 Resp: 388778

Ion Ratio Lower Upper




41 100

42 69.0 55.0 82.6

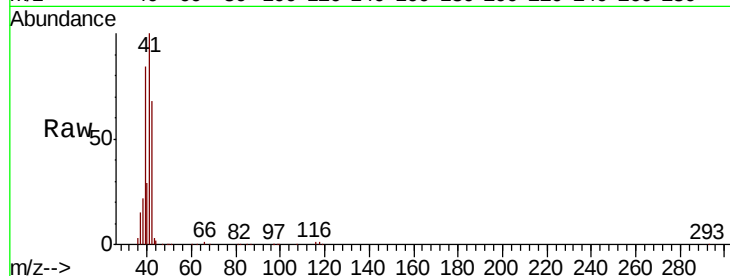

Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 42.10 (41.80 to 42.80): VL0

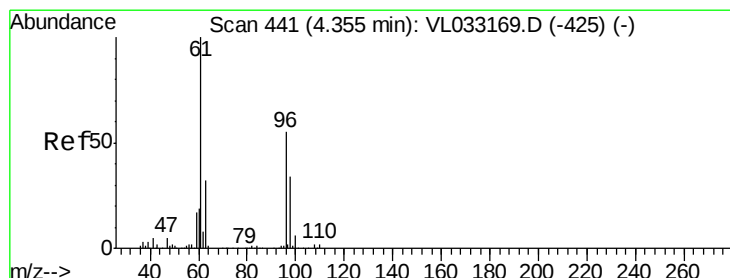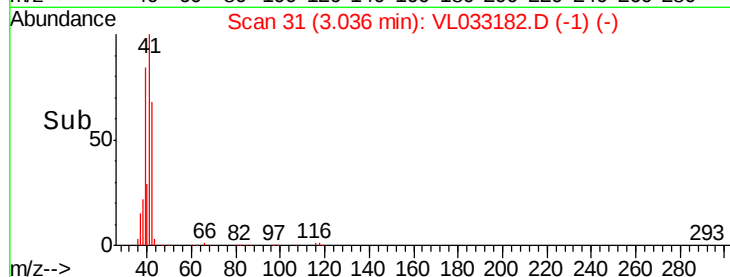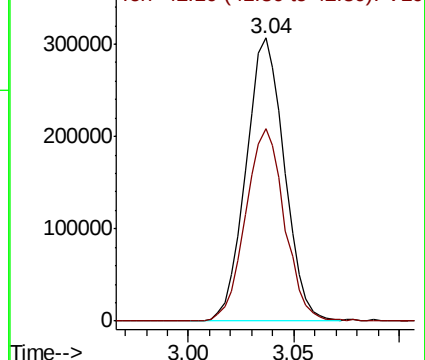

#18

1,1-Dichloroethene

Concen: 8.086 ppbv

RT: 4.35 min Scan# 440

Delta R.T. -0.00 min

Lab File: VL033182.D

Acq: 6 Feb 2019 17:54


Tgt Ion: 96 Resp: 372805

Ion Ratio Lower Upper

96 100

61 190.9 145.0 217.6



98 61.2 50.0 75.0

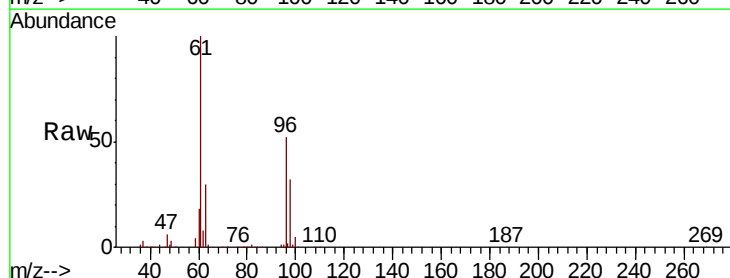


Abundance Ion 96.00 (95.70 to 96.70): VL0

Ion 61.10 (60.80 to 61.80): VL0

Ion 98.00 (97.70 to 98.70): VL0

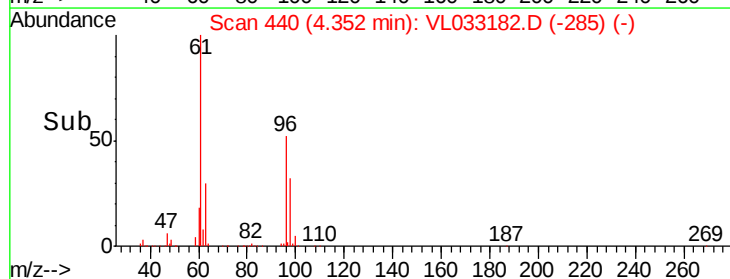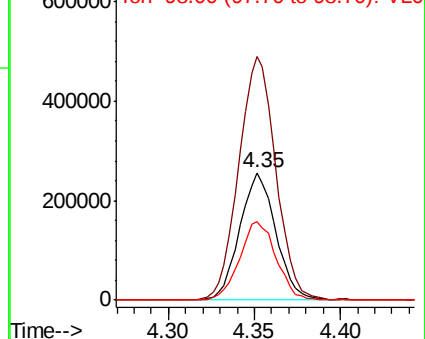

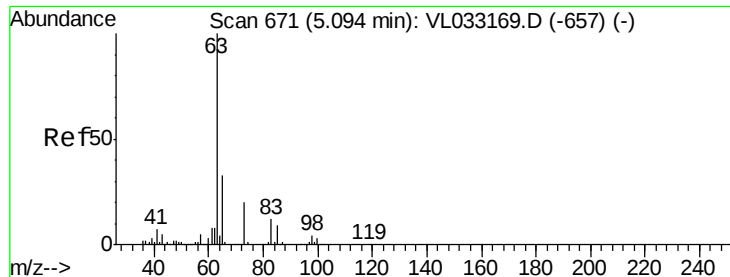

#24

1,1-Dichloroethane

Concen: 11.904 ppbv

RT: 5.09 min Scan# 670

Delta R.T. -0.00 min

Lab File: VL033182.D

Acq: 6 Feb 2019 17:54

Instrument :

MSVOA_L

ClientSampleId :

1000DL


Tgt Ion: 63 Resp: 1578560

Ion Ratio Lower Upper




63 100

98 4.6 2.1 6.5

100 2.7 1.4 4.2

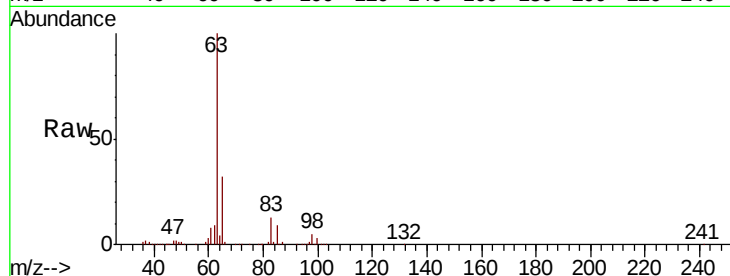

Abundance Ion 63.10 (62.80 to 63.80): VL0
Ion 98.00 (97.70 to 98.70): VL0
Ion 100.00 (99.70 to 100.70): VL0

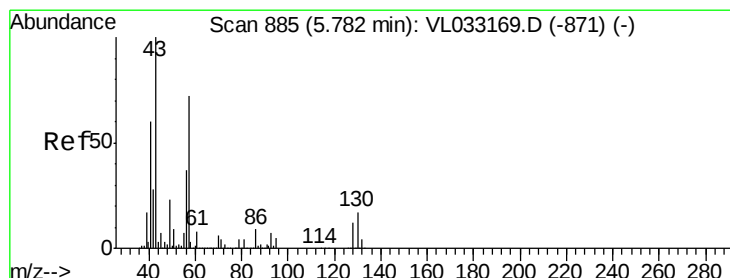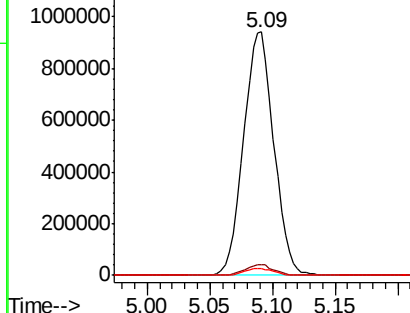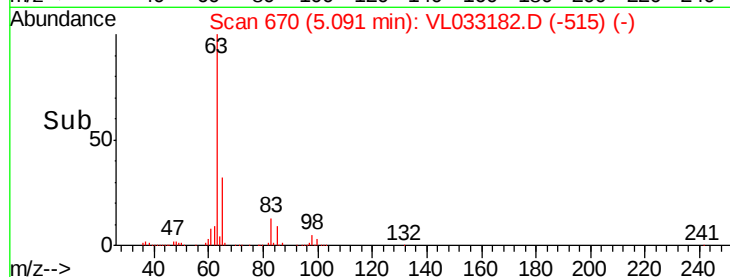

#26

Hexane

Concen: 12.755 ppbv

RT: 5.78 min Scan# 884

Delta R.T. -0.00 min

Lab File: VL033182.D

Acq: 6 Feb 2019 17:54

Tgt Ion: 57 Resp: 1456344


Ion Ratio Lower Upper

57 100



41 88.2 69.4 104.2


43 70.1 176.7 265.1#

56 52.5 41.4 62.0

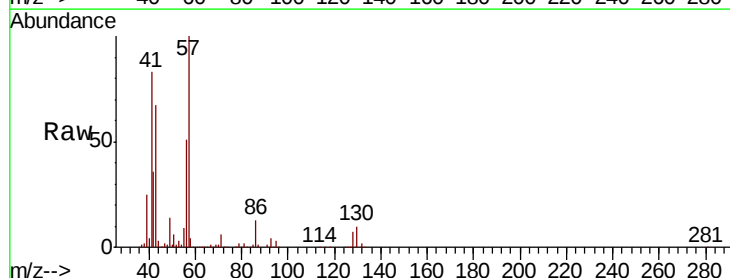

Abundance Ion 57.10 (56.80 to 57.80): VL0
Ion 41.10 (40.80 to 41.80): VL0
Ion 43.10 (42.80 to 43.80): VL0
Ion 56.10 (55.80 to 56.80): VL0



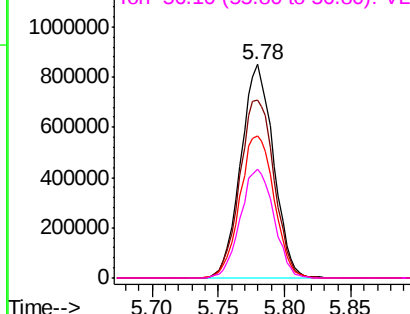
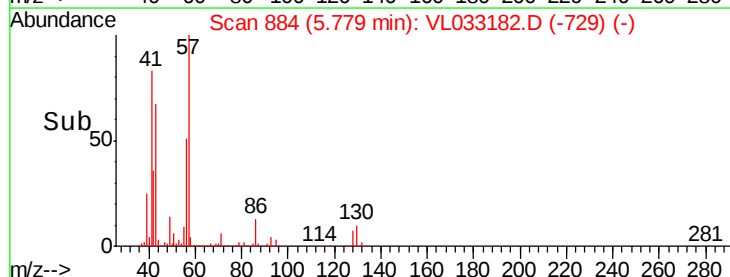


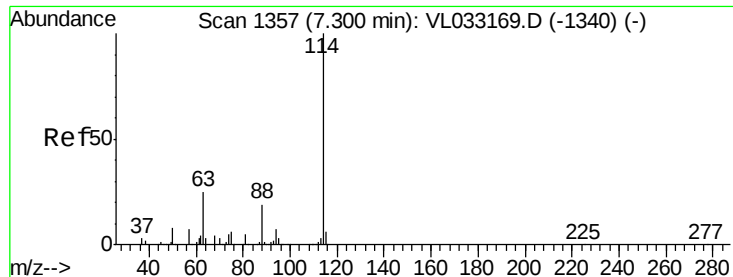

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.29 min Scan# 1353
 Delta R.T. -0.01 min
 Lab File: VL033182.D
 Acq: 6 Feb 2019 17:54




Instrument :
 MSVOA_L
 ClientSampleId :
 1000DL


Tgt Ion:114 Resp: 2376399
 Ion Ratio Lower Upper
 114 100
 63 26.9 20.8 31.2
 88 18.5 14.6 22.0

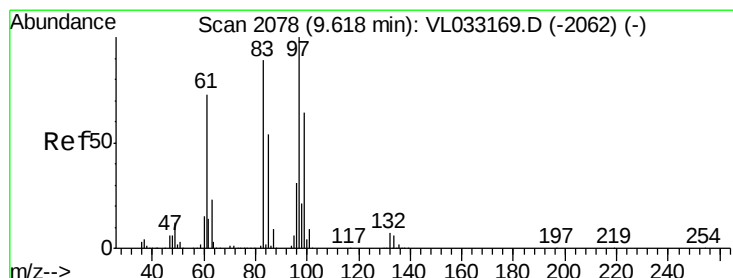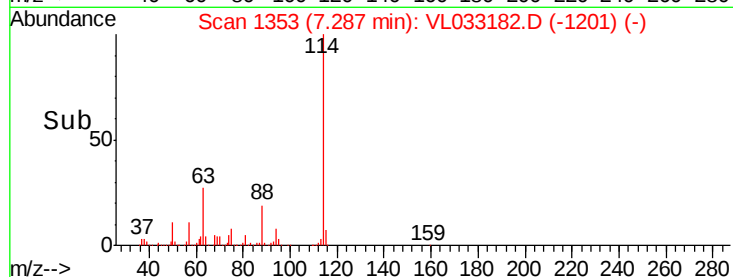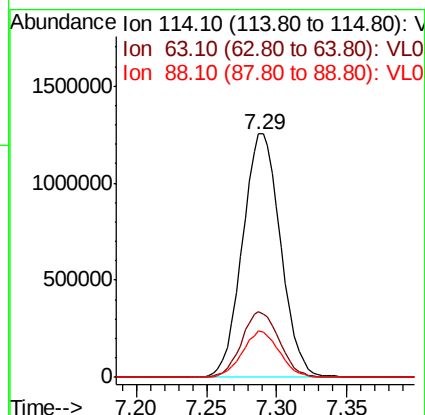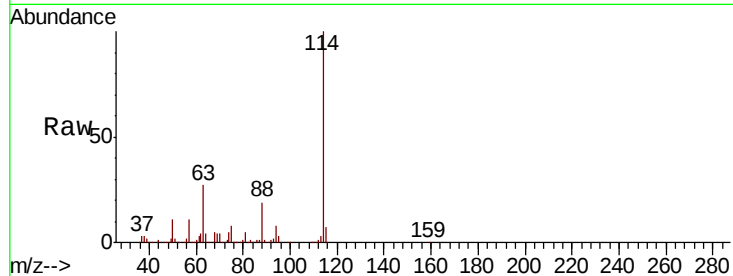

#47
 1,1,2-Trichloroethane
 Concen: 8.320 ppbv
 RT: 9.61 min Scan# 2077
 Delta R.T. -0.00 min
 Lab File: VL033182.D
 Acq: 6 Feb 2019 17:54

Tgt Ion: 97 Resp: 820621
 Ion Ratio Lower Upper
 97 100
 83 88.4 71.4 107.2
 85 57.1 43.5 65.3
 99 61.8 51.4 77.0

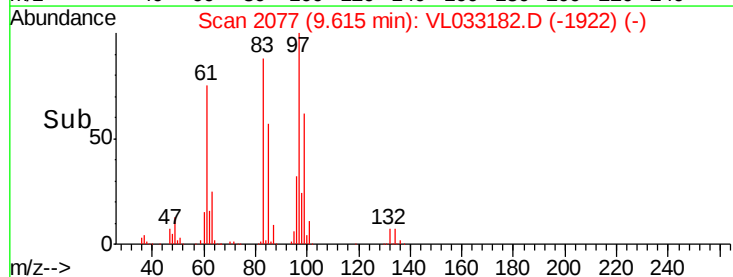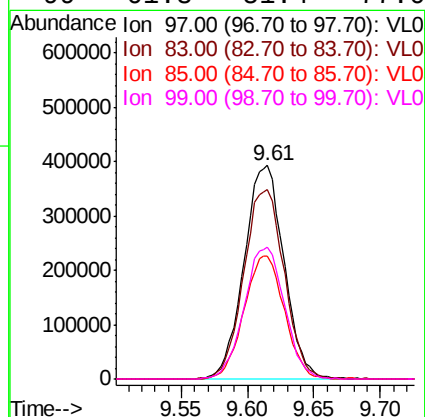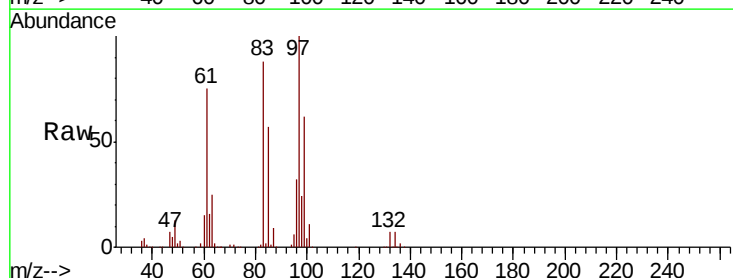

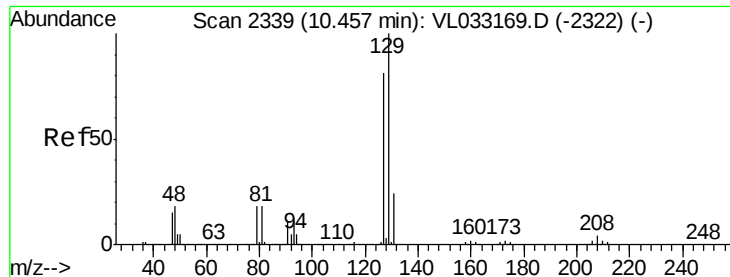

#48

Dibromochloromethane

Concen: 7.628 ppbv

RT: 10.45 min Scan# 2336

Delta R.T. -0.01 min

Lab File: VL033182.D

Acq: 6 Feb 2019 17:54

Instrument :

MSVOA_L

ClientSampleId :


1000DL

Tgt Ion:129 Resp: 1185421

Ion Ratio Lower Upper




129 100

127 77.9 39.1 117.3

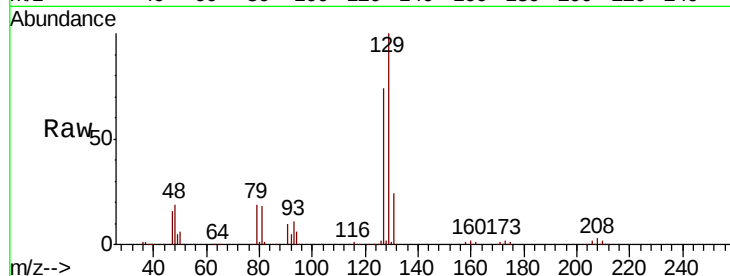

Abundance Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

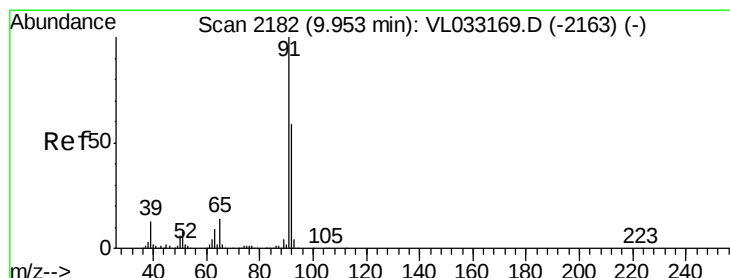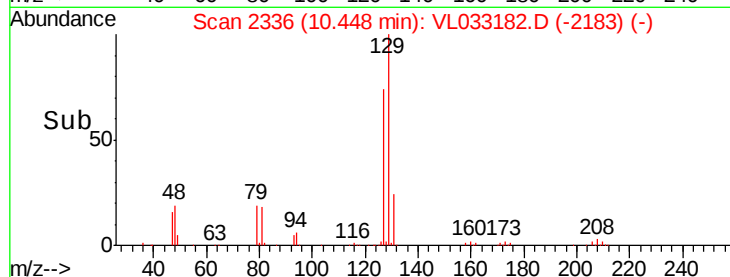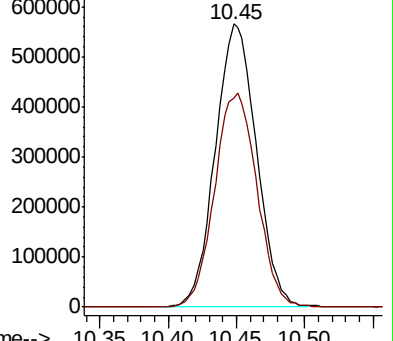

#53

Toluene

Concen: 6.436 ppbv

RT: 9.95 min Scan# 2180

Delta R.T. -0.01 min

Lab File: VL033182.D


Acq: 6 Feb 2019 17:54

Tgt Ion: 91 Resp: 1835486

Ion Ratio Lower Upper



91 100


92 59.0 48.0 72.0

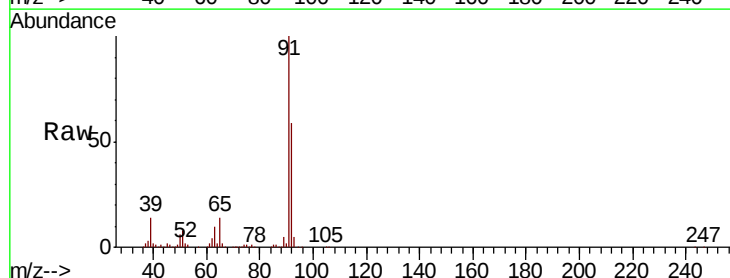

Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 92.10 (91.80 to 92.80): VL0



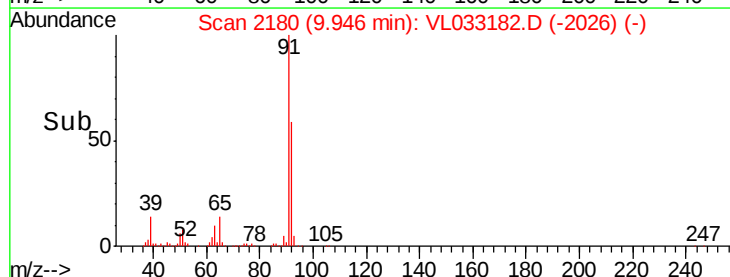
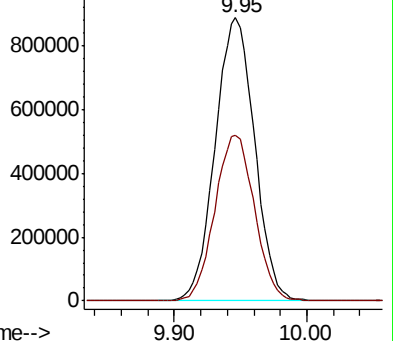


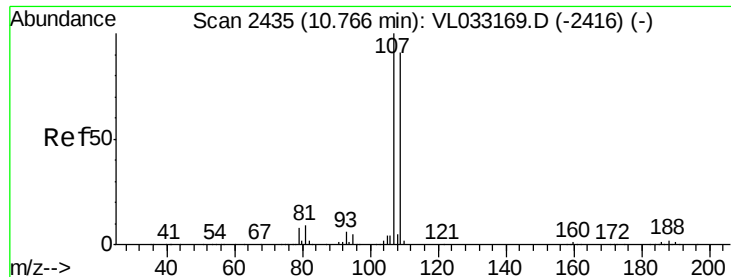

#54
1,2-Dibromoethane
Concen: 7.991 ppbv
RT: 10.76 min Scan# 2433
Delta R.T. -0.01 min
Lab File: VL033182.D
Acq: 6 Feb 2019 17:54




Instrument :
MSVOA_L
ClientSampleId :
1000DL


Tgt Ion:107 Resp: 1236898
Ion Ratio Lower Upper
107 100
109 94.5 73.2 109.8

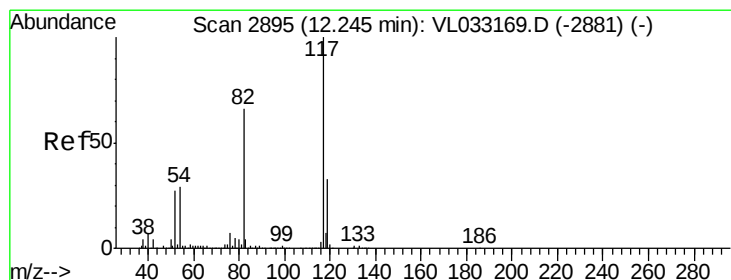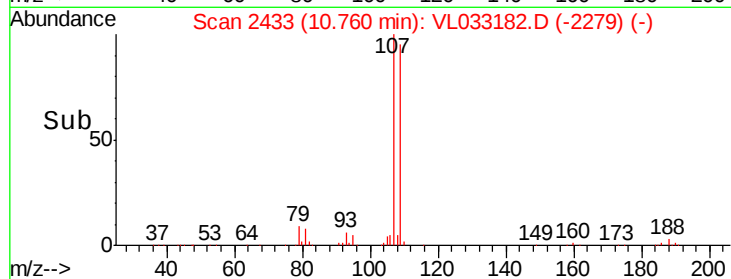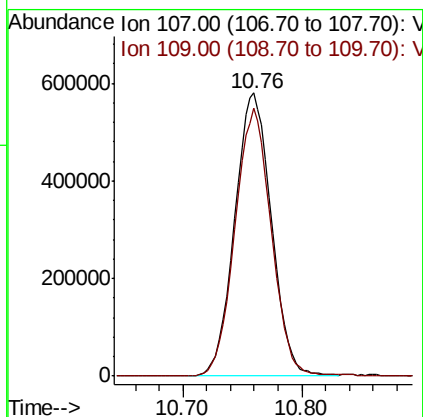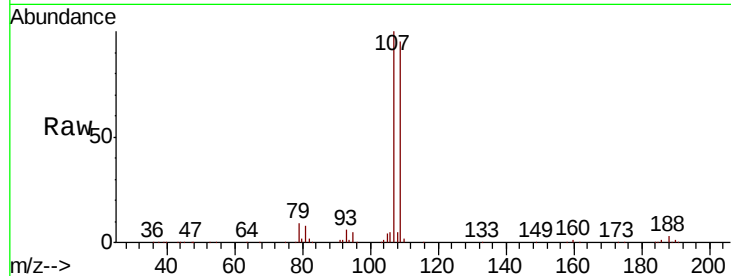

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.24 min Scan# 2894
Delta R.T. -0.00 min
Lab File: VL033182.D
Acq: 6 Feb 2019 17:54

Tgt Ion:117 Resp: 2489478
Ion Ratio Lower Upper
117 100
82 66.2 53.8 80.8
119 32.2 46.9 70.3#

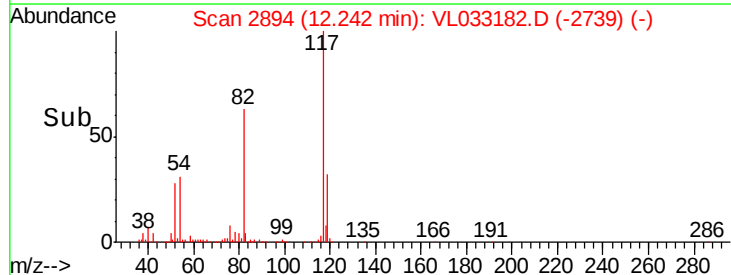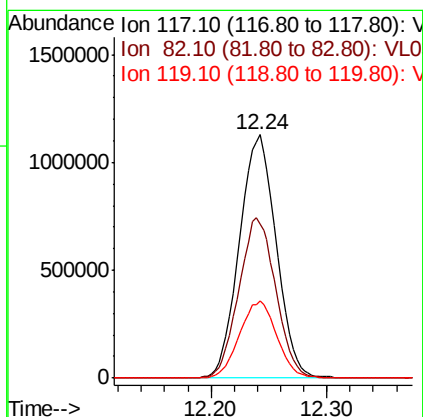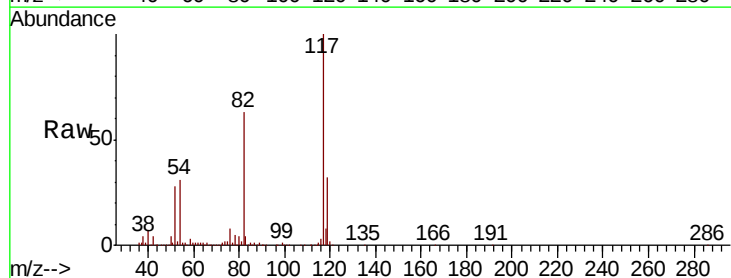


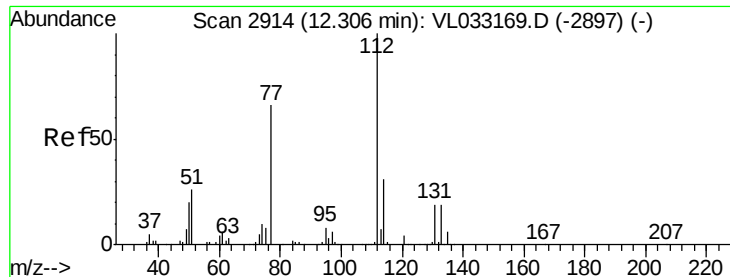




#57
Chlorobenzene
Concen: 8.773 ppbv
RT: 12.30 min Scan# 2912
Delta R.T. -0.01 min
Lab File: VL033182.D
Acq: 6 Feb 2019 17:54

Instrument :
MSVOA_L
ClientSampleId :
1000DL

Tgt Ion: 112 Resp: 1932489
Ion Ratio Lower Upper
112 100
77 69.0 54.0 81.0
114 30.8 27.9 34.1

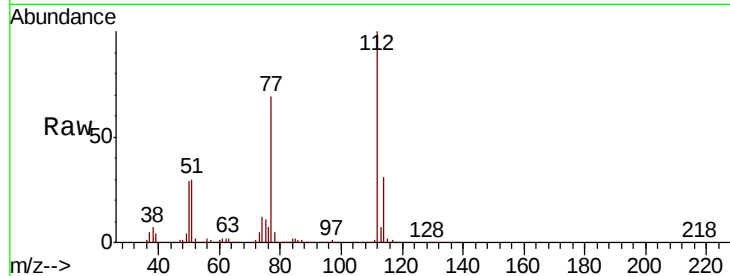


Abundance Ion 112.10 (111.80 to 112.80): V
Ion 77.10 (76.80 to 77.80): VL0
Ion 114.10 (113.80 to 114.80): V

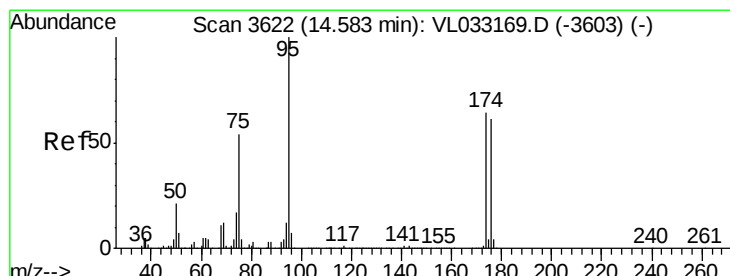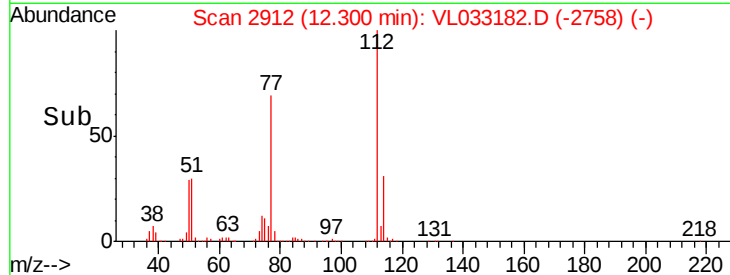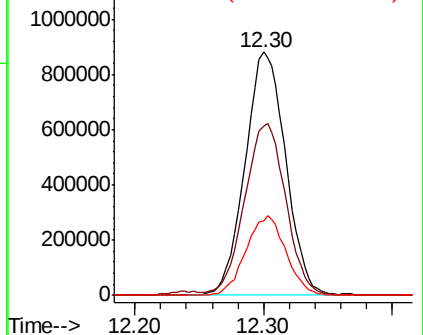

#68
1-Bromo-4-Fluorobenzene
Concen: 11.573 ppbv
RT: 14.58 min Scan# 3621
Delta R.T. -0.00 min
Lab File: VL033182.D
Acq: 6 Feb 2019 17:54

Tgt Ion: 95 Resp: 2245173
Ion Ratio Lower Upper
95 100
174 63.5 51.1 76.7
175 4.5 3.8 5.6

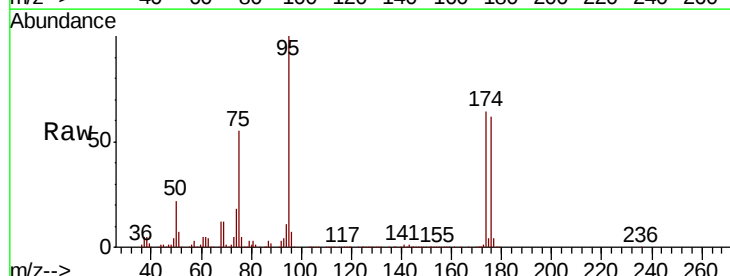

Abundance Ion 95.10 (94.80 to 95.80): VL0
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

