


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL020519\
 Data File : VL033168.D
 Acq On : 6 Feb 2019 1:12
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL020519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 20 06:00:52 2019
 Last Update : Wed Feb 20 06:00:52 2019

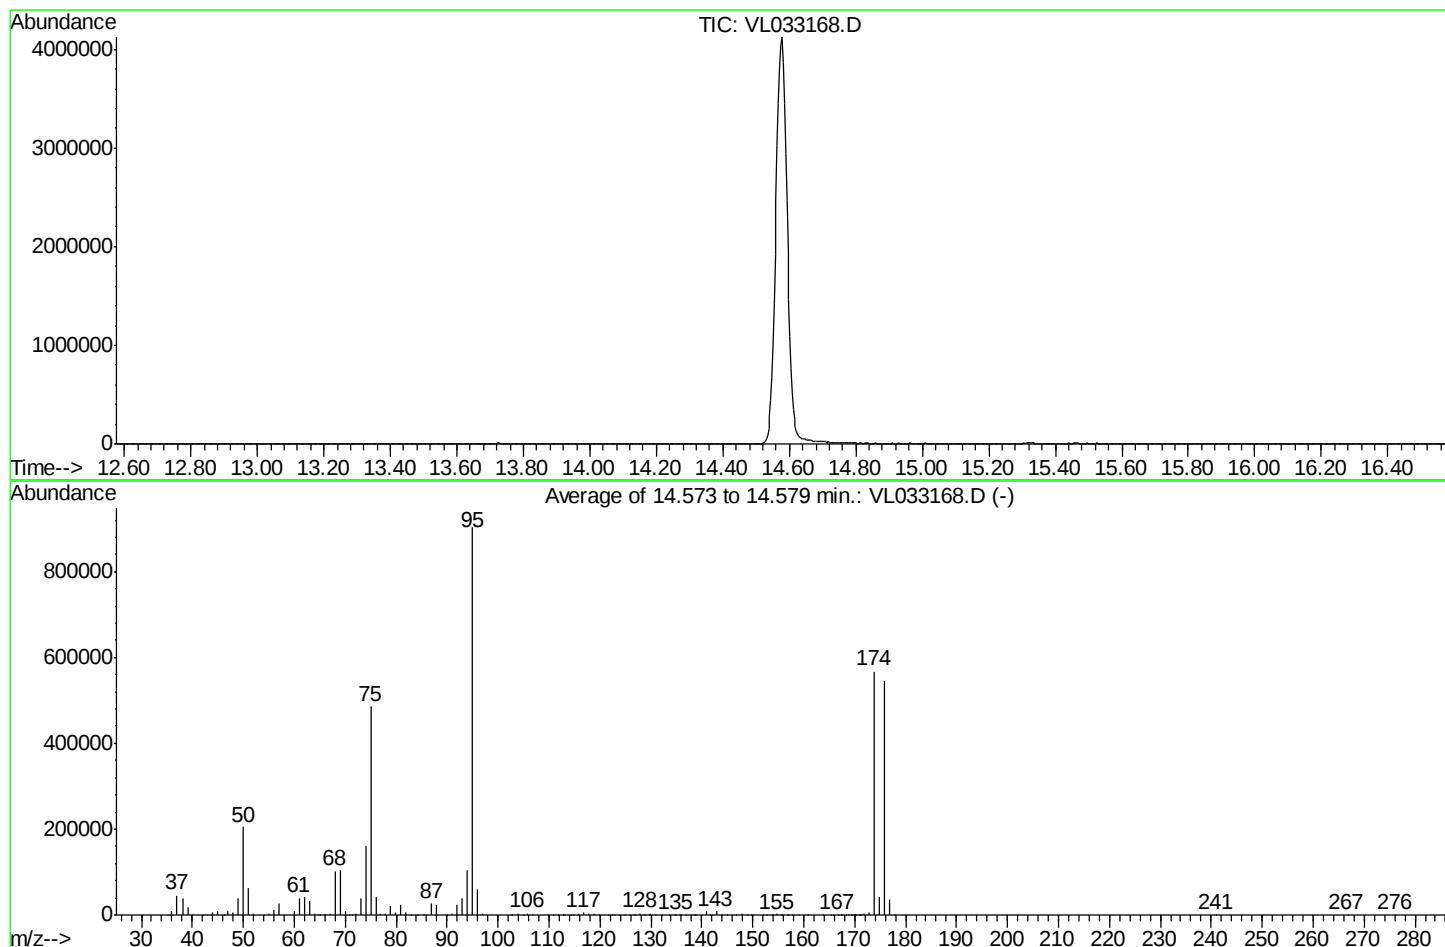

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	205354	PASS
75	95	30	66	53.8	485738	PASS
95	95	100	100	100.0	903232	PASS
96	95	5	9	6.7	60802	PASS
173	174	0.00	2	1.0	5924	PASS
174	95	50	120	62.8	566997	PASS
175	174	4	9	7.3	41541	PASS
176	174	93	101	96.3	545898	PASS
177	176	5	9	6.8	37008	PASS