

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020623\
 Data File : VL040142.D
 Acq On : 6 Feb 2023 11:58
 Operator : SY/MD
 Sample : VL0206ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0206ABL01

Quant Time: Feb 07 05:53:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jan 31 05:24:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.185	49	893684	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.648	114	2411637	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.465	117	2064663	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.777	95	1599201	9.320	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	93.200%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020623\
Data File : VL040142.D
Acq On : 6 Feb 2023 11:58
Operator : SY/MD
Sample : VL0206ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0206ABL01

Quant Time: Feb 07 05:53:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jan 31 05:24:57 2023
Response via : Initial Calibration




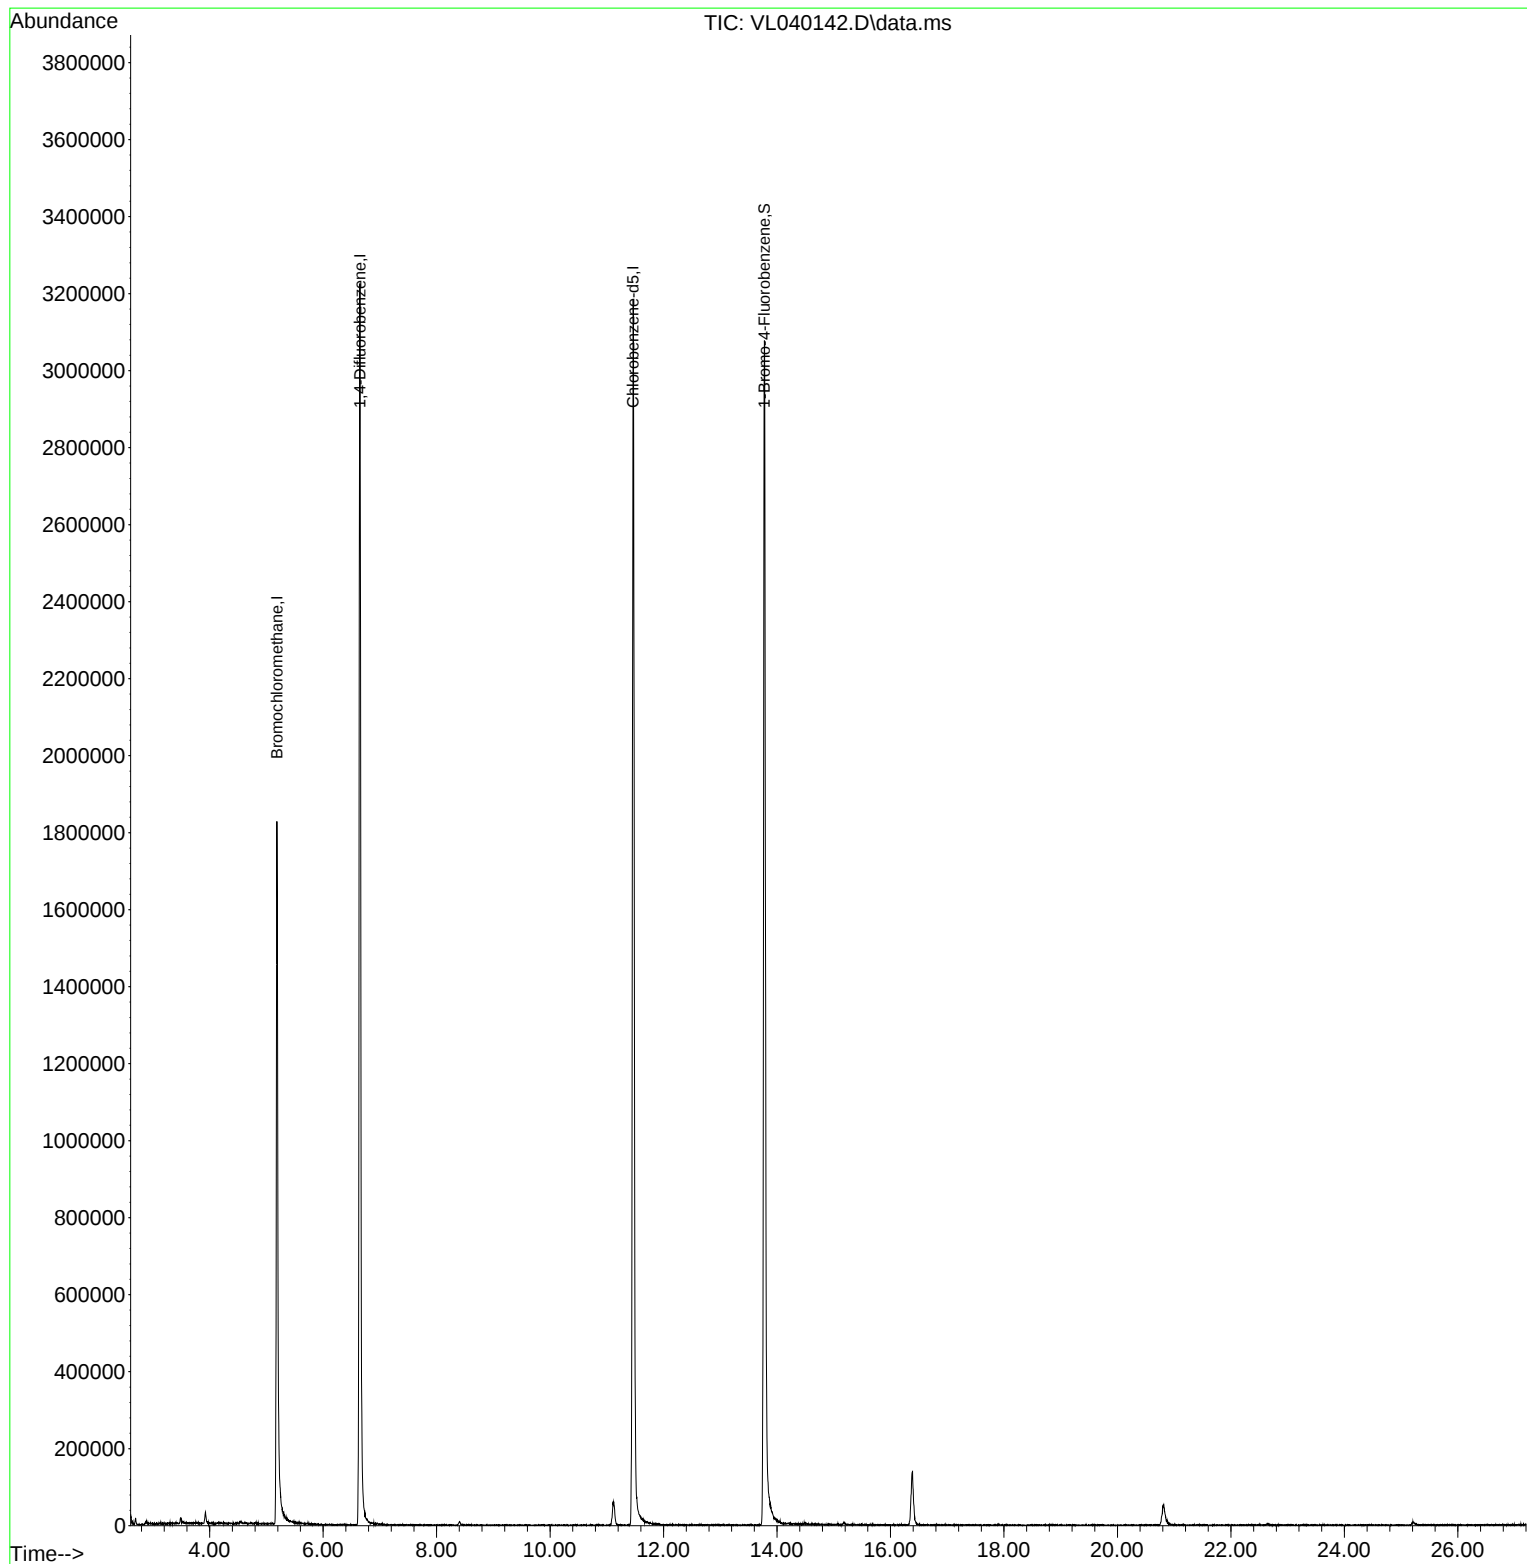




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.185 min Scan# 803
Delta R.T. 0.006 min
Lab File: VL040142.D
Acq: 6 Feb 2023 11:58




Instrument :
MSVOA_L
ClientSampleId :
VL0206ABL01


Tgt Ion: 49 Resp: 893684
Ion Ratio Lower Upper
49 100
128 50.8 23.6 71.0
130 63.6 29.8 89.3

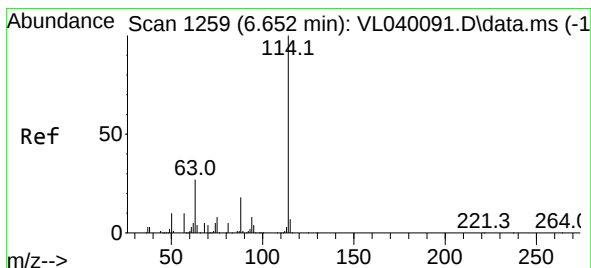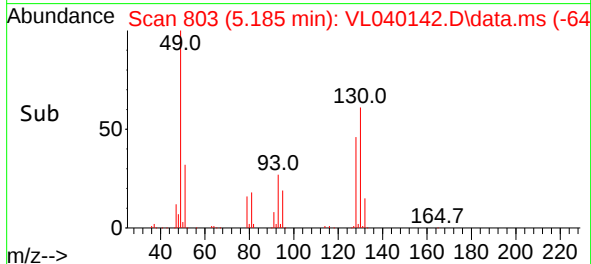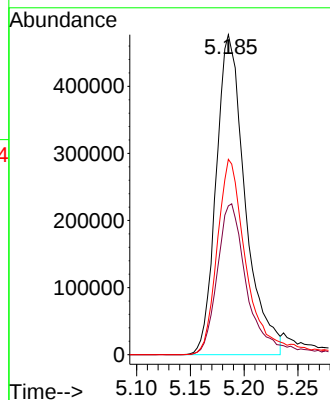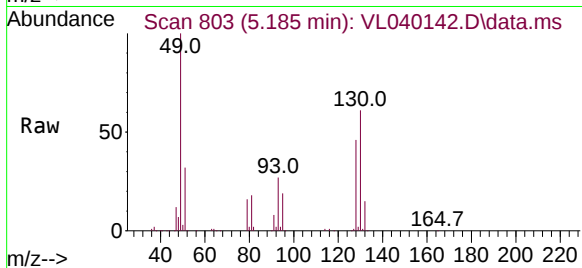

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.648 min Scan# 1258
Delta R.T. 0.006 min
Lab File: VL040142.D
Acq: 6 Feb 2023 11:58

Tgt Ion: 114 Resp: 2411637
Ion Ratio Lower Upper
114 100
63 26.0 21.8 32.8
88 18.4 14.8 22.2


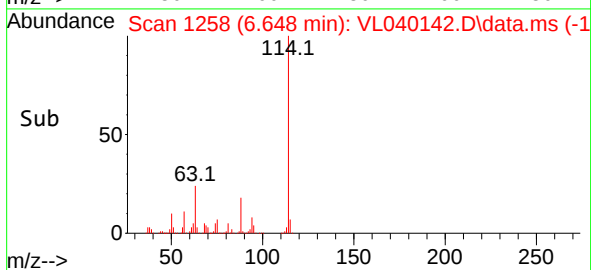
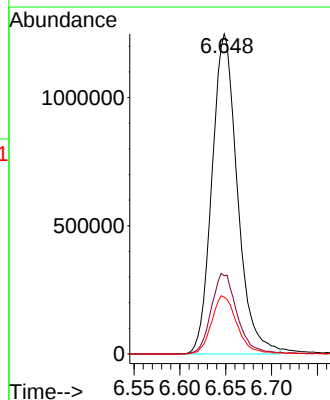
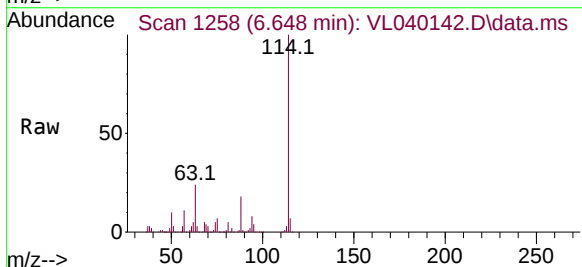


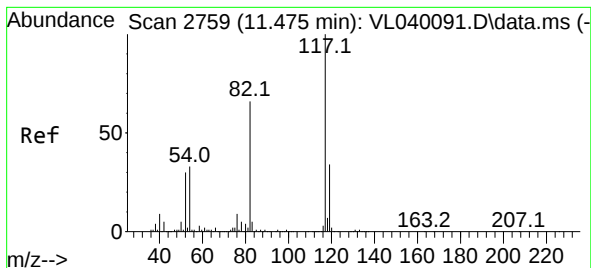

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.465 min Scan# 21
Delta R.T. 0.006 min
Lab File: VL040142.D
Acq: 6 Feb 2023 11:58

Instrument :
MSVOA_1
ClientSampleId :
VL0206ABL01

Tgt Ion:117 Resp: 2064663
Ion Ratio Lower Upper
117 100
82 68.0 54.4 81.6
119 33.3 26.8 40.2

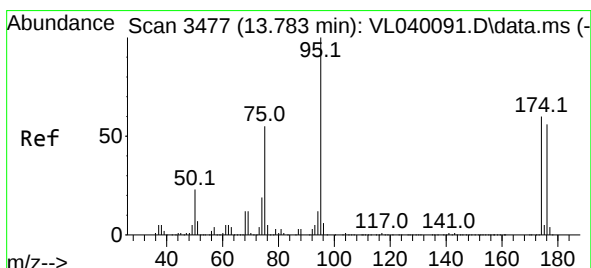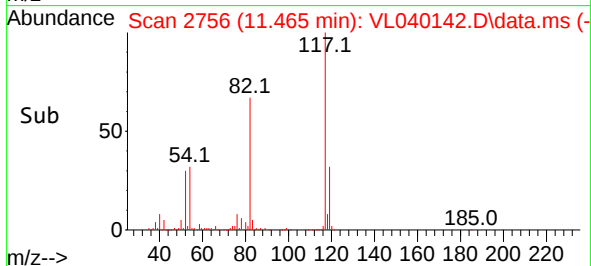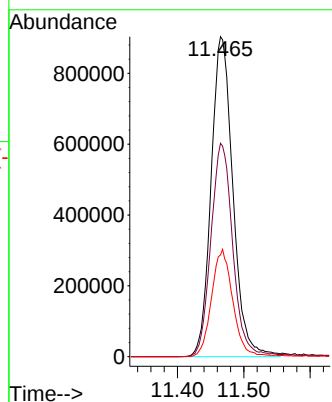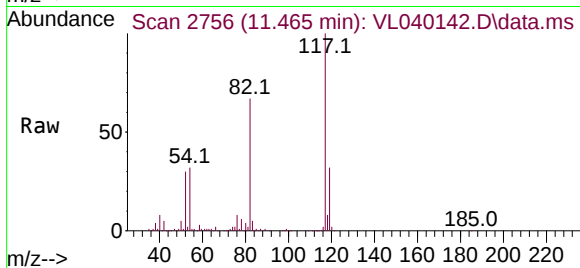

#68
1-Bromo-4-Fluorobenzene
Concen: 9.320 ppbv
RT: 13.777 min Scan# 3475
Delta R.T. 0.006 min
Lab File: VL040142.D
Acq: 6 Feb 2023 11:58

Tgt Ion: 95 Resp: 1599201
Ion Ratio Lower Upper
95 100
174 60.0 47.7 71.5
175 4.1 3.4 5.2

