
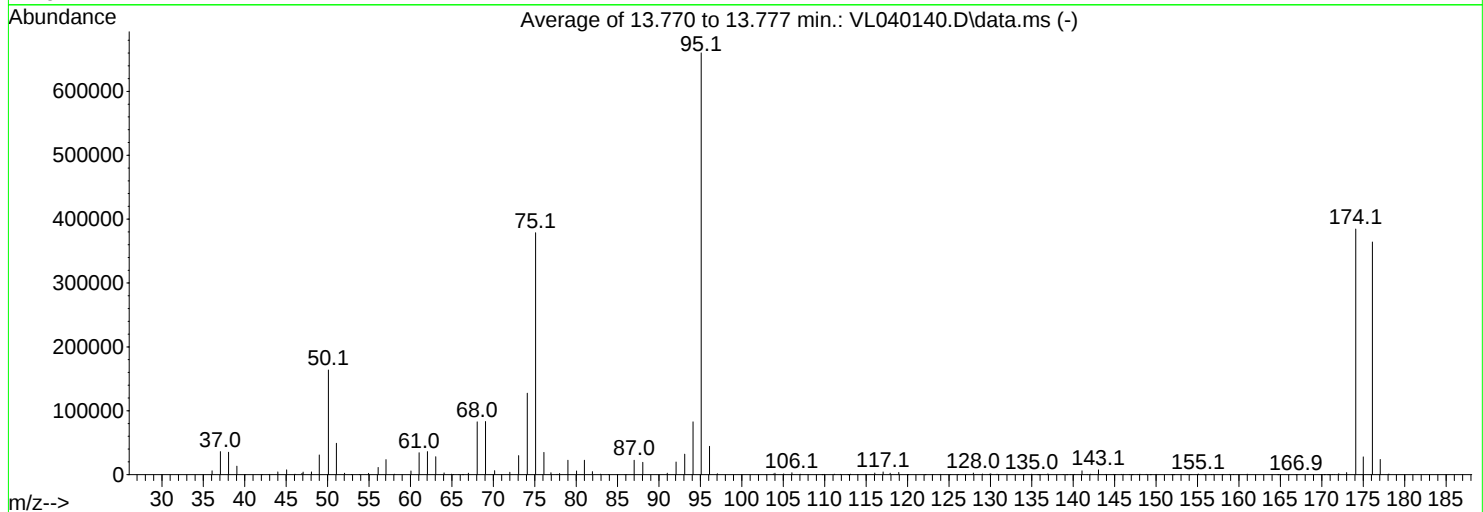


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020623\
Data File : VL040140.D
Acq On : 6 Feb 2023 10:12
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 31 05:24:57 2023

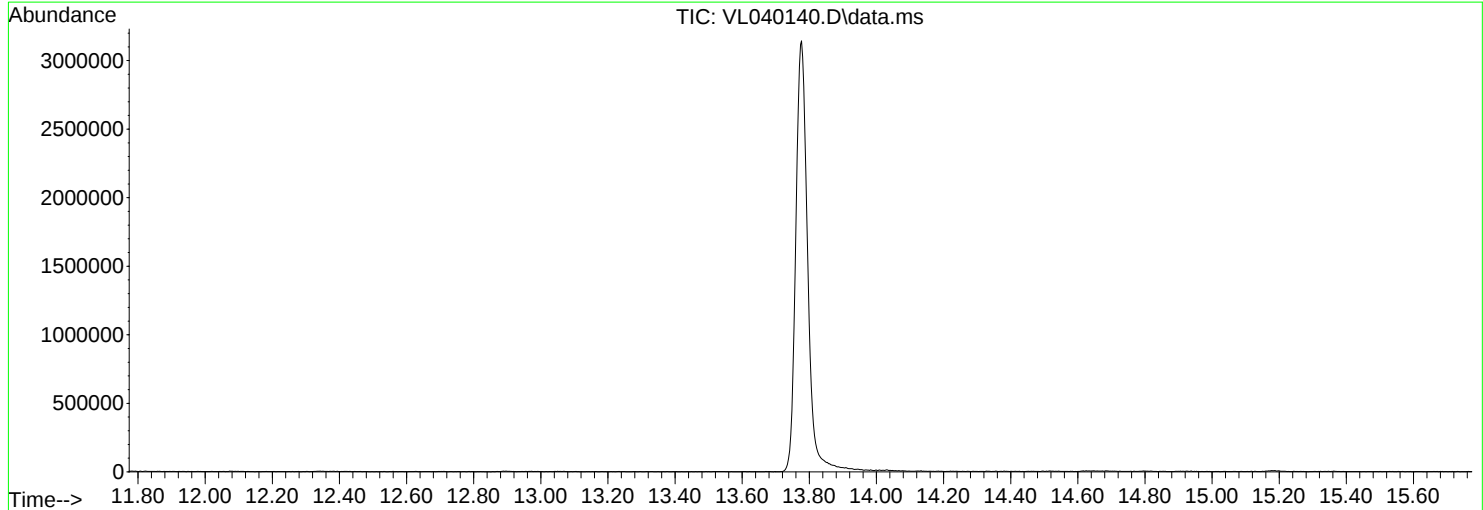

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	163883	PASS
75	95	30	66	57.4	378816	PASS
95	95	100	100	100.0	660331	PASS
96	95	5	9	6.7	44237	PASS
173	174	0.00	2	0.9	3319	PASS
174	95	50	120	58.2	384491	PASS
175	174	4	9	7.2	27837	PASS
176	174	93	101	94.8	364309	PASS
177	176	5	9	6.5	23715	PASS

Average of 13.770 to 13.777 min.: VL040140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6116	47.05	4029	58.05	709	68.05	8269
37.05	36141	48.05	4338	60.05	5896	69.05	8322
38.05	34979	49.00	30901	61.05	34437	70.15	625
39.05	13280	50.10	163883	62.05	36107	71.00	36
39.95	94	51.05	49045	63.05	27973	72.00	3818
42.00	84	52.05	2217	64.05	2812	73.05	29896
42.95	404	52.90	366	64.95	866	74.10	127515
44.00	4396	53.85	240	65.20	379	75.10	378816
45.05	7564	54.95	2077	65.85	185	76.10	34877
46.05	686	56.10	11178	66.30	79	76.95	3137
46.90	2078	57.05	23520	67.00	2155	77.70	421

Average of 13.770 to 13.777 min.: VL040140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.00	1675	91.00	2164	106.05	3096	117.05	4181
79.00	22661	92.05	19848	107.05	845	117.90	2225
80.05	5755	93.10	31997	109.70	115	118.95	3495
81.00	22448	94.10	82741	109.95	411	120.00	89
81.95	4694	95.10	660331	111.15	803	122.10	90
82.95	720	96.10	44237	111.90	541	123.05	304
83.90	174	97.05	1422	112.80	121	123.95	569
85.90	262	102.95	247	113.10	646	125.20	183
86.10	167	103.80	993	114.00	178	126.15	249
87.00	22624	104.00	2320	114.95	573	127.05	449
88.05	19357	105.05	1160	116.05	2432	127.95	2551

Average of 13.770 to 13.777 min.: VL040140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.05	1118	139.20	125	146.10	439	153.80	215
129.90	678	139.70	160	146.80	299	154.20	267
130.05	1447	140.10	586	147.10	159	155.10	1037
130.80	705	141.05	6133	147.80	296	155.80	92
131.00	358	141.70	227	148.05	827	156.00	256
134.00	50	142.05	738	148.80	418	156.70	208
135.00	890	143.05	7639	149.30	111	156.95	552
135.70	79	143.95	501	150.00	510	158.00	88
135.90	113	144.90	418	151.90	64	158.90	445
136.95	1314	145.10	270	152.10	87	159.35	304
138.80	168	145.80	537	153.00	618	161.00	690

Average of 13.770 to 13.777 min.: VL040140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
164.70	72	175.00	27837				
166.90	77	176.10	364309				
169.90	116	177.05	23715				
170.30	63	178.10	1095				
170.70	111						
170.90	140						
171.25	202						
171.50	211						
172.05	1411						
173.00	3319						
174.10	384491						