
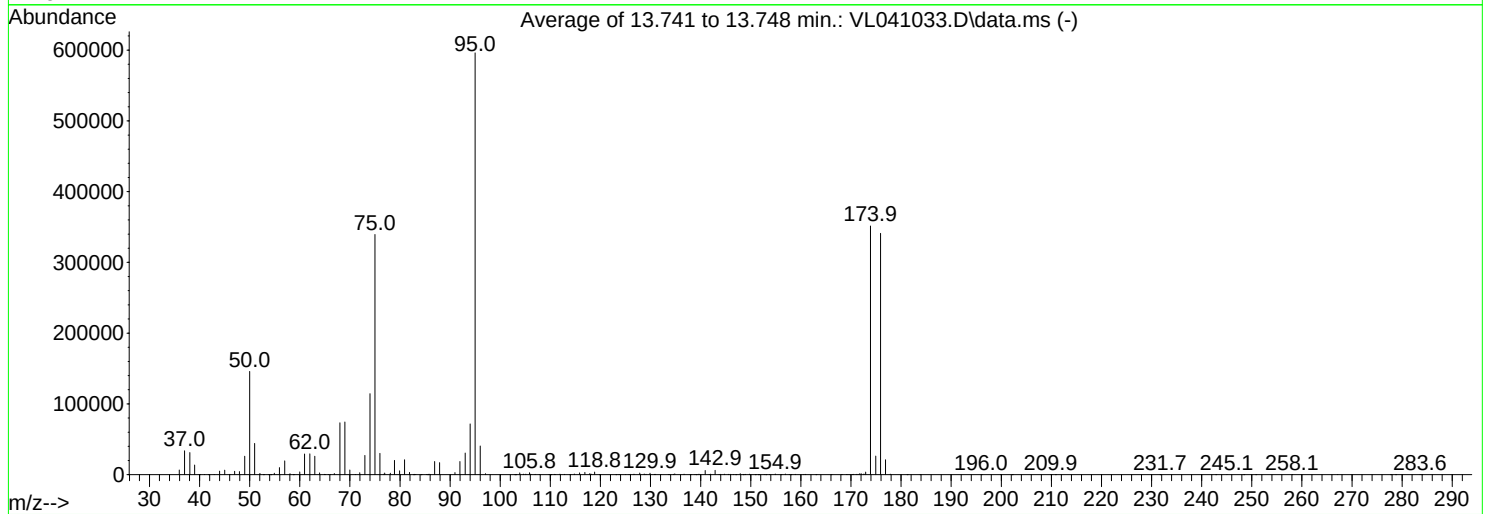


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020724\
Data File : VL041033.D
Acq On : 7 Feb 2024 9:48
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL012324AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Feb 08 02:04:13 2024

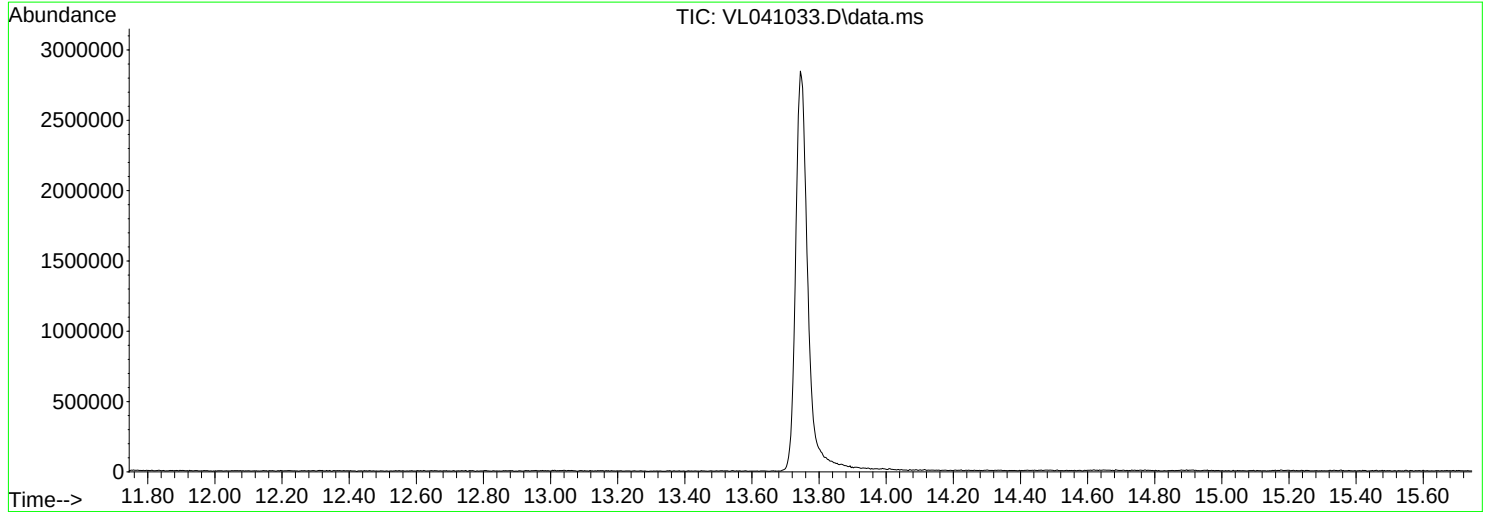

AutoFind: Scans 3464, 3465, 3466; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	145856	PASS
75	95	30	66	56.9	339499	PASS
95	95	100	100	100.0	596203	PASS
96	95	5	9	6.8	40508	PASS
173	174	0.00	2	1.0	3661	PASS
174	95	50	120	58.9	351403	PASS
175	174	4	9	7.5	26299	PASS
176	174	93	101	97.1	341141	PASS
177	176	5	9	6.2	21144	PASS

Average of 13.741 to 13.748 min.: VL041033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	6540	46.05	506	55.95	9962	65.70	2011
37.00	33797	47.00	4877	57.00	19520	66.15	2311
38.05	31245	47.95	4307	58.05	1330	66.90	1711
39.00	13594	49.00	26026	58.70	55	68.00	7326
39.90	14	50.00	145856	60.00	3962	69.00	74429
40.10	273	51.00	44184	60.95	29264	70.00	6605
41.00	153	52.05	1827	62.00	29379	71.10	275
41.80	50	52.75	112	63.00	26008	71.95	2777
42.90	283	53.80	124	63.95	2500	73.00	27208
44.00	4972	54.20	69	64.90	567	74.00	114464
45.00	6301	54.90	2161	65.10	190	75.00	339499

Average of 13.741 to 13.748 min.: VL041033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	30088	84.20	58	95.00	596203	107.80	160
76.80	675	85.30	166	96.00	40508	109.75	307
76.95	2309	85.50	112	97.05	1315	109.90	313
78.05	1965	85.80	630	102.90	114	110.10	57
78.90	20189	86.00	154	103.10	105	110.80	544
79.90	5429	86.90	18512	103.90	2543	111.00	335
80.90	20992	87.90	17000	104.65	795	111.90	667
81.90	3199	90.95	2889	105.10	672	112.85	435
82.70	93	91.95	18560	105.85	2684	113.90	116
82.95	521	93.00	30432	106.10	654	114.80	878
83.15	331	94.00	71597	106.95	418	115.85	2507

Average of 13.741 to 13.748 min.: VL041033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.90	3073	126.70	603	134.85	1171	143.95	409
117.85	1437	127.85	2333	136.70	750	144.75	658
118.10	810	128.75	982	137.90	75	145.60	389
118.85	3595	129.10	402	138.85	158	145.95	545
119.80	87	129.90	1954	139.10	73	146.60	214
123.10	72	130.80	544	139.65	667	147.00	120
123.70	271	131.00	526	140.90	5888	147.90	1456
123.90	140	132.05	151	141.70	296	148.50	79
125.05	219	133.55	250	141.95	655	148.95	567
125.70	150	133.80	307	142.90	6184	149.75	717
125.95	548	134.60	484	143.70	193	150.90	52

Average of 13.741 to 13.748 min.: VL041033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
151.50	87	160.60	262	171.05	414	181.20	119
151.70	159	160.95	575	171.40	557	183.80	96
152.70	339	163.00	78	171.75	1315	196.00	63
153.00	104	166.00	112	172.05	1292	199.90	102
153.75	141	168.10	130	172.60	969	202.20	59
154.90	1026	168.25	236	172.95	3661	209.90	120
156.00	97	169.15	257	173.90	351403	210.80	84
156.90	944	169.40	291	174.95	26299	231.70	83
157.70	191	169.80	175	175.90	341141	242.80	54
158.00	64	170.30	282	176.90	21144	245.05	172
158.90	563	170.55	510	177.85	734	248.40	58

Average of 13.741 to 13.748 min.: VL041033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
250.80	75						
258.10	217						
267.15	200						
277.70	72						
278.70	77						
283.60	166						
283.90	58						

Instrument :
MSVOA_L
ClientSampleId :
BFB