

Data Path : W:\HPCHEM1\MSVOA L\DATA\VL020916\
 Data File : VL026841.D
 Acq On : 10 Feb 2016 5:33
 Operator : SY/AP
 Sample : H1388-02
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IAS-2

Manual Integrations
 APPROVED

MMDadoda
 2/11/2016 1:24:13 PM

Quant Time: Feb 10 08:03:42 2016
 Quant Method : W:\HPCHEM1\MSVOA L\METHODS\VL020916AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Feb 10
 QLast Update : Wed Feb 10 03:14:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	6.70	49	1334192	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	8.37	114	3677487	10.00	ppbv	0.00
55) Chlorobenzene-d5	13.79	117	1455152	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	16.33	95	1642157	15.72	ppbv	-0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	157.20%#

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.67	85	183320	0.64	ppbv	96
3) Chlorodifluoromethane	3.60	51	921741m	4.26	ppbv	
4) Chloromethane	3.78	50	59609	0.70	ppbv	97
9) Propene	3.64	41	158425	2.71	ppbv #	75
10) Heptane	9.40	43	89178	0.47	ppbv #	82
11) Trichlorofluoromethane	4.73	101	144765	0.42	ppbv	96
12) 1,1,2-Trichlorotrifluoroet	5.34	101	36113	0.15	ppbv	96
13) Ethanol	4.37	45	6304623	626.88	ppbv	98
15) Acetone	4.63	43	17920261	97.77	ppbv #	64
19) Isopropyl Alcohol	4.81	45	4806684	73.51	ppbv #	92
20) Methylene Chloride	5.20	84	57988	0.61	ppbv	97
25) Ethyl Acetate	6.71	43	641222	2.33	ppbv #	93
29) Chloroform	6.79	83	29142	0.12	ppbv	92
30) Cyclohexane	8.32	84	38241m	0.30	ppbv	
34) 2-Butanone	6.24	43	129343	0.72	ppbv	98
35) Carbon Tetrachloride	8.21	117	25770	0.10	ppbv	98
36) Benzene	8.07	78	202486	0.69	ppbv #	95
38) Trichloroethene	9.12	130	4285	0.03	ppbv	88
43) Methyl Methacrylate	9.31	69	71138	0.70	ppbv	95
44) 2,2,4-Trimethylpentane	9.13	57	49175	0.10	ppbv #	70
52) Tetrachloroethene	12.84	164	25515	0.22	ppbv	96
53) Toluene	11.28	91	1782708	5.43	ppbv	99
58) Ethyl Benzene	14.46	91	102741	0.59	ppbv	98
59) m/p-Xylene	14.74	91	258073	1.72	ppbv	99
60) o-Xylene	15.54	91	78301	0.48	ppbv	98
61) Styrene	15.36	104	18247	0.33	ppbv	99
69) p-Isopropyltoluene	19.84	119	24969	0.13	ppbv #	75
72) 4-Ethyltoluene	17.87	105	32995	0.22	ppbv #	94
73) 1,3,5-Trimethylbenzene	18.04	105	30056	0.20	ppbv	90
74) 1,2,4-Trimethylbenzene	18.88	105	111580	0.67	ppbv #	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL020916\
Data File : VL026841.D
Acq On : 10 Feb 2016 5:33
Operator : SY/AP
Sample : H1388-02
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IAS-2

Manual Integrations
APPROVED

MMDadoda
2/11/2016 1:24:13 PM

Quant Time: Feb 10 08:03:42 2016
Quant Method : W:\HPCHEM1\MSVOA L\METHODS\VL020916AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Feb
QLast Update : Wed Feb 10 03:14:04 2016
Response via : Initial Calibration

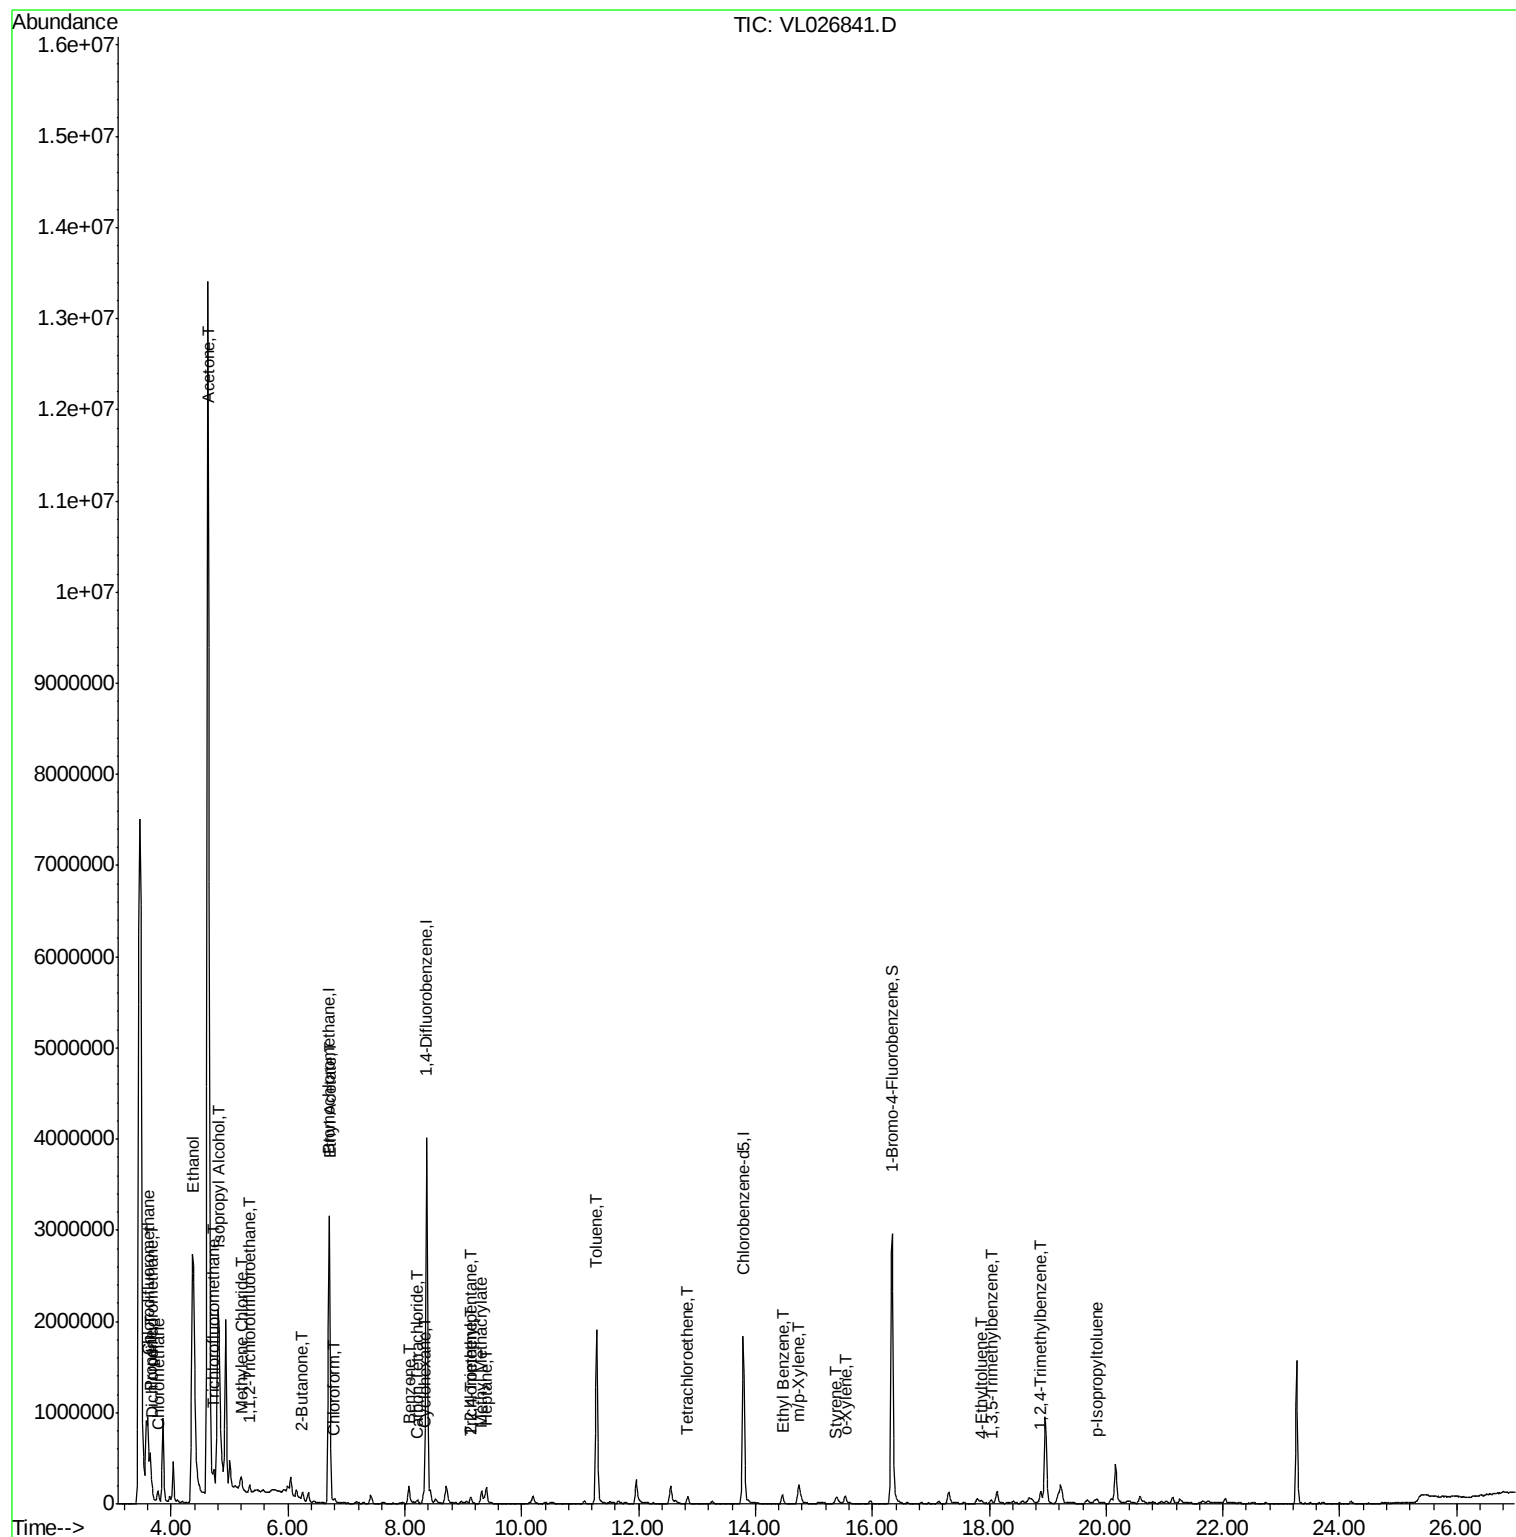

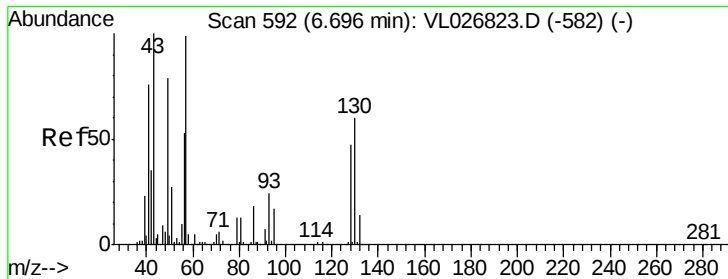

#1





Bromochloromethane
Concen: 10.00 ppbv
RT: 6.70 min Scan# 593
Delta R.T. 0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampleId :
IAS-2

Tot Ion: 49 Resp: 1334192
Ion Ratio Lower Upper
49 100
128 62.5 29.7 89.1
130 80.6 38.3 114.8

Manual Integrations
APPROVED




MMDadoda
2/11/2016 1:24:13 PM

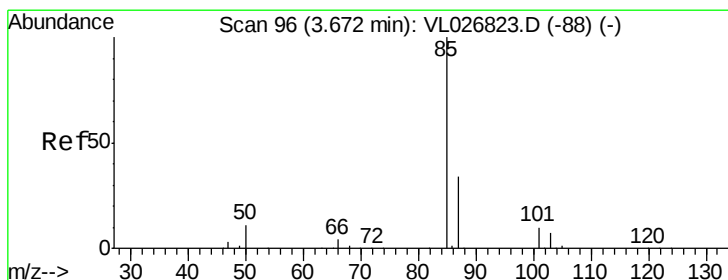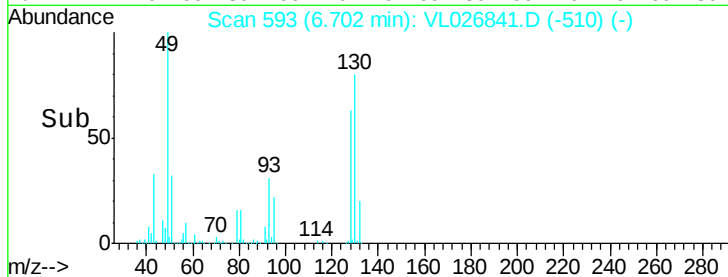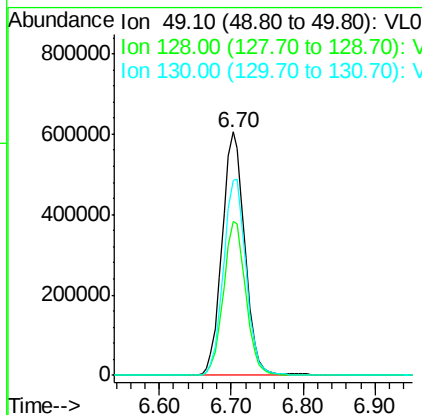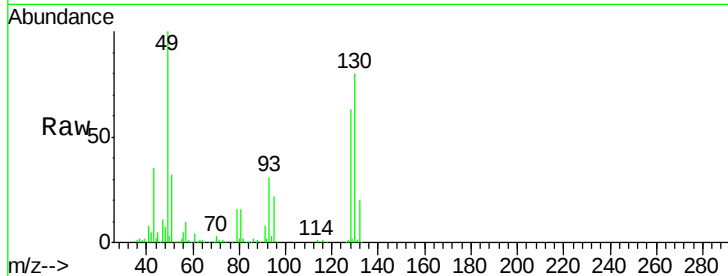


#2

Dichlorodifluoromethane
Concen: 0.64 ppbv
RT: 3.67 min Scan# 96
Delta R.T. -0.00 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion: 85 Resp: 183320
Ion Ratio Lower Upper
85 100
87 31.7 27.3 40.9

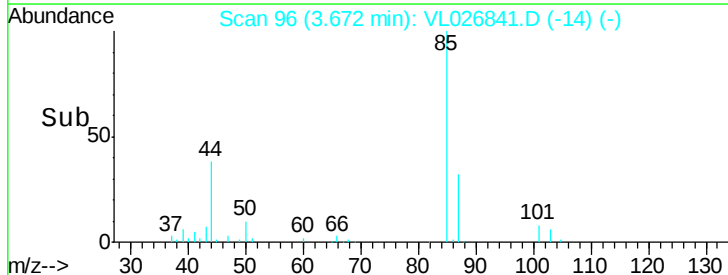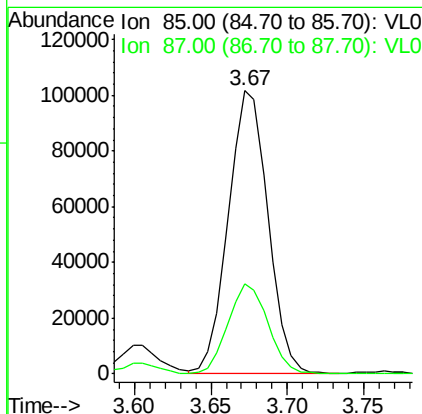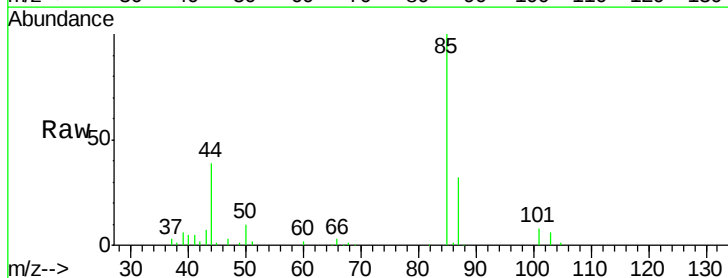

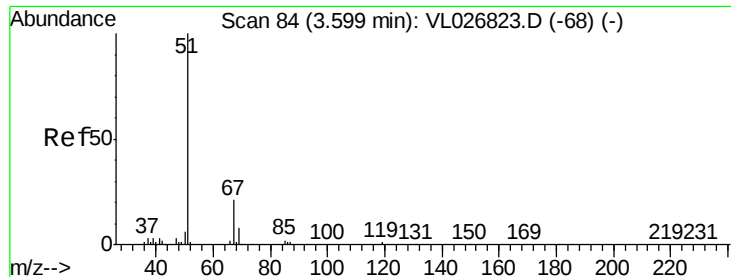

#3

Chlorodifluoromethane

Concen: 4.26 ppbv m

RT: 3.60 min Scan# 84

Delta R.T. -0.00 min

Lab File: VL026841.D

Acq: 10 Feb 2016 5:33

Tot Ion: 51 Resp: 921741

Ion Ratio Lower Upper

51 100

67 22.4 16.4 24.6

Instrument :

MSVOA_L


ClientSampled :

IAS-2

Manual Integrations
APPROVED

MMDadoda

2/11/2016 1:24:13 PM

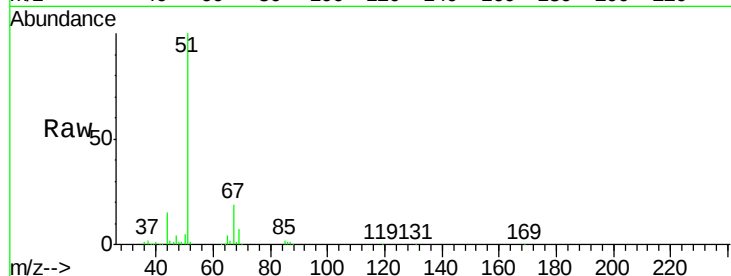

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

3.60

600000

500000

400000



300000

200000

100000

0

Time--> 3.55 3.60 3.65

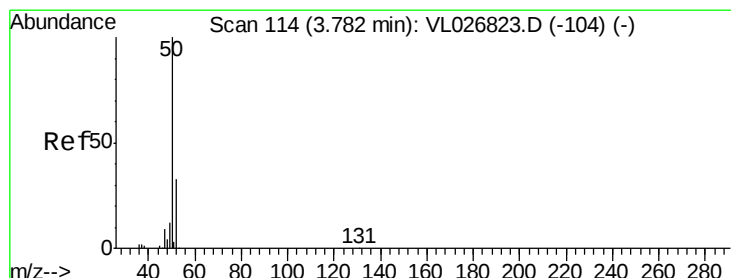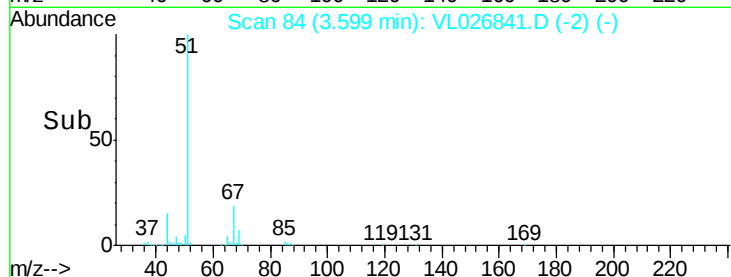

#4

Chloromethane

Concen: 0.70 ppbv

RT: 3.78 min Scan# 114

Delta R.T. -0.00 min

Lab File: VL026841.D


Acq: 10 Feb 2016 5:33

Tgt Ion: 50 Resp: 59609

Ion Ratio Lower Upper

50 100

52 31.4 26.3 39.5

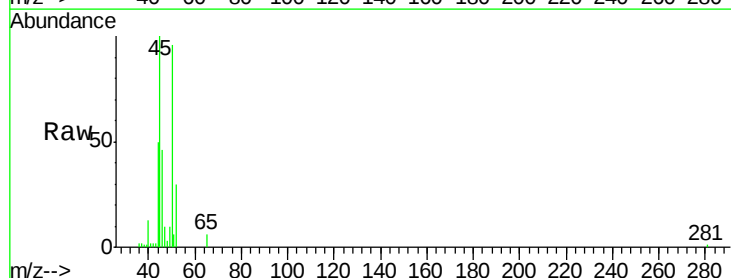

Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

3.78

30000

25000

20000


15000


10000

5000

0

Time--> 3.70 3.75 3.80 3.85

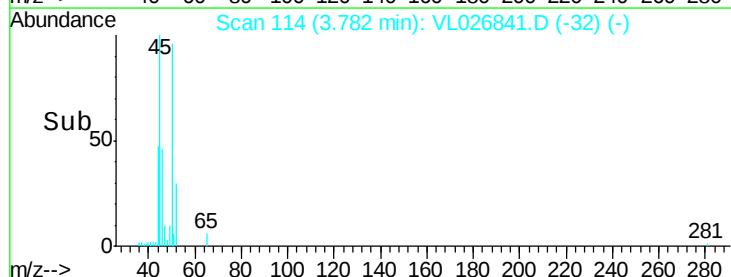

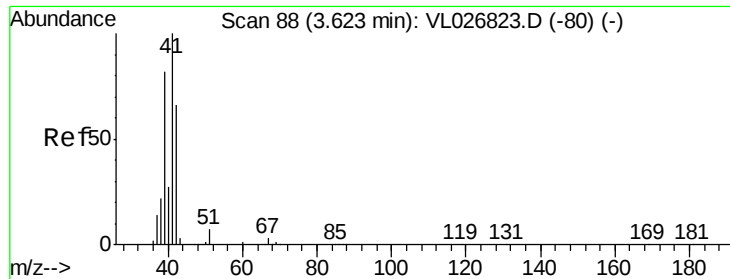

#9

Propene

Concen: 2.71 ppbv

RT: 3.64 min Scan# 90

Delta R.T. 0.01 min

Lab File: VL026841.D

Acq: 10 Feb 2016 5:33

Instrument :

MSVOA_L





ClientSampleId :

IAS-2

Tot Ion	Ratio	Lower	Upper
41	100		
42	46.1	52.8	79.2#

Manual Integrations
APPROVED

MMDadoda
2/11/2016 1:24:13 PM

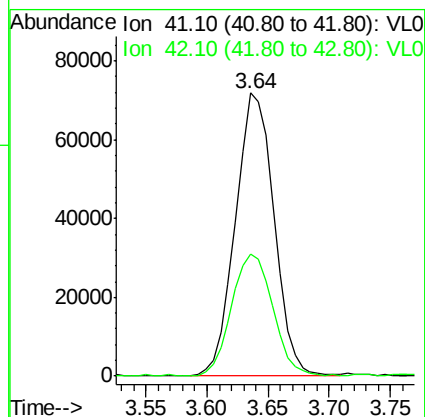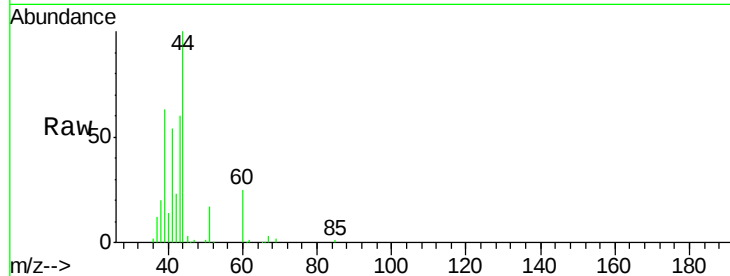

#10

Heptane

Concen: 0.47 ppbv




RT: 9.40 min Scan# 1035


Delta R.T. -0.01 min

Lab File: VL026841.D

Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
43	100		
57	42.3	44.0	66.0#

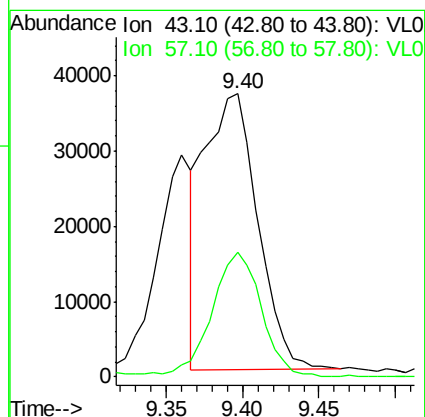







#11
 Trichlorofluoromethane
 Concen: 0.42 ppbv
 RT: 4.73 min Scan# 270
 Delta R.T. 0.01 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Instrument :
 MSVOA_L
 ClientSampleId :
 IAS-2

Tot Ion:101 Resp: 144765
 Ion Ratio Lower Upper
 101 100
 103 62.4 52.7 79.1




Manual Integrations
 APPROVED


MMDadoda
 2/11/2016 1:24:13 PM



#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.15 ppbv
 RT: 5.34 min Scan# 370
 Delta R.T. -0.00 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Tgt Ion:101 Resp: 36113
 Ion Ratio Lower Upper
 101 100
 151 90.8 69.4 104.0









#13
Ethanol
Concen: 626.88 ppbv
RT: 4.37 min Scan# 210
Delta R.T. 0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampleId :
IAS-2

Tot Ion: 45 Resp: 6304623
Ion Ratio Lower Upper
45 100
46 40.8 15.8 63.4




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

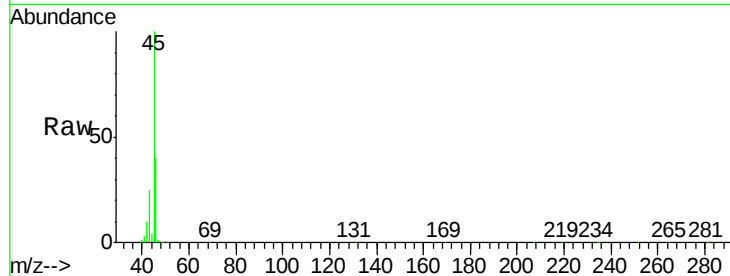

#15
Acetone
Concen: 97.77 ppbv
RT: 4.63 min Scan# 253
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion: 43 Resp: 17920261
Ion Ratio Lower Upper
43 100
58 51.6 25.2 37.8#



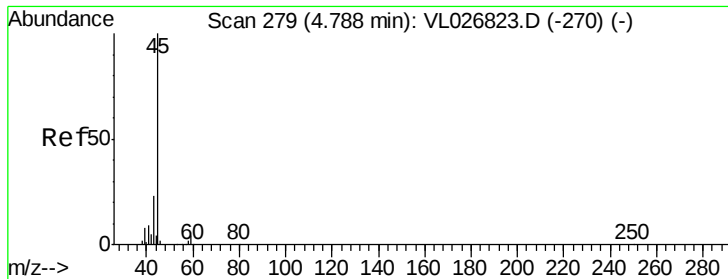

#19





Isopropyl Alcohol
 Concen: 73.51 ppbv
 RT: 4.81 min Scan# 282
 Delta R.T. 0.02 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Instrument :
 MSVOA_L
 ClientSampleID :
 IAS-2

Tot Ion: 45 Resp: 4806684
 Ion Ratio Lower Upper
 45 100
 58 0.0 2.2 3.2#

Manual Integrations
 APPROVED




MMDadoda
 2/11/2016 1:24:13 PM

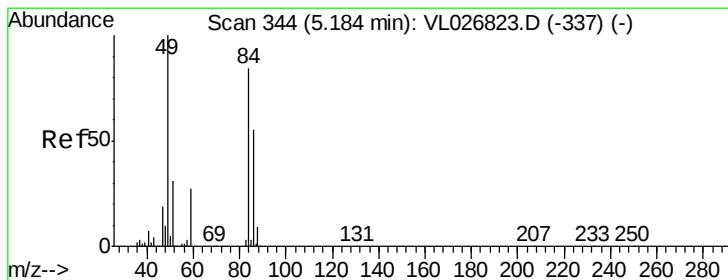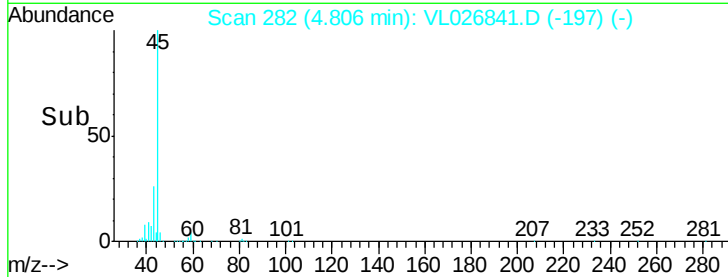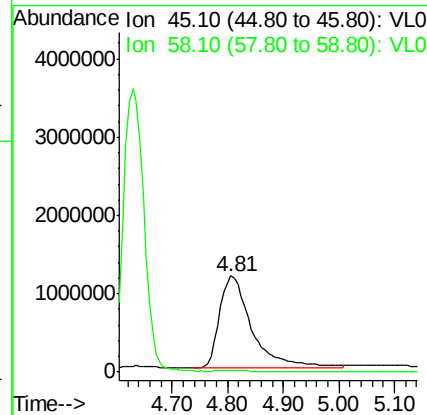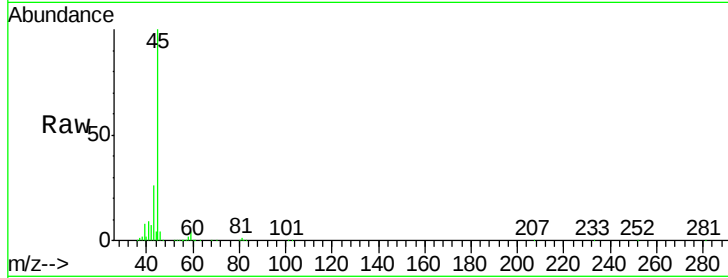


#20

Methylene Chloride
 Concen: 0.61 ppbv
 RT: 5.20 min Scan# 346
 Delta R.T. 0.01 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Tgt Ion: 84 Resp: 57988
 Ion Ratio Lower Upper
 84 100
 49 115.5 94.9 142.3
 51 34.9 29.5 44.3
 86 67.2 51.9 77.9

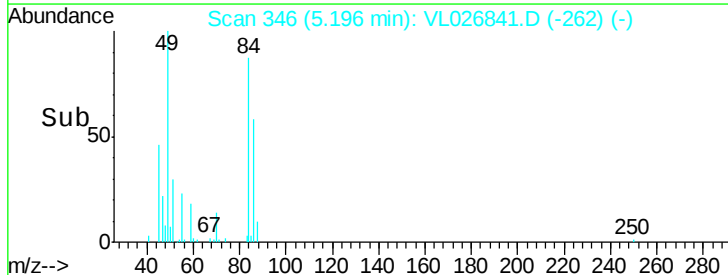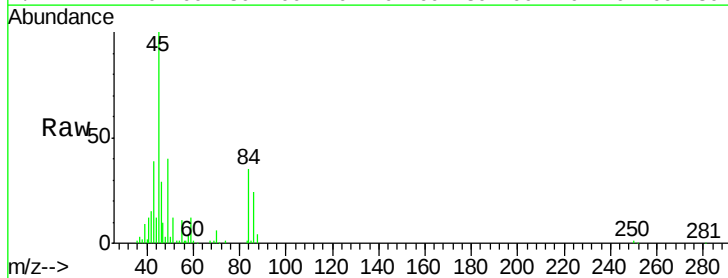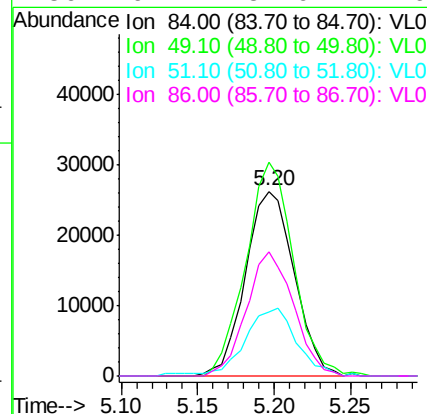



#25

Ethyl Acetate

Concen: 2.33 ppbv

RT: 6.71 min Scan# 595

Delta R.T. -0.00 min

Lab File: VL026841.D

Acq: 10 Feb 2016 5:33

Instrument :

MSVOA_L


ClientSampleId :

IAS-2




Tot Ion:	43	Resp:	641222
Ion Ratio	Lower	Upper	
43	100		
45	13.8	7.8	11.8#
61	12.4	7.9	11.9#
70	9.8	6.9	10.3

Manual Integrations
APPROVED

MMDadoda
2/11/2016 1:24:13 PM



Abundance Ion 43.10 (42.80 to 43.80): VL0
Ion 45.10 (44.80 to 45.80): VL0
Ion 61.10 (60.80 to 61.80): VL0
Ion 70.10 (69.80 to 70.80): VL0

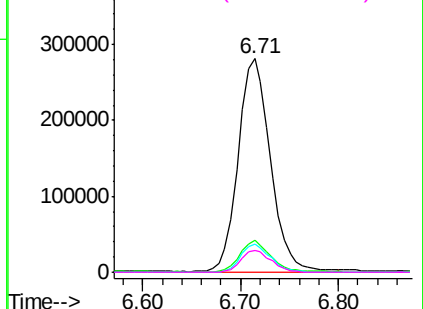

#29

Chloroform

Concen: 0.12 ppbv


RT: 6.79 min Scan# 608

Delta R.T. -0.00 min



Lab File: VL026841.D


Acq: 10 Feb 2016 5:33

Tgt Ion:	83	Resp:	29142
Ion Ratio	Lower	Upper	
83	100		
85	57.9	51.5	77.3



Abundance Ion 83.00 (82.70 to 83.70): VL0
Ion 85.00 (84.70 to 85.70): VL0

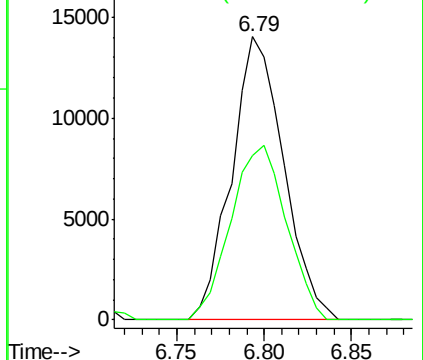







#30
Cvclohexane
Concen: 0.30 ppbv m
RT: 8.32 min Scan# 859
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampleId :
IAS-2

Tot Ion	Ratio	Lower	Upper
84	100		
56	407.9	99.4	149.2#
41	102.4	56.7	85.1#




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

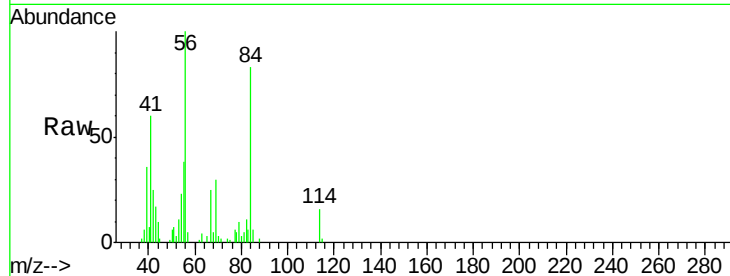

#33
1,4-Difluorobenzene
Concen: 10.00 ppbv
RT: 8.37 min Scan# 867
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
114	100		
63	22.3	19.7	29.5
88	16.5	13.8	20.6









#34
2-Butanone
Concen: 0.72 ppbv
RT: 6.24 min Scan# 518
Delta R.T. -0.00 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampleId :
IAS-2

Tot Ion	43	Resp	129343
Ion Ratio	Lower	Upper	
43	100		
72	25.7	19.8	29.8




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

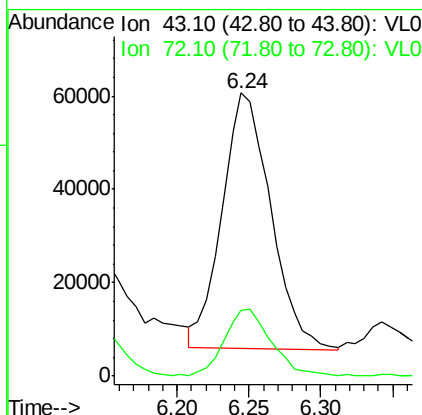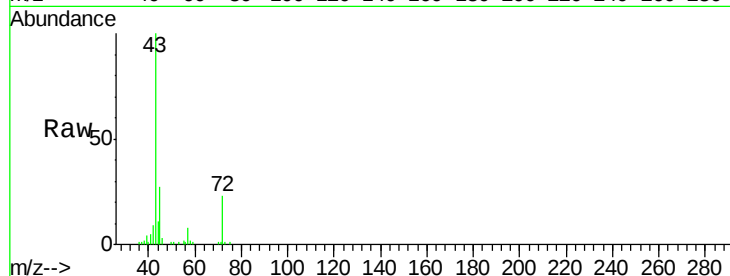

#35
Carbon Tetrachloride
Concen: 0.10 ppbv
RT: 8.21 min Scan# 840
Delta R.T. -0.00 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion	117	Resp	25770
Ion Ratio	Lower	Upper	
117	100		
119	98.1	76.6	115.0
121	32.7	25.0	37.4





#36

Benzene

Concen: 0.69 ppbv

RT: 8.07 min Scan# 818

Delta R.T. -0.00 min

Lab File: VL026841.D

Acq: 10 Feb 2016 5:33

Instrument :

MSVOA_L





ClientSampleId :

IAS-2

Tot Ion:	78	Resp:	202486
Ion Ratio	Lower	Upper	
78	100		
77	22.3	19.0	28.6
50	14.0	14.2	21.4#

Manual Integrations
APPROVED

MMDadoda
2/11/2016 1:24:13 PM

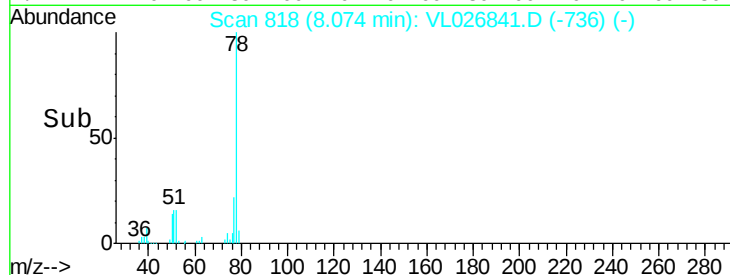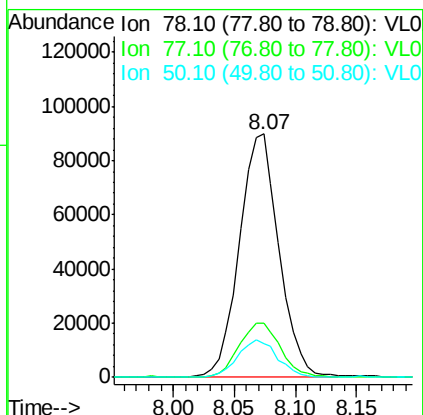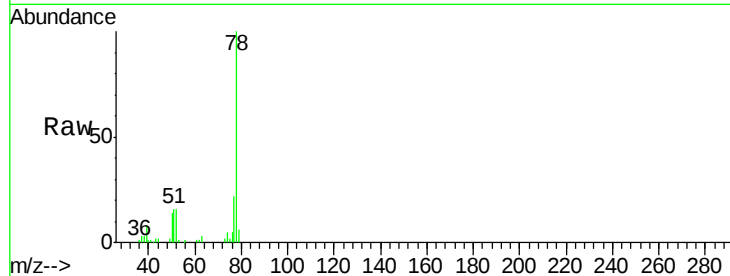

#38

Trichloroethene

Concen: 0.03 ppbv




RT: 9.12 min Scan# 989


Delta R.T. -0.00 min

Lab File: VL026841.D

Acq: 10 Feb 2016 5:33

Tgt Ion:	130	Resp:	4285
Ion Ratio	Lower	Upper	
130	100		
95	88.4	83.0	124.6
132	80.0	76.0	114.0
97	66.0	54.0	81.0

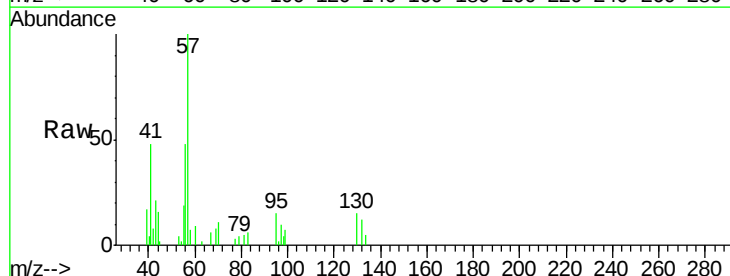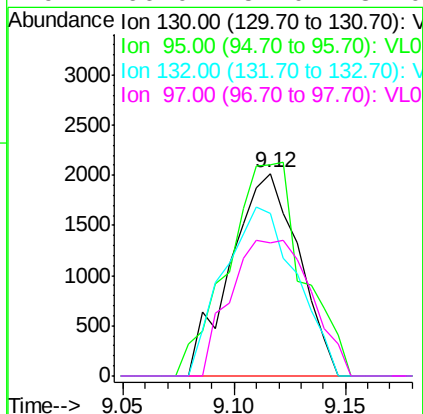







#43
Methvl Methacrylate
Concen: 0.70 ppbv
RT: 9.31 min Scan# 1021
Delta R.T. -0.00 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampled :
IAS-2

Tot Ion	Ratio	Lower	Upper
69	100		
41	126.0	106.5	159.7
100	34.2	27.2	40.8




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM



#44
2,2,4-Trimethylpentane
Concen: 0.10 ppbv
RT: 9.13 min Scan# 991
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
57	100		
41	43.2	23.2	34.8#
56	51.3	26.2	39.4#









#52
Tetrachloroethene
Concen: 0.22 ppbv
RT: 12.84 min Scan# 1600
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampleId :
IAS-2

Tot Ion	Ratio	Lower	Upper
164	100		
166	122.6	100.3	150.5
129	93.2	80.0	120.0
131	99.2	76.7	115.1




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

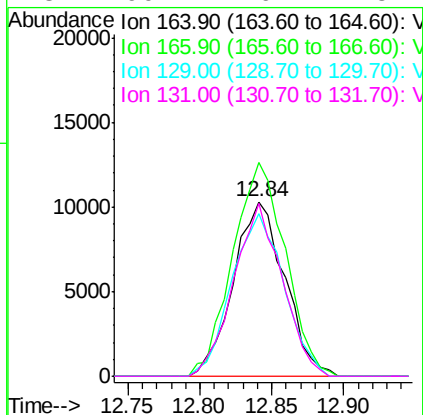

#53
Toluene
Concen: 5.43 ppbv
RT: 11.28 min Scan# 1344
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
91	100		
92	58.7	47.3	70.9

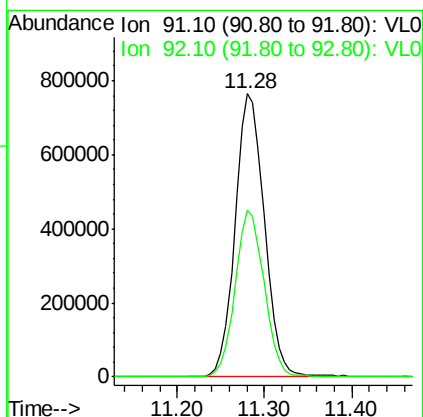







#55
Chlorobenzene-d5
Concen: 10.00 ppbv
RT: 13.79 min Scan# 1756
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampled :
IAS-2

Tot Ion	Ratio	Lower	Upper
117	100		
82	60.7	51.9	77.9
119	32.5	48.5	72.7#




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

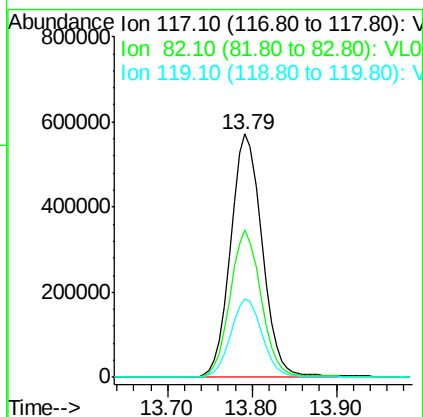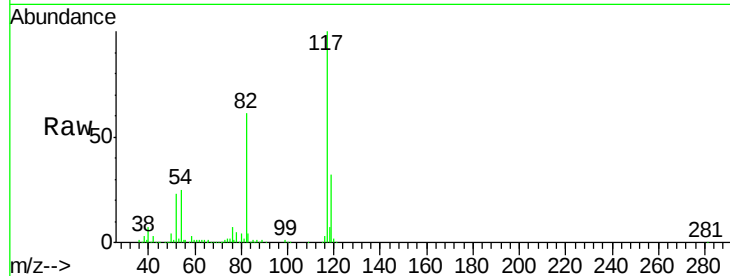

#58
Ethyl Benzene
Concen: 0.59 ppbv
RT: 14.46 min Scan# 1865
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
91	100		
106	30.1	24.9	37.3

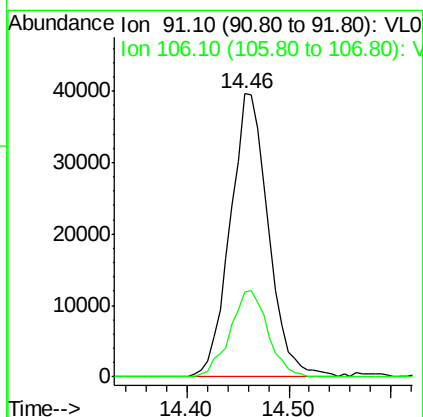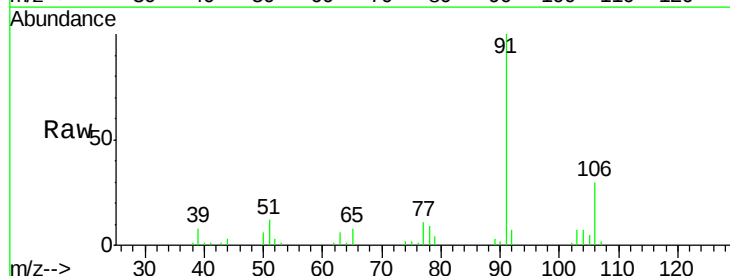







#59
m/p-Xylene
Concen: 1.72 ppbv
RT: 14.74 min Scan# 1911
Delta R.T. -0.04 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampled :
IAS-2

Tot Ion: 91 Resp: 258073
Ion Ratio Lower Upper
91 100
106 47.0 38.2 57.2




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

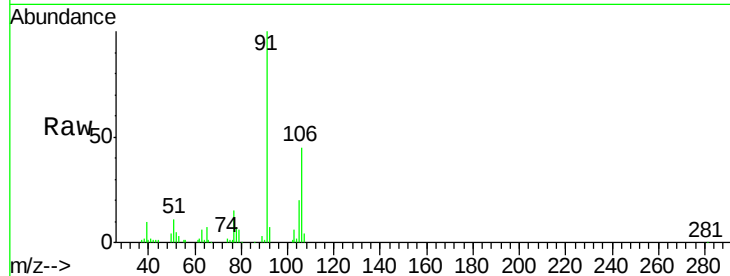

#60
o-Xylene
Concen: 0.48 ppbv
RT: 15.54 min Scan# 2042
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion: 91 Resp: 78301
Ion Ratio Lower Upper
91 100
106 45.7 22.3 66.8



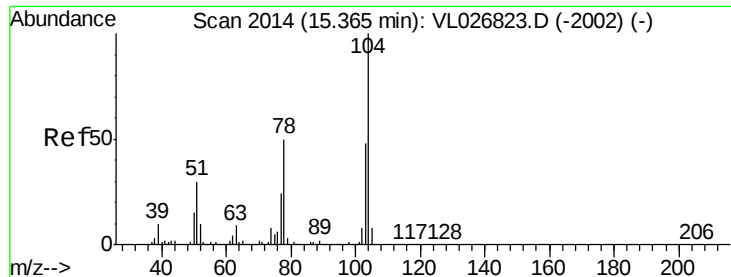





#61
Stvrene
Concen: 0.33 ppbv
RT: 15.36 min Scan# 2013
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Instrument :
MSVOA_L
ClientSampled :
IAS-2

Tot Ion	Ratio	Lower	Upper
104	100		
78	49.0	39.8	59.6
103	48.9	38.2	57.4




Manual Integrations
APPROVED


MMDadoda
2/11/2016 1:24:13 PM

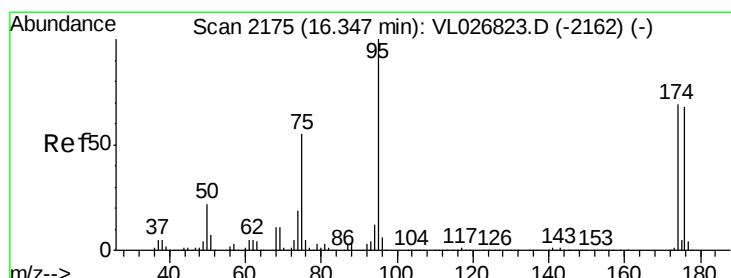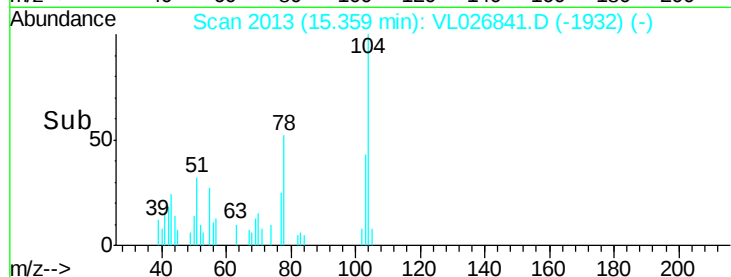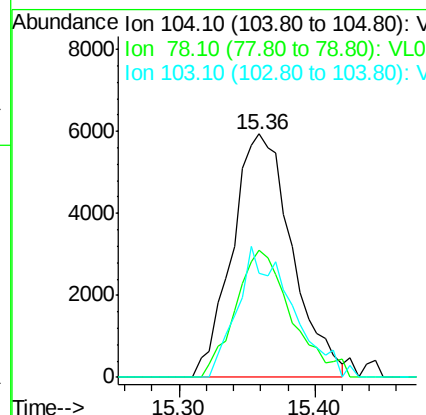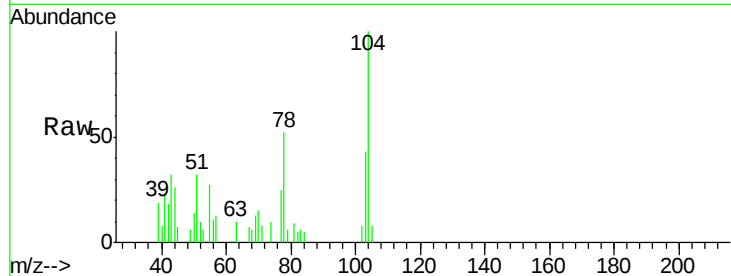

#68
1-Bromo-4-Fluorobenzene
Concen: 15.72 ppbv
RT: 16.33 min Scan# 2173
Delta R.T. -0.01 min
Lab File: VL026841.D
Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
95	100		
174	73.5	55.6	83.4
175	4.9	3.9	5.9

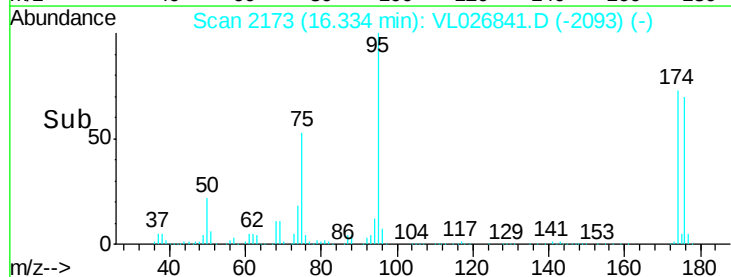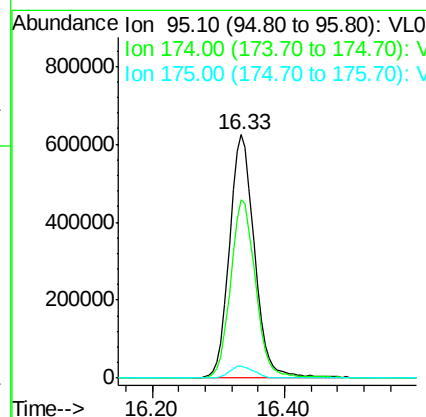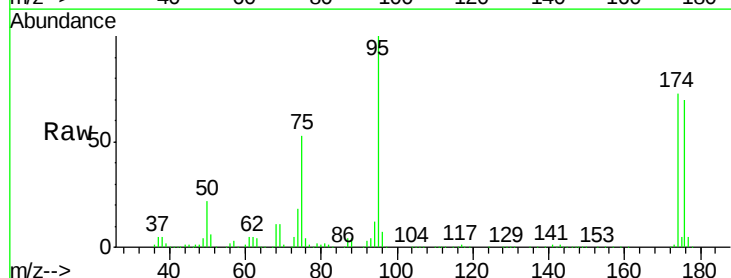

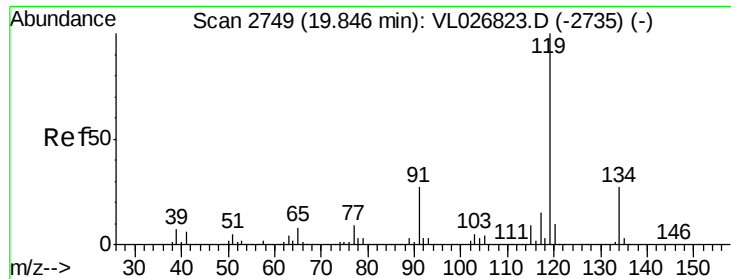





#69
 p-Isopropyltoluene
 Concen: 0.13 ppbv
 RT: 19.84 min Scan# 2748
 Delta R.T. -0.01 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Instrument :
 MSVOA_L
 ClientSampled :
 IAS-2

Tot Ion	Ratio	Resp	Lower	Upper
119	100	24969		
134	22.0		21.3	31.9
91	48.3		21.5	32.3#




Manual Integrations
 APPROVED


MMDadoda
 2/11/2016 1:24:13 PM

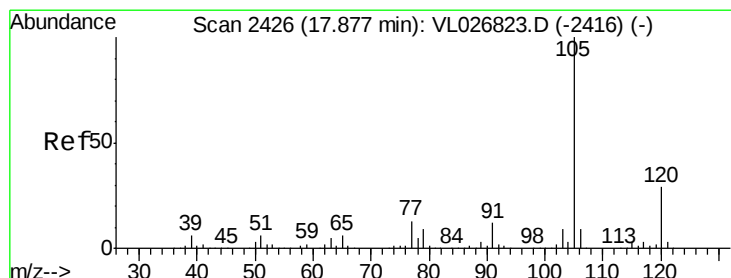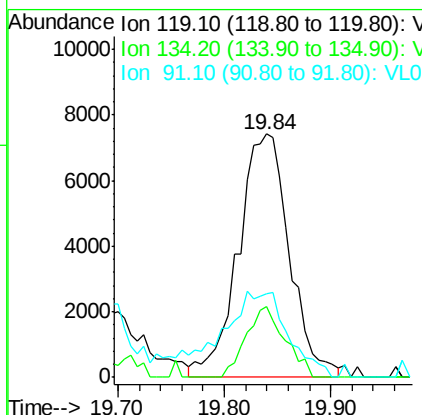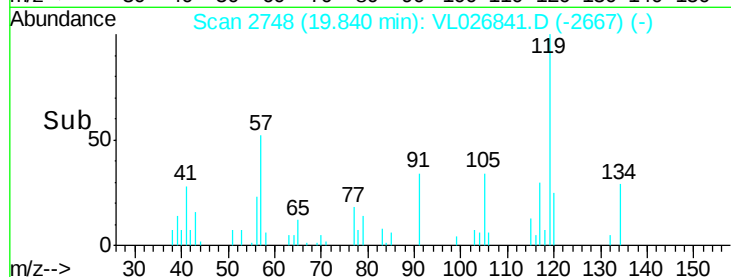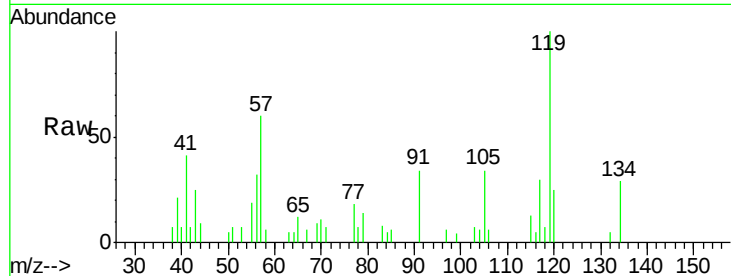

#72
 4-Ethyltoluene
 Concen: 0.22 ppbv
 RT: 17.87 min Scan# 2425
 Delta R.T. -0.01 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Resp	Lower	Upper
105	100	32995		
120	31.0		23.8	35.6
91	20.1		10.2	15.4#
77	12.7		10.8	16.2

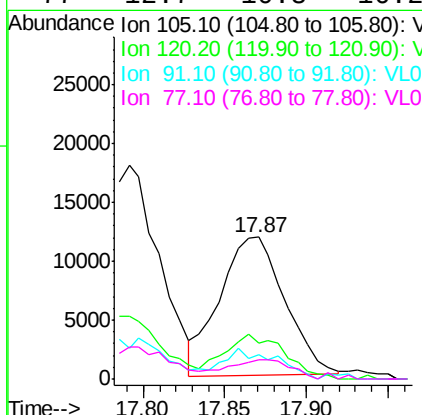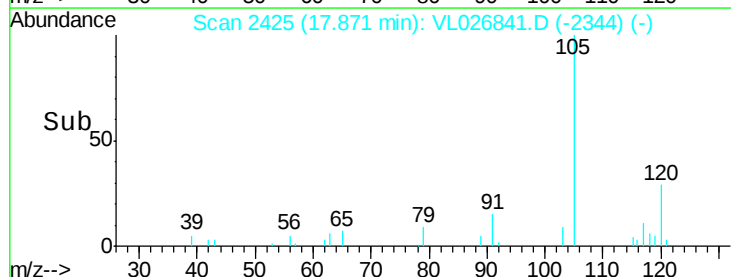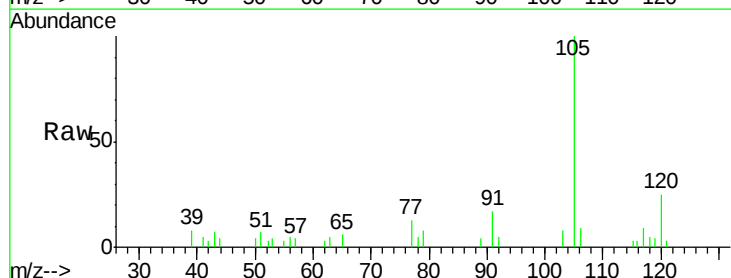

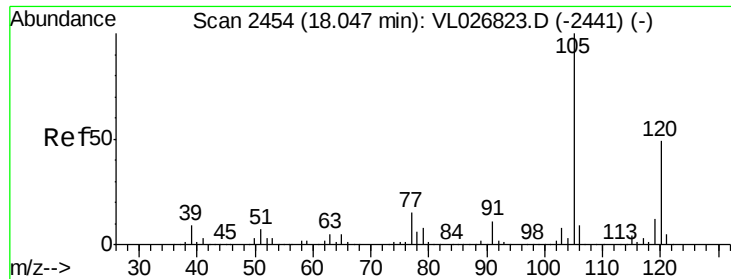





#73
 1,3,5-Trimethylbenzene
 Concen: 0.20 ppbv
 RT: 18.04 min Scan# 2452
 Delta R.T. -0.01 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Instrument :
 MSVOA_L
 ClientSampleId :
 IAS-2

Tot Ion	Ratio	Lower	Upper
105	100		
120	42.0	39.4	59.0

Manual Integrations
 APPROVED

MMDadoda
 2/11/2016 1:24:13 PM

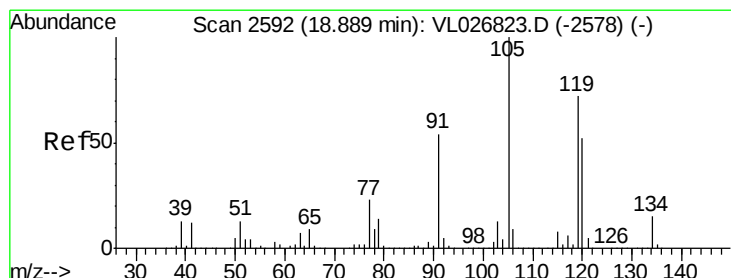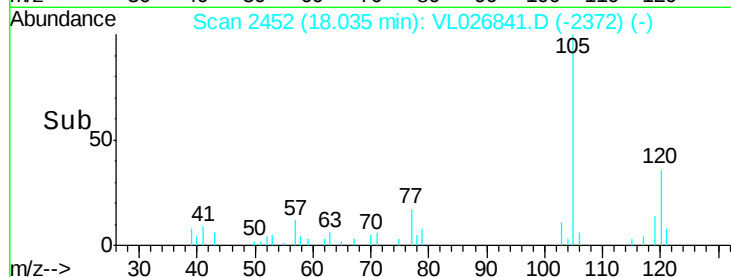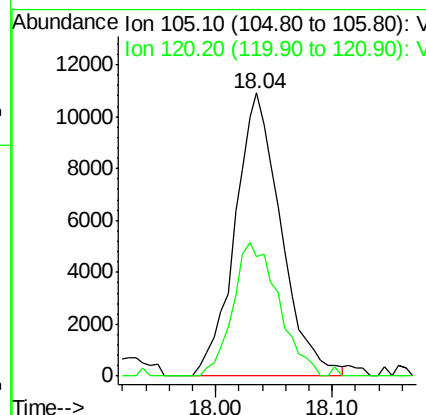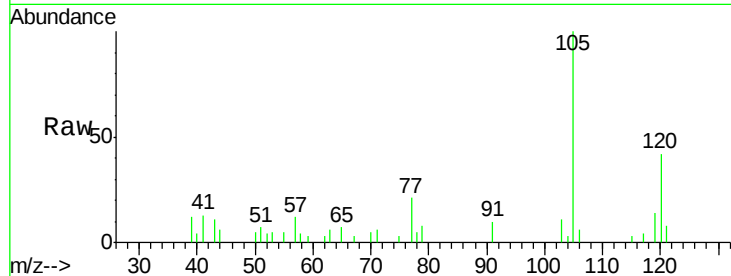

#74
 1,2,4-Trimethylbenzene
 Concen: 0.67 ppbv
 RT: 18.88 min Scan# 2591
 Delta R.T. -0.01 min
 Lab File: VL026841.D
 Acq: 10 Feb 2016 5:33

Tgt Ion	Ratio	Lower	Upper
105	100		
120	45.3	41.3	61.9
91	12.8	43.3	64.9#
77	12.8	18.3	27.5#

