


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL020916\
Data File : VL026822.D
Acq On : 9 Feb 2016 16:15
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL020916AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Feb 10 03:14:04 2016
Last Update : Wed Feb 10 03:14:04 2016

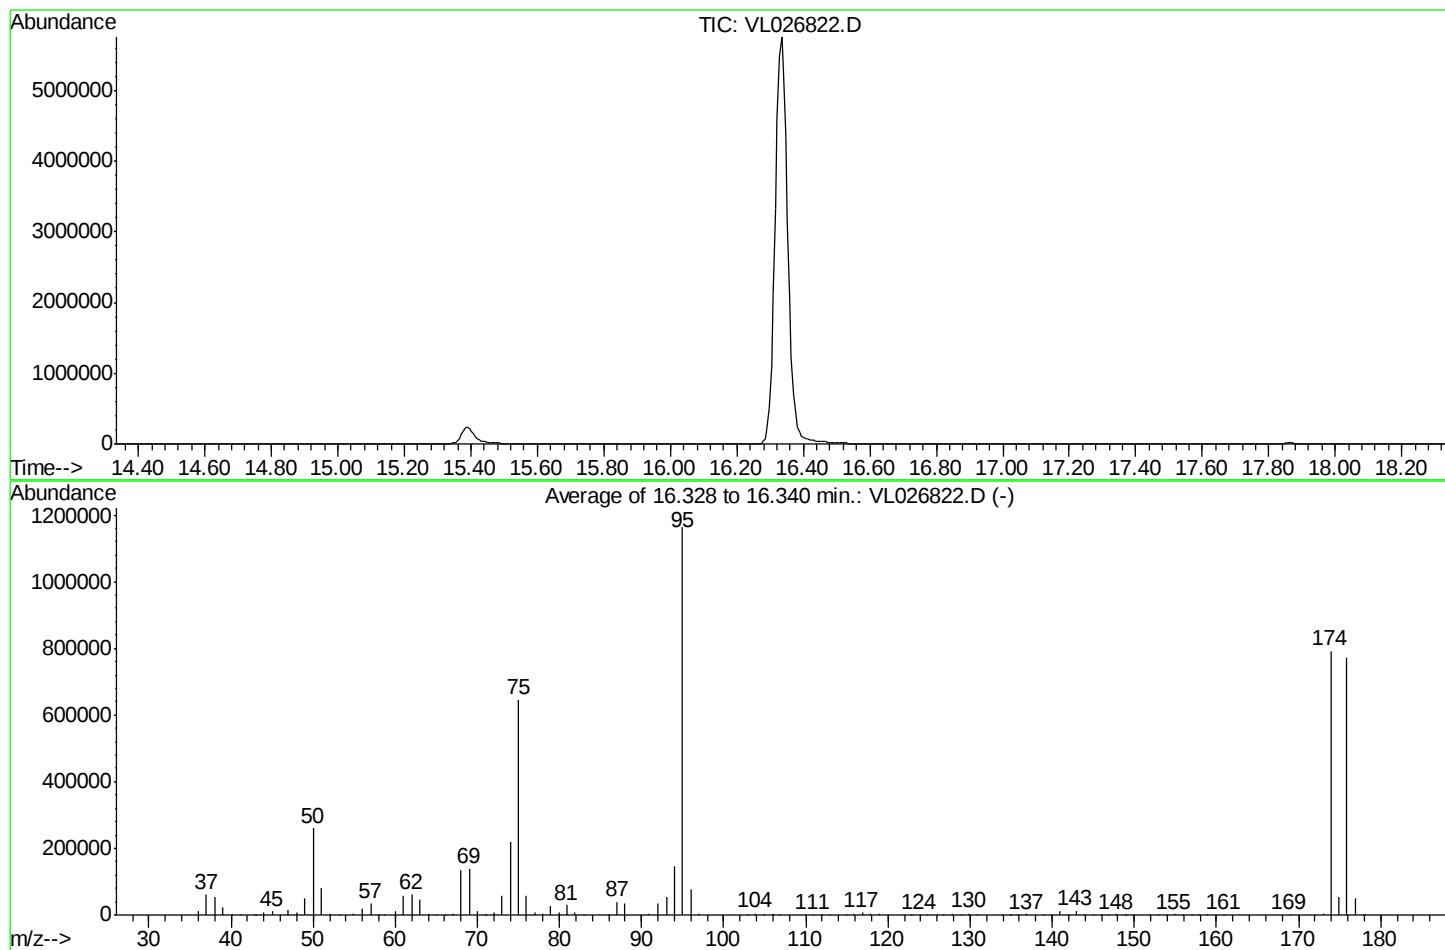

AutoFind: Scans 2172, 2173, 2174; Background Corrected with Scan 2157

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.4	260864	PASS
75	95	30	66	55.6	646890	PASS
95	95	100	100	100.0	1163264	PASS
96	95	5	9	6.6	76301	PASS
173	174	0.00	2	0.7	5390	PASS
174	95	50	120	68.1	792725	PASS
175	174	4	9	7.0	55861	PASS
176	174	93	101	97.5	773034	PASS
177	176	5	9	6.5	50002	PASS