
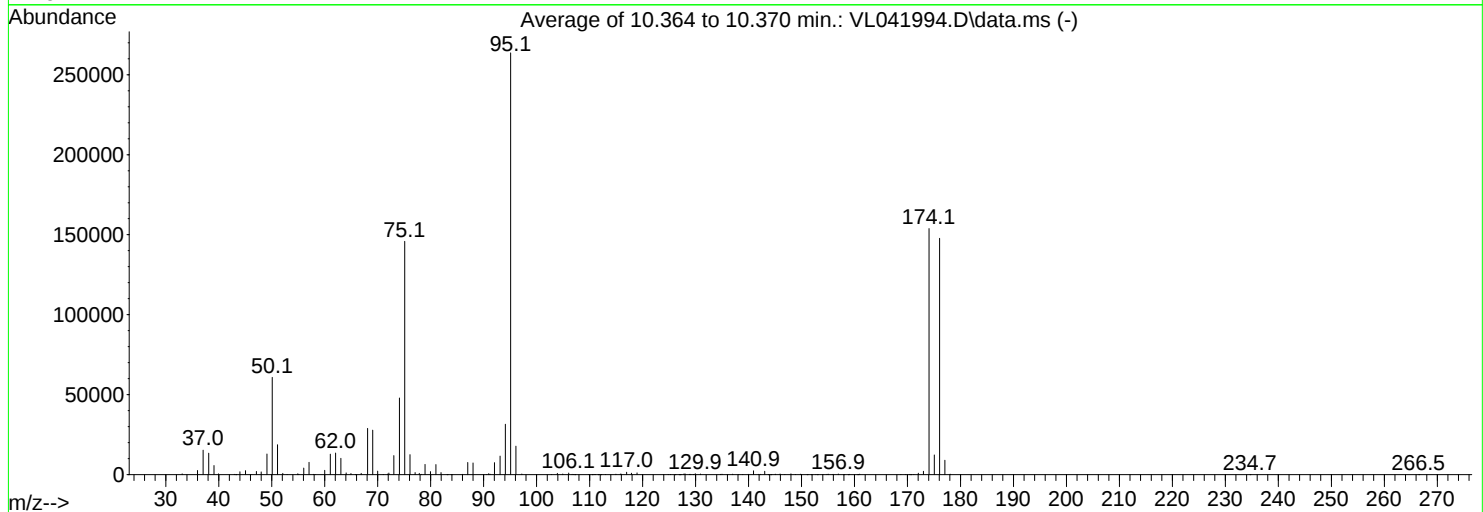


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021125\
Data File : VL041994.D
Acq On : 11 Feb 2025 08:38
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 14 23:15:42 2025

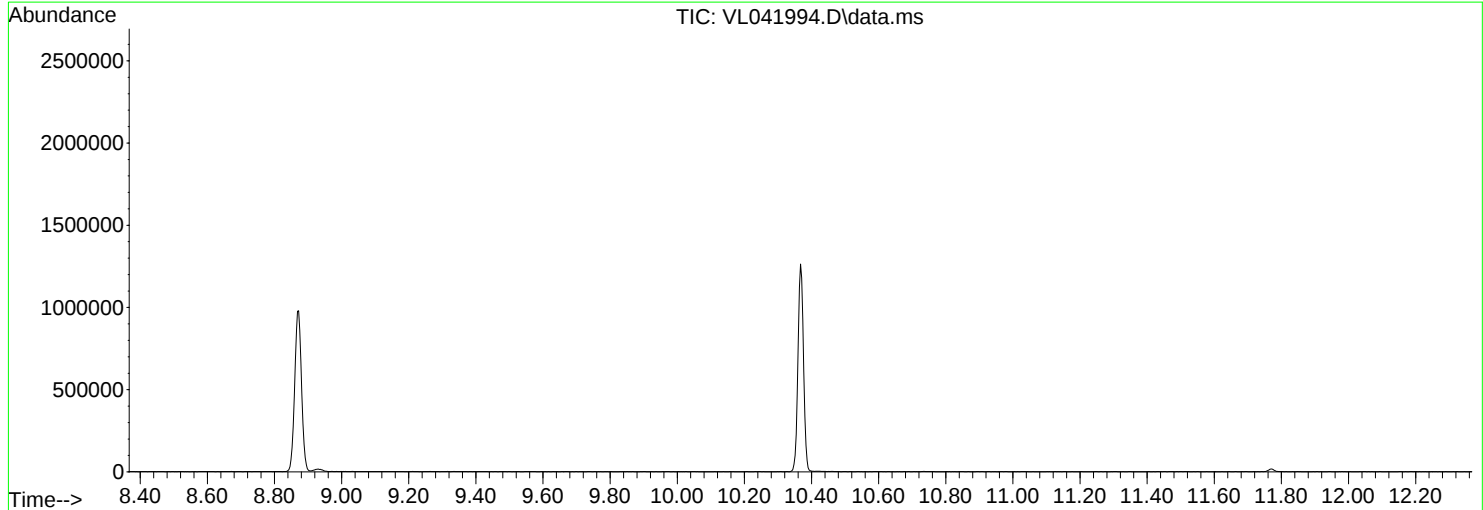

AutoFind: Scans 3175, 3176, 3177; Background Corrected with Scan 3153

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.1	60800	PASS
75	95	30	66	55.3	145813	PASS
95	95	100	100	100.0	263701	PASS
96	95	5	9	6.8	17853	PASS
173	174	0.00	2	1.4	2101	PASS
174	95	50	120	58.4	153877	PASS
175	174	4	9	8.0	12298	PASS
176	174	93	101	96.0	147797	PASS
177	176	5	9	6.1	8993	PASS

Average of 10.364 to 10.370 min.: VL041994.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	554	47.10	2025	57.90	190	68.10	2891
36.00	2562	48.00	1713	58.20	104	69.05	2777
37.05	15267	49.10	12910	60.00	2691	70.00	222
38.10	13414	50.10	60800	61.05	12782	71.05	7
39.10	5676	51.10	18693	62.05	13525	71.90	424
39.95	478	52.10	857	63.05	10202	72.10	1035
42.95	184	52.90	78	64.05	1152	73.05	11946
43.20	32	54.90	550	64.95	692	74.10	47901
44.00	1806	55.10	328	65.80	35	75.10	145813
45.05	2512	56.05	4067	66.05	128	76.10	12517
46.05	159	57.05	7674	66.90	833	77.05	1353

Average of 10.364 to 10.370 min.: VL041994.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.85	831	90.60	92	104.95	411	112.10	63
78.20	204	90.95	568	106.05	976	113.00	159
78.95	6416	91.20	273	106.70	172	114.95	352
79.95	1918	92.05	7528	107.00	67	115.80	372
81.00	6288	93.10	11606	107.20	58	116.00	327
81.95	1279	94.10	31504	109.85	83	117.00	1543
83.10	43	95.10	263701	110.50	57	117.90	956
83.90	28	96.10	17853	110.90	83	118.95	1131
86.00	188	97.20	379	111.10	82	123.95	143
87.00	7614	102.80	110	111.60	28	124.85	126
88.00	7294	103.90	833	111.80	104	125.25	70

Average of 10.364 to 10.370 min.: VL041994.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.10	18	135.00	346	144.20	17	154.05	106
126.90	33	136.05	125	145.05	256	154.80	163
127.10	41	137.00	320	145.95	395	155.05	327
127.80	421	138.15	69	146.85	154	155.95	169
128.00	525	138.90	145	148.00	500	156.95	433
128.85	222	140.00	186	148.85	158	157.90	25
129.10	168	140.95	2379	149.85	267	158.15	115
129.60	150	141.90	218	151.05	63	158.80	58
129.95	653	142.20	175	151.85	53	159.00	197
130.95	458	143.05	2130	152.70	65	160.60	40
134.70	162	143.70	29	153.00	54	161.00	299

Average of 10.364 to 10.370 min.: VL041994.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
168.75	91	178.05	274				
169.65	70	234.65	57				
170.40	90	266.50	29				
170.60	35						
171.20	153						
172.05	926						
173.00	2101						
174.05	153877						
175.05	12298						
176.05	147797						
177.05	8993						

Instrument :

MSVOA_L

ClientSampleId :

BFB