


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL021419\
 Data File : VL033199.D
 Acq On : 14 Feb 2019 14:11
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL020519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 06 09:13:11 2019
 Last Update : Wed Feb 06 09:13:11 2019

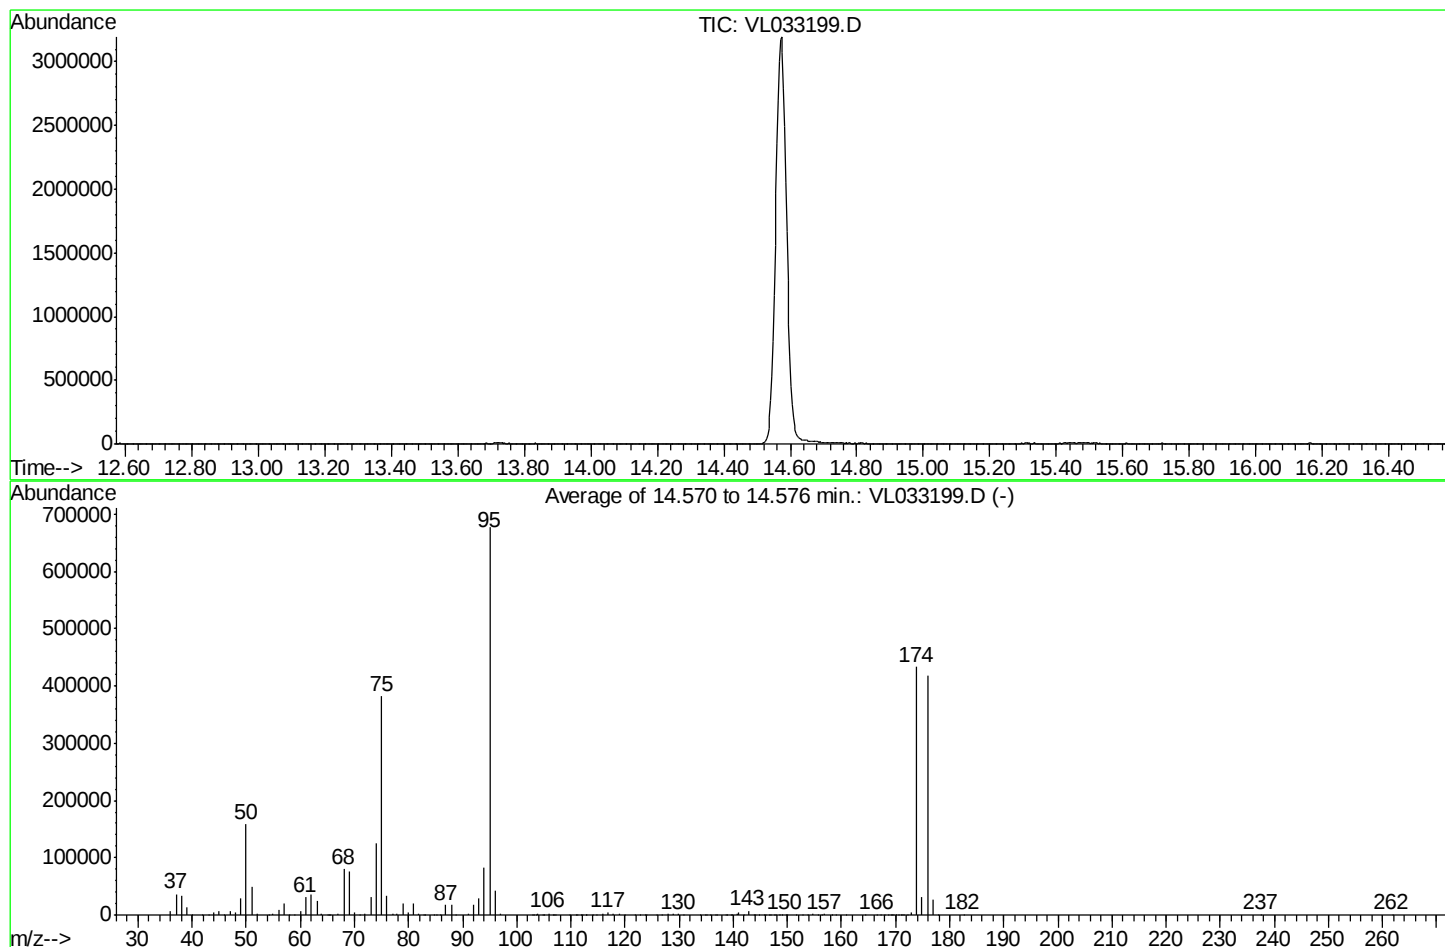

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	158314	PASS
75	95	30	66	56.4	381674	PASS
95	95	100	100	100.0	676970	PASS
96	95	5	9	6.4	43242	PASS
173	174	0.00	2	1.2	5213	PASS
174	95	50	120	64.0	433280	PASS
175	174	4	9	7.0	30368	PASS
176	174	93	101	96.5	418304	PASS
177	176	5	9	6.2	26039	PASS