

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL021419\
 Data File : VL033201.D
 Acq On : 14 Feb 2019 16:23
 Operator : SY/AP
 Sample : VL0214ABL01
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 08:21:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL020519AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Feb 20 06:00:52 2019
 QLast Update : Wed Feb 20 06:00:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	924233	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.28	114	2115108	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.24	117	2135774m	10.00	ppbv	0.00

System Monitoring Compounds


68) 1-Bromo-4-Fluorobenzene	14.57	95	1739301	10.45	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.50%


Target Compounds					Ovalue
15) Acetone	3.92	43	21521m	0.207	ppbv
20) Methylene Chloride	4.41	84	9249	0.223	ppbv # 86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL021419\
Data File : VL033201.D
Acq On : 14 Feb 2019 16:23
Operator : SY/AP
Sample : VL0214ABL01
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 08:21:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL020519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Feb 20 06:00:52 2019
QLast Update : Wed Feb 20 06:00:52 2019
Response via : Initial Calibration

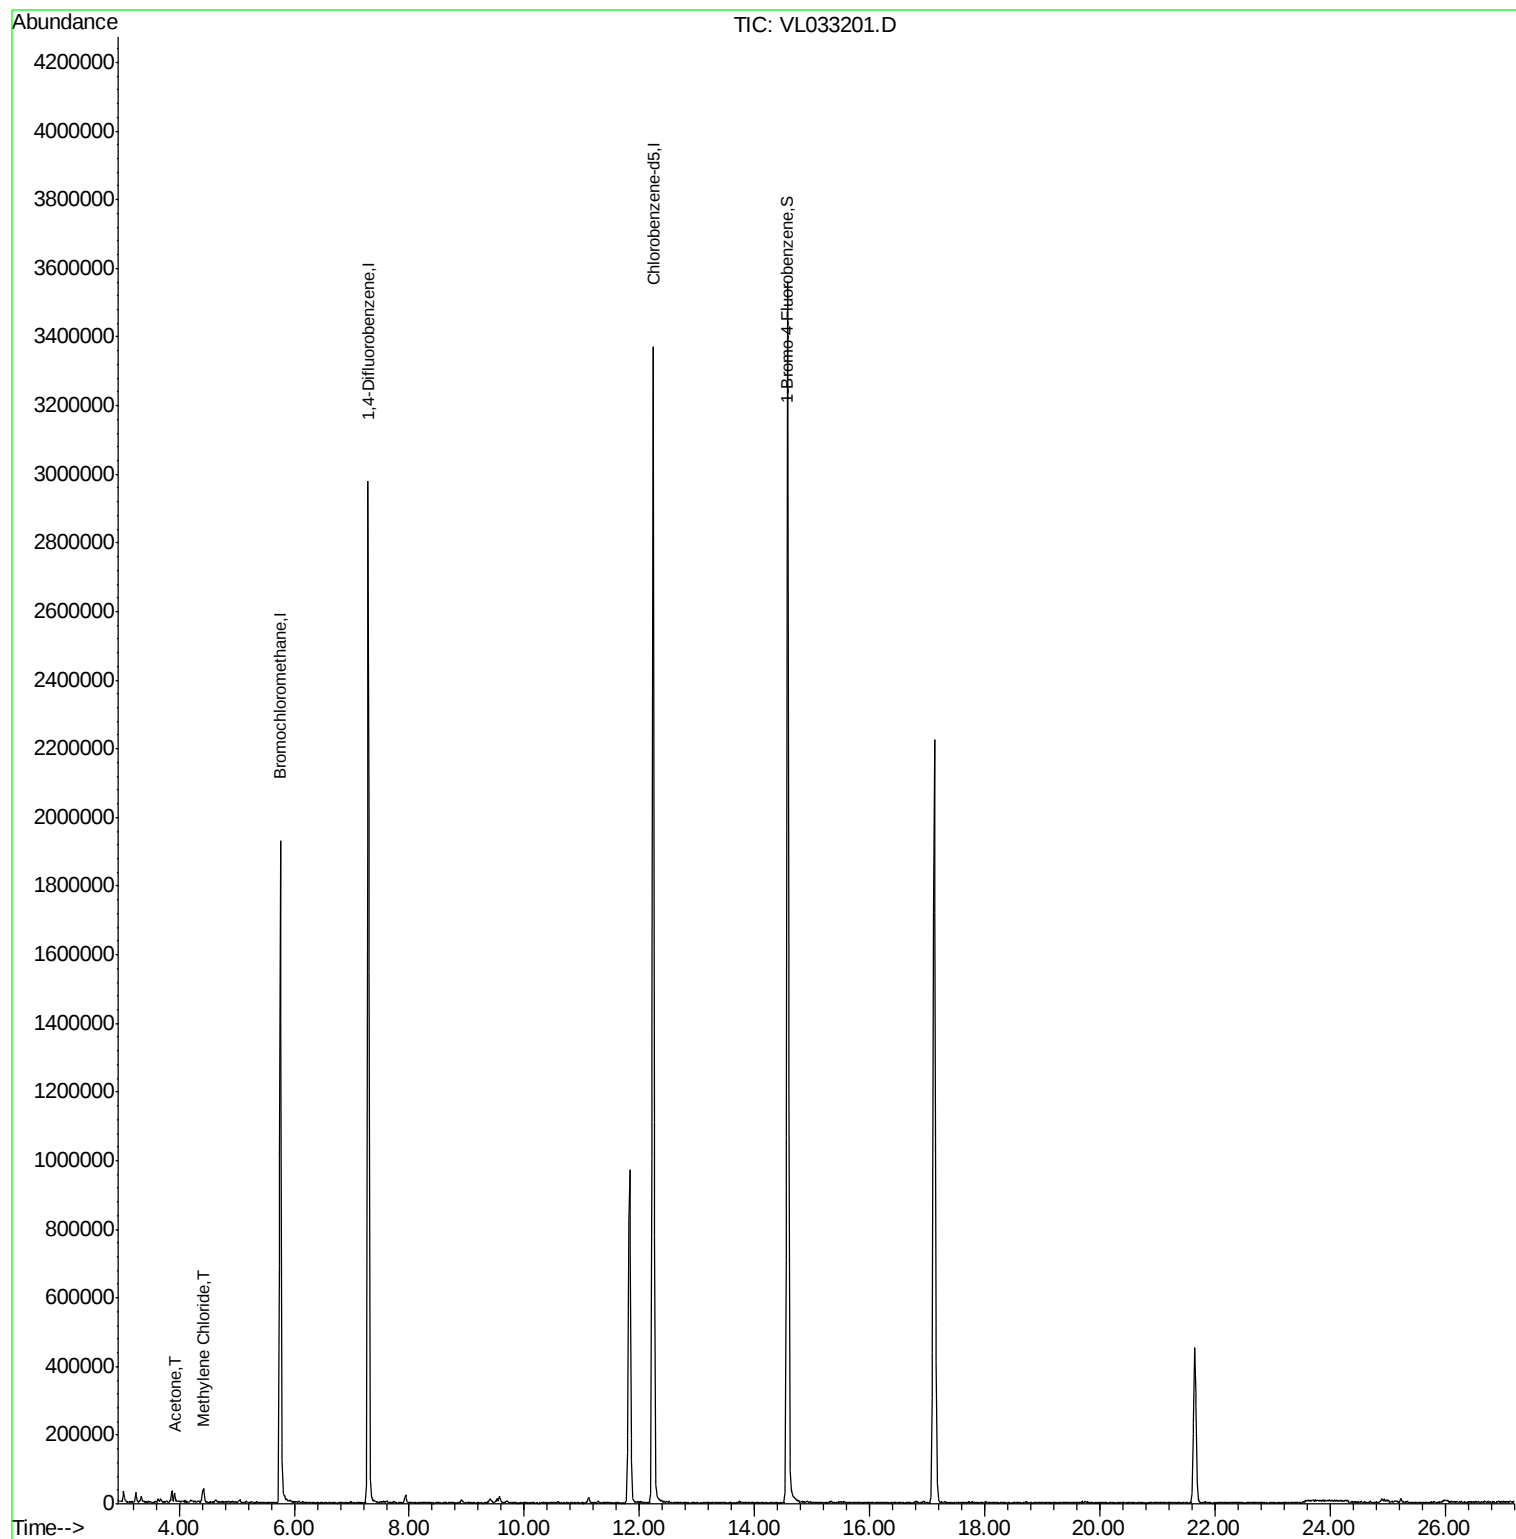

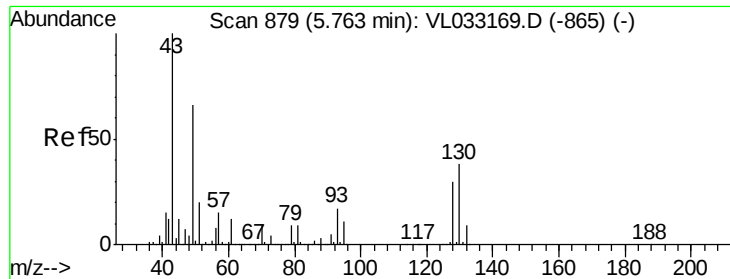

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 877

Delta R.T. -0.01 min

Lab File: VL033201.D

Acq: 14 Feb 2019 16:23


Tot Ion: 49 Resp: 924233

Ion Ratio Lower Upper

49 100

128 45.3 23.6 71.0




130 59.8 30.3 91.0

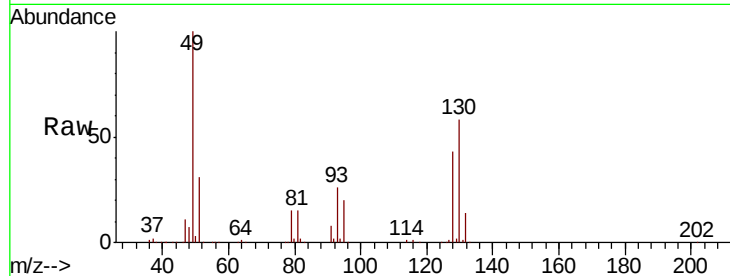

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

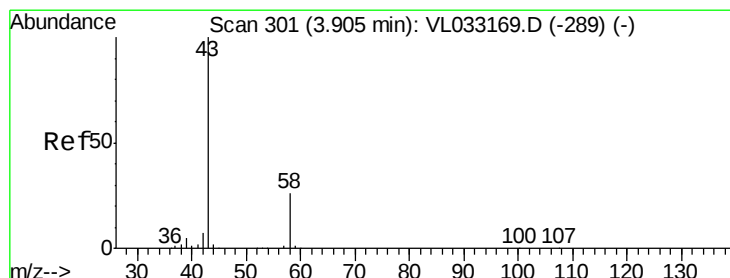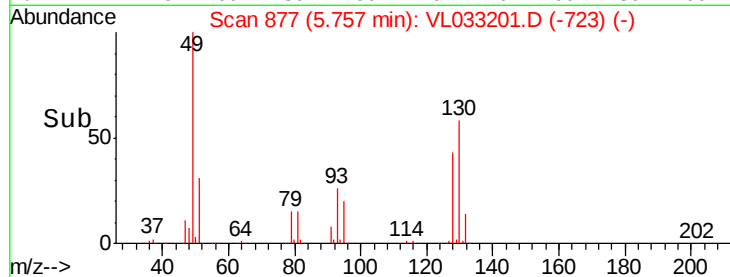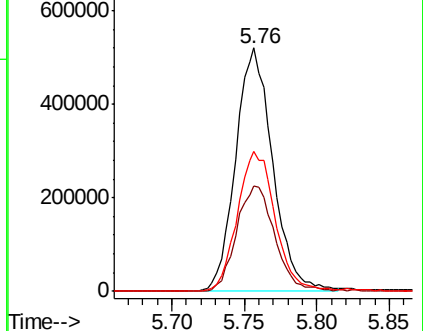

#15

Acetone

Concen: 0.207 ppbv m

RT: 3.92 min Scan# 306

Delta R.T. 0.02 min

Lab File: VL033201.D


Acq: 14 Feb 2019 16:23

Tgt Ion: 43 Resp: 21521

Ion Ratio Lower Upper



43 100


58 34.9 21.1 31.7#

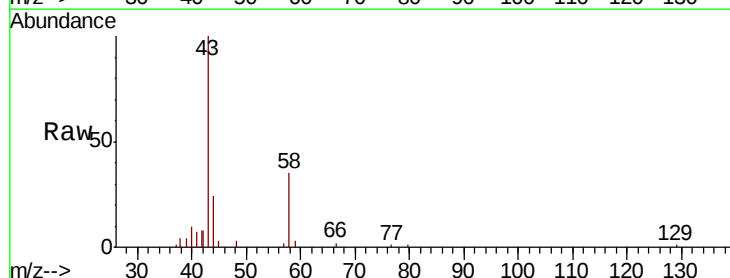

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

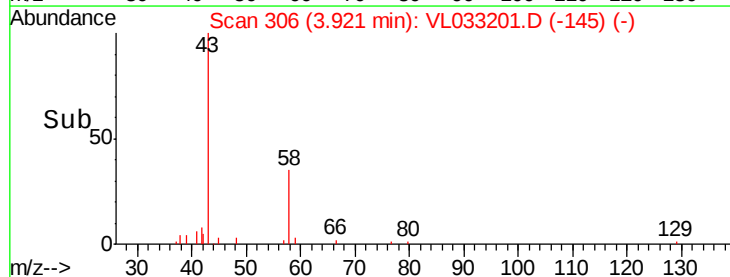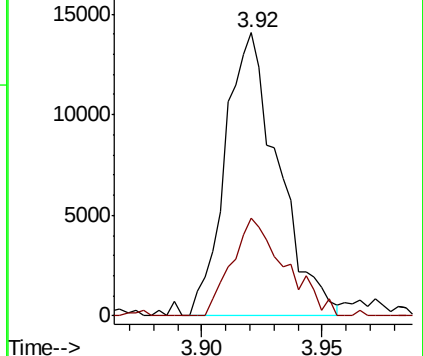

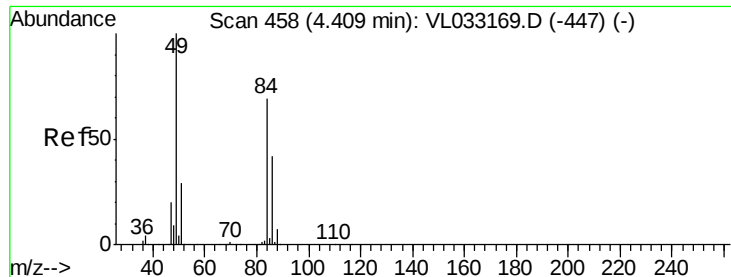

#20

Methylene Chloride

Concen: 0.223 ppbv

RT: 4.41 min Scan# 457

Delta R.T. -0.00 min

Lab File: VL033201.D

Acq: 14 Feb 2019 16:23

Tot Ion: 84 Resp: 9249


Ion Ratio Lower Upper

84 100

49 126.7 115.8 173.8

51 55.7 33.0 49.6#

86 56.6 48.2 72.2



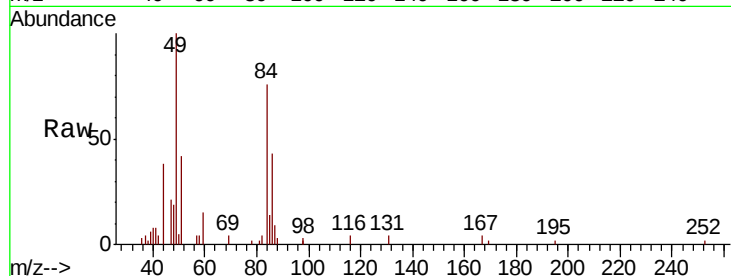


Abundance Ion 84.00 (83.70 to 84.70): VL0

Ion 49.10 (48.80 to 49.80): VL0

Ion 51.10 (50.80 to 51.80): VL0

Ion 86.00 (85.70 to 86.70): VL0

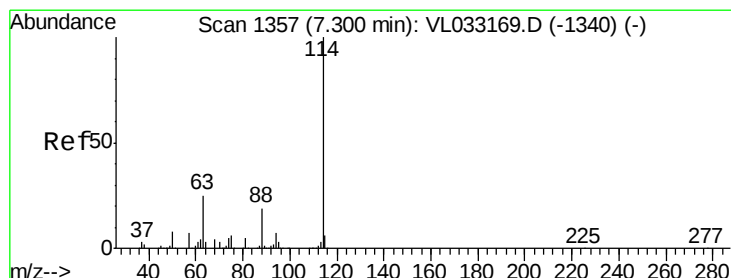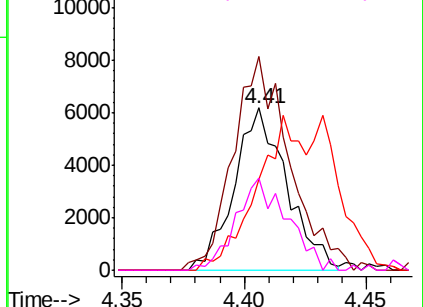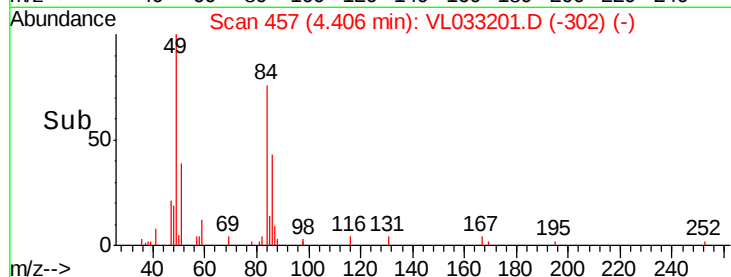

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.28 min Scan# 1352

Delta R.T. -0.02 min

Lab File: VL033201.D

Acq: 14 Feb 2019 16:23


Tgt Ion: 114 Resp: 2115108

Ion Ratio Lower Upper

114 100

63 26.8 20.8 31.2



88 18.7 14.6 22.0

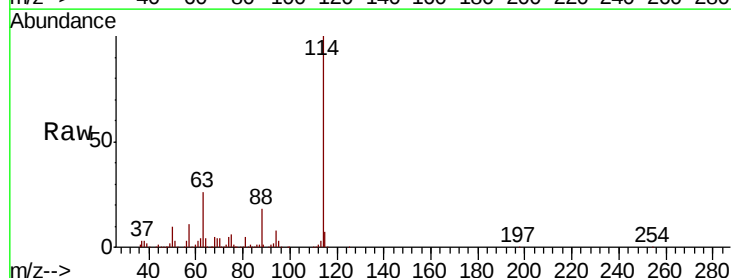


Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0


Ion 88.10 (87.80 to 88.80): VL0

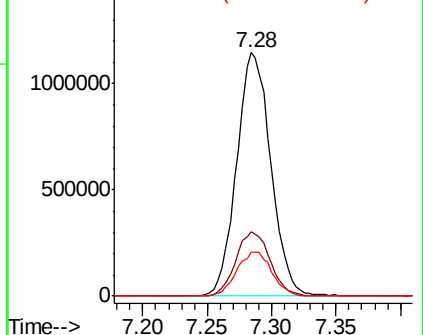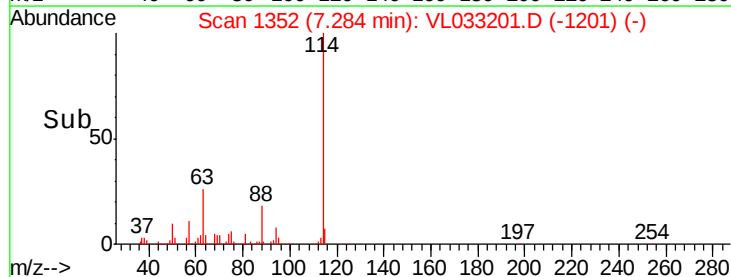



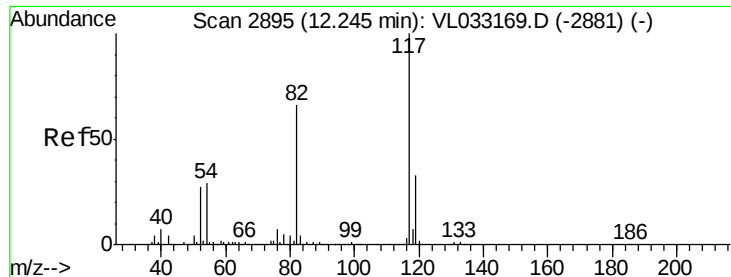


#55
Chlorobenzene-d5
Concen: 10.000 ppbv m
RT: 12.24 min Scan# 2893
Delta R.T. -0.01 min
Lab File: VL033201.D
Acq: 14 Feb 2019 16:23

Tot Ion:117 Resp: 2135774
Ion Ratio Lower Upper
117 100
82 67.4 53.8 80.8
119 0.0 46.9 70.3#

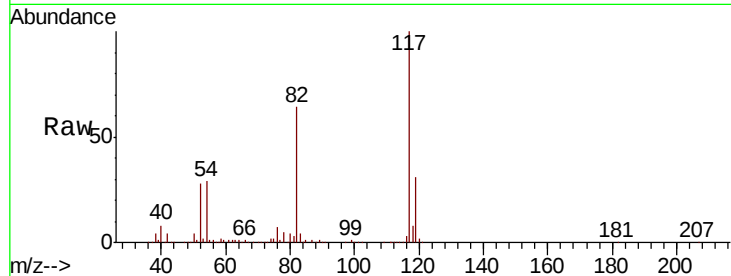


Abundance Ion 117.10 (116.80 to 117.80): V
Ion 82.10 (81.80 to 82.80): VL0
Ion 119.10 (118.80 to 119.80): V

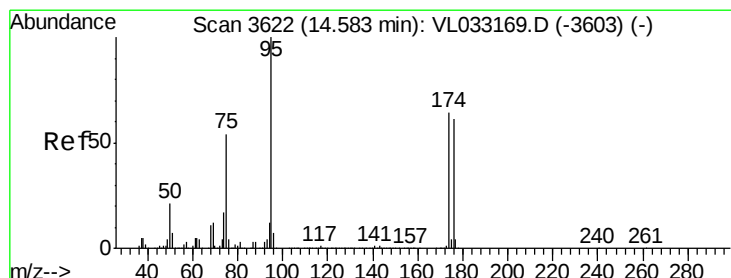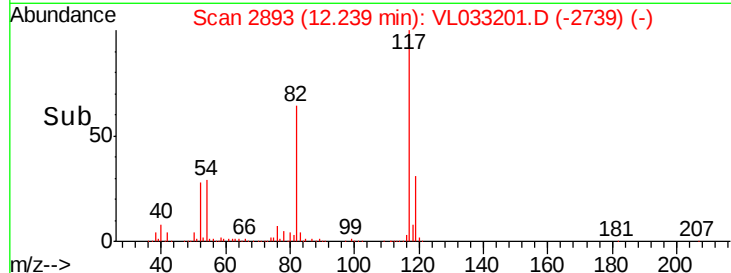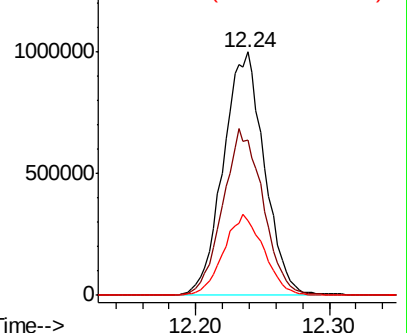

#68
1-Bromo-4-Fluorobenzene
Concen: 10.450 ppbv
RT: 14.57 min Scan# 3619
Delta R.T. -0.01 min
Lab File: VL033201.D
Acq: 14 Feb 2019 16:23

Tgt Ion: 95 Resp: 1739301
Ion Ratio Lower Upper
95 100
174 63.5 51.1 76.7
175 4.5 3.8 5.6

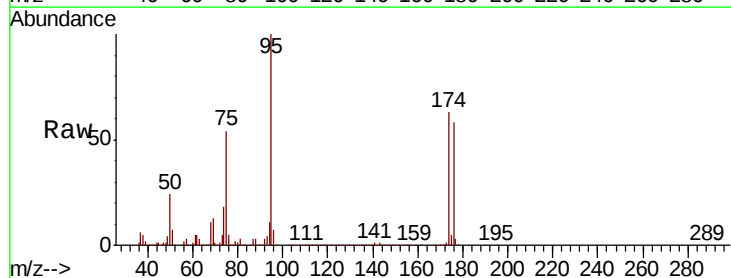

Abundance Ion 95.10 (94.80 to 95.80): VL0
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

