


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021422\
 Data File : VL038335.D
 Acq On : 14 Feb 2022 9:49
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Jan 24 14:12:48 2022
 Last Update : Mon Jan 24 14:12:48 2022

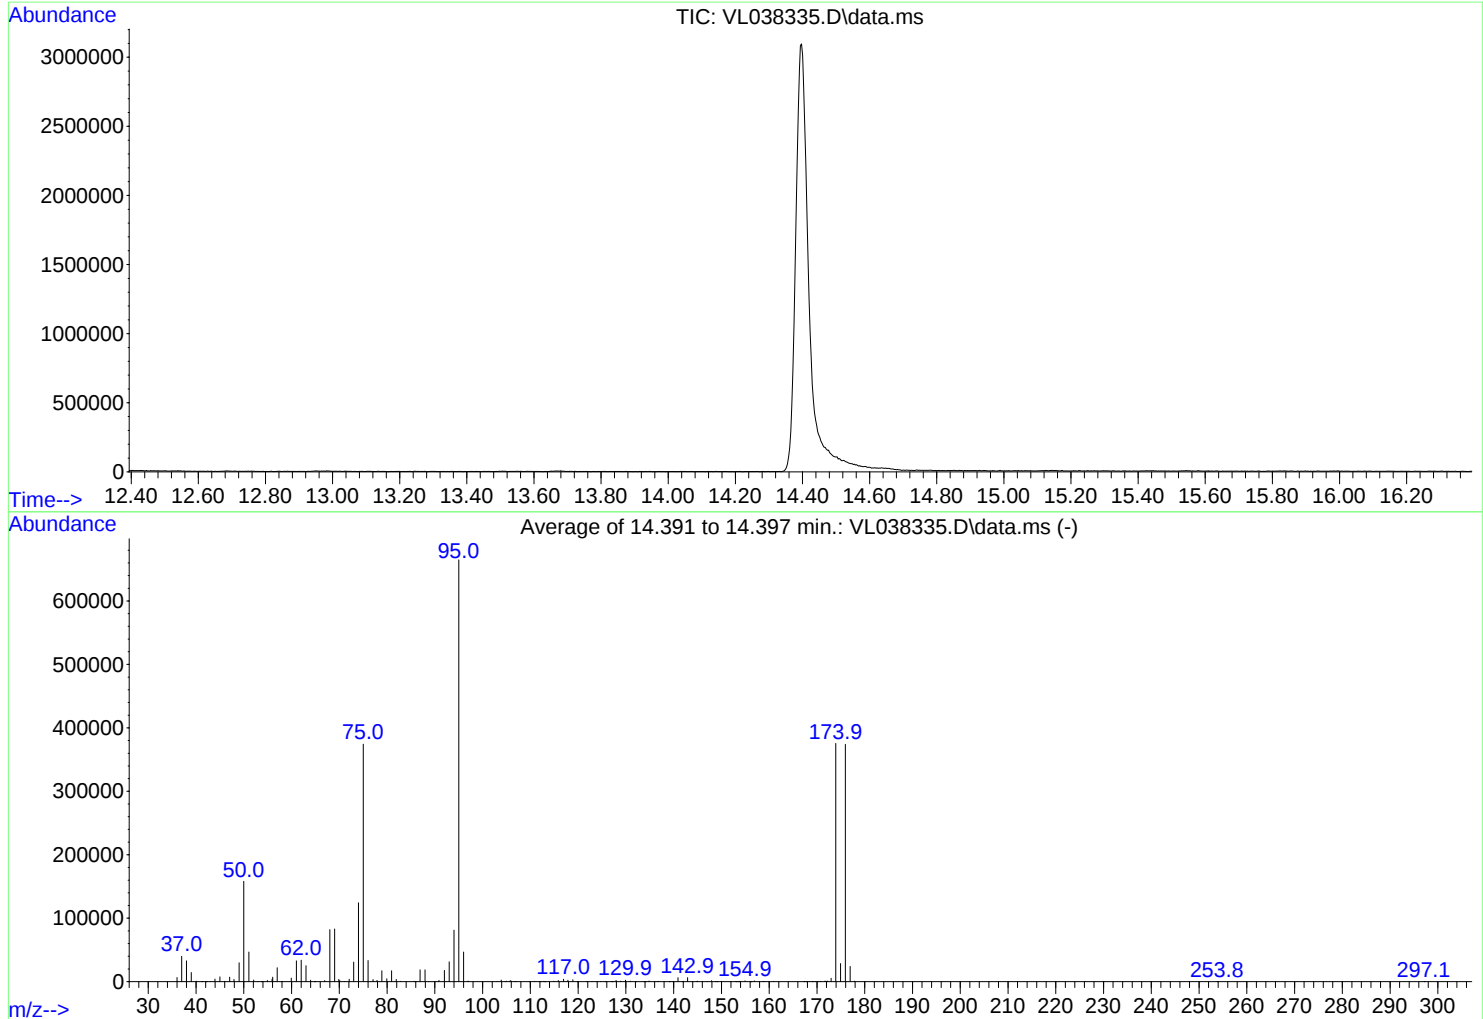

AutoFind: Scans 3609, 3610, 3611; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	158016	PASS
75	95	30	66	56.3	374315	PASS
95	95	100	100	100.0	664832	PASS
96	95	5	9	7.0	46563	PASS
173	174	0.00	2	1.4	5237	PASS
174	95	50	120	56.5	375445	PASS
175	174	4	9	7.6	28459	PASS
176	174	93	101	99.6	373952	PASS
177	176	5	9	6.4	23853	PASS

Average of 14.391 to 14.397 min.: VL038335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6622	47.05	7000	56.05	7080	66.95	1741
37.00	39907	47.95	3659	57.00	21845	68.00	8209
38.00	32869	49.00	29771	57.90	208	69.00	8306
39.00	14370	50.00	158016	58.10	446	69.90	342
40.05	797	51.05	46808	59.95	5615	70.10	1832
41.20	75	52.05	2549	61.00	32811	71.15	313
42.10	83	52.95	218	62.00	33923	72.05	3786
43.00	394	53.70	85	63.00	25128	73.00	30909
43.95	4050	54.00	208	64.00	2176	74.00	124461
45.00	7601	54.95	1799	64.80	150	75.00	374315
45.95	635	55.90	3687	65.05	602	76.00	33213

Average of 14.391 to 14.397 min.: VL038335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	3380	88.70	260	104.70	215	113.00	106
77.90	2095	89.95	174	104.95	851	114.90	682
78.90	17307	90.85	2168	105.70	863	115.85	1683
79.95	4691	92.00	17680	105.90	1828	116.95	3912
80.95	17112	93.00	31248	106.80	238	117.85	2255
81.90	3618	94.00	81157	106.95	361	118.90	2980
82.85	454	95.00	664832	109.75	359	119.80	69
85.65	493	96.00	46563	110.90	519	121.80	129
85.90	96	96.95	1131	111.85	198	122.90	279
86.90	18696	103.00	226	112.10	153	123.75	399
87.95	18567	103.90	2585	112.80	416	124.70	266

Average of 14.391 to 14.397 min.: VL038335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	87	136.00	429	144.80	221	153.60	136
126.90	324	136.70	189	145.00	802	154.05	191
127.10	76	136.85	506	146.00	614	154.95	1351
127.95	2031	139.05	146	147.05	284	156.00	149
128.90	864	139.70	209	147.95	1542	156.20	55
129.90	2183	139.95	408	148.75	335	156.90	1300
130.95	803	140.90	6239	149.00	95	157.90	167
132.00	71	141.80	128	149.95	573	158.65	420
133.80	56	142.05	438	151.90	126	158.90	197
134.00	80	142.90	6426	152.90	309	159.10	231
134.85	899	144.00	481	153.10	116	159.90	78

Average of 14.391 to 14.397 min.: VL038335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.90	616	172.95	5237				
167.30	68	173.95	375445				
167.80	78	174.95	28459				
168.40	340	175.95	373952				
169.00	65	176.95	23853				
169.65	224	177.85	799				
170.30	403	253.80	57				
170.80	494	297.10	90				
171.70	923						
172.00	489						
172.25	1034						