
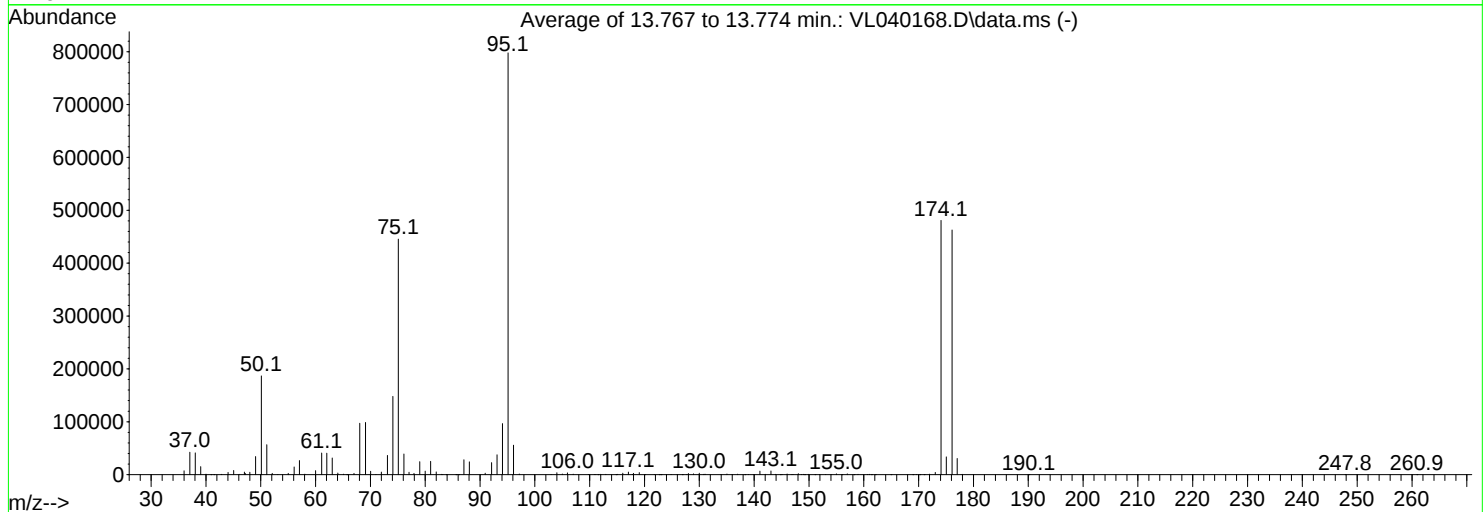


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021523\
 Data File : VL040168.D
 Acq On : 15 Feb 2023 9:50
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Feb 15 17:01:01 2023

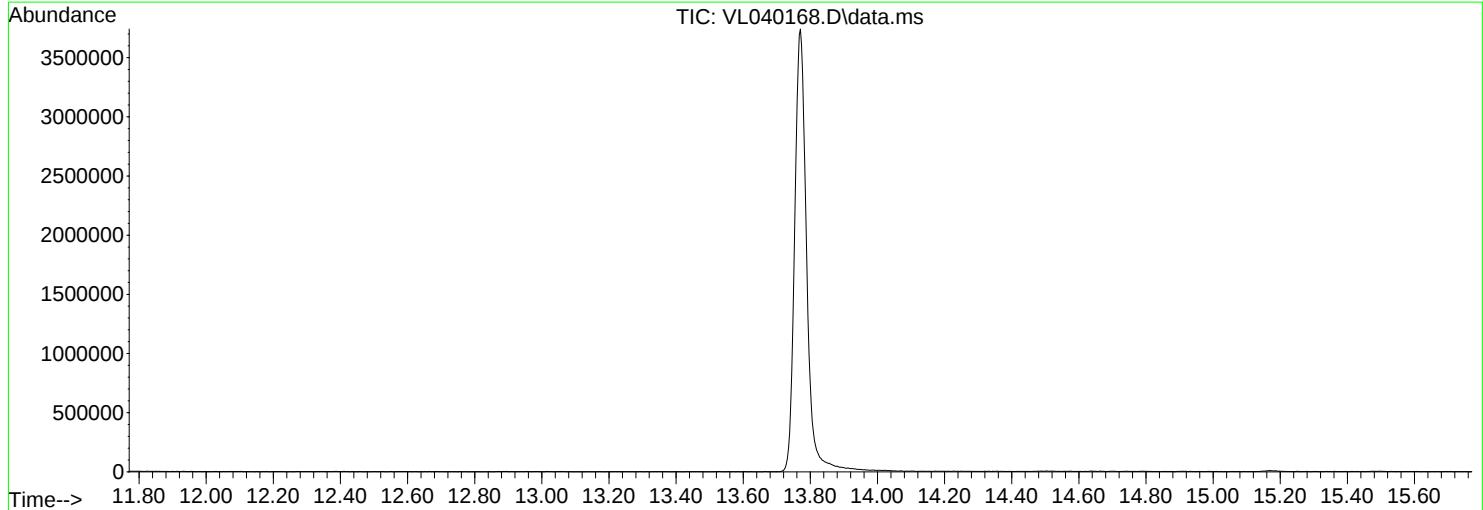

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	186709	PASS
75	95	30	66	55.8	445504	PASS
95	95	100	100	100.0	797824	PASS
96	95	5	9	7.0	55696	PASS
173	174	0.00	2	0.9	4141	PASS
174	95	50	120	60.3	480811	PASS
175	174	4	9	7.0	33677	PASS
176	174	93	101	96.2	462720	PASS
177	176	5	9	6.6	30477	PASS

Average of 13.767 to 13.774 min.: VL040168.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7289	47.00	4947	58.05	782	69.10	9868
37.05	42368	47.20	2179	60.00	7715	70.05	650
38.05	41213	48.00	4519	61.10	40880	71.00	21
39.05	15268	49.05	34349	62.05	40725	72.00	478
40.00	894	50.10	186709	63.05	31472	73.10	36216
40.90	57	51.10	56600	64.05	2955	74.10	148032
41.45	159	52.10	2449	65.10	931	75.10	445504
42.85	648	53.10	311	65.70	113	76.10	39171
44.05	4117	55.00	2318	66.05	203	77.05	4688
45.05	7825	56.10	14566	67.00	2400	77.95	2516
46.05	523	57.05	26747	68.05	97155	79.00	24595

Average of 13.767 to 13.774 min.: VL040168.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	6841	90.95	2611	107.00	1003	117.80	700
81.00	25029	92.10	22843	109.75	309	118.00	2427
82.00	5202	93.10	37416	110.85	414	119.05	4033
83.00	628	94.10	96427	111.10	301	120.00	132
83.20	361	95.10	797824	111.50	95	121.80	199
83.85	158	96.10	55696	112.00	698	122.70	117
85.60	83	97.15	1123	112.95	676	123.00	110
85.80	421	102.95	219	114.80	179	124.00	371
86.10	67	104.00	3521	115.05	643	124.85	216
87.05	28315	105.00	1288	116.05	2817	126.00	378
88.05	24248	105.95	3347	117.05	4718	126.90	83

Average of 13.767 to 13.774 min.: VL040168.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.70	382	138.95	231	148.05	1803	157.00	1427
128.00	2072	139.95	426	148.65	214	158.20	60
128.95	1462	141.05	6671	149.00	533	158.95	614
130.00	2799	142.05	755	149.20	95	160.70	192
130.80	519	143.05	6864	149.90	712	161.05	518
131.05	824	143.90	567	151.10	75	161.40	63
133.95	208	144.80	145	151.95	215	162.10	105
135.05	1143	145.10	470	153.05	359	164.95	123
136.00	280	146.00	1095	154.05	424	168.95	186
137.00	1038	146.90	270	155.00	1593	169.60	202
138.30	54	147.10	205	156.00	124	170.20	146

Average of 13.767 to 13.774 min.: VL040168.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.00	166						
172.00	945						
173.05	4141						
174.10	480811						
175.05	33677						
176.10	462720						
177.05	30477						
177.95	738						
190.10	104						
247.80	79						
260.90	85						