
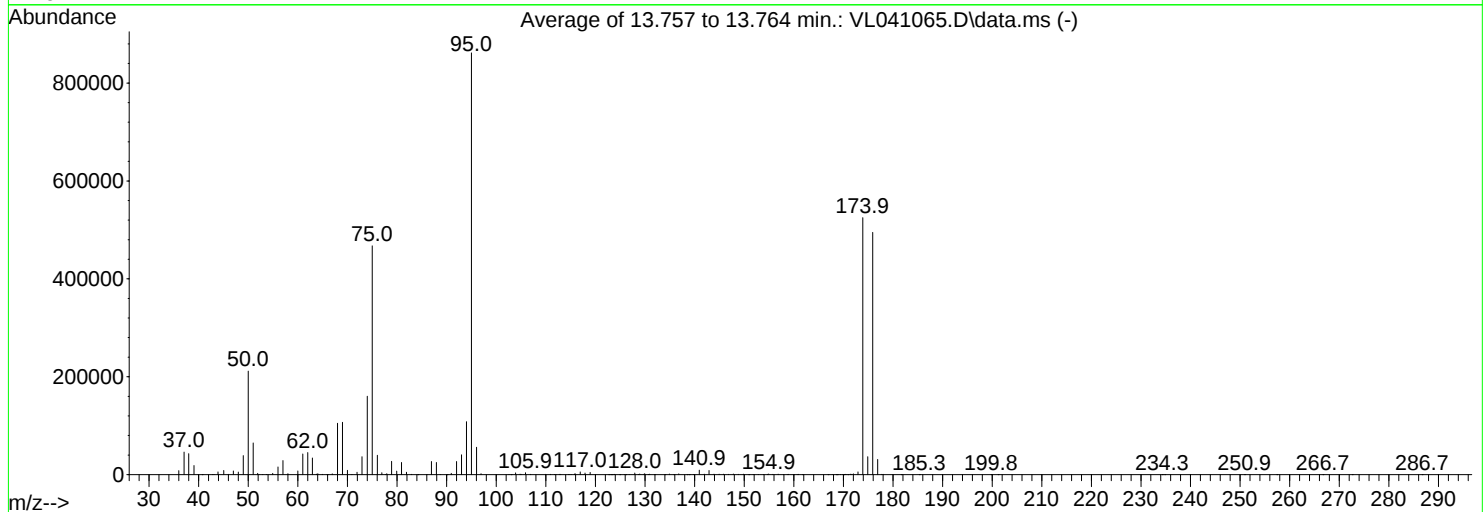


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021524\
Data File : VL041065.D
Acq On : 15 Feb 2024 10:54
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL012324AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Sat Feb 17 00:11:10 2024

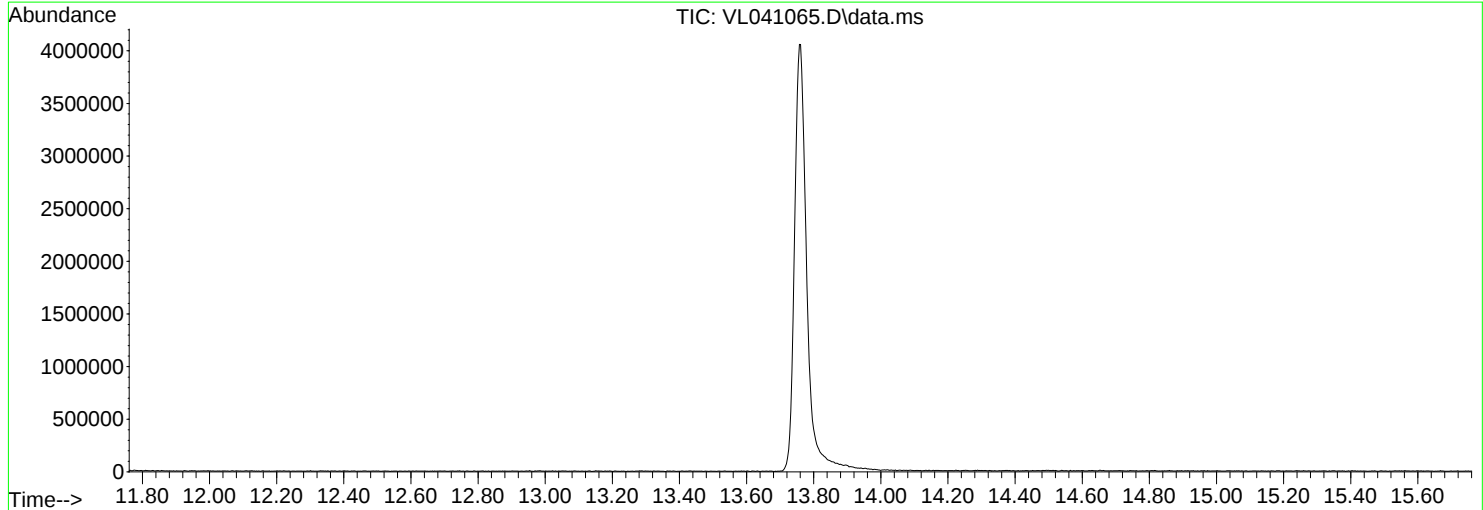

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	211456	PASS
75	95	30	66	54.2	467371	PASS
95	95	100	100	100.0	861760	PASS
96	95	5	9	6.5	55936	PASS
173	174	0.00	2	1.1	5668	PASS
174	95	50	120	60.9	524949	PASS
175	174	4	9	7.0	36651	PASS
176	174	93	101	94.3	494912	PASS
177	176	5	9	6.3	31075	PASS

Average of 13.757 to 13.764 min.: VL041065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8243	47.00	7547	57.00	28947	68.00	10511
37.05	46040	48.00	5333	58.00	2033	69.00	10681
38.00	42760	49.00	38768	60.00	7677	70.00	881
39.05	18533	50.00	211456	61.00	42016	70.90	32
39.95	275	51.00	64869	62.00	45208	71.95	4885
40.70	72	51.90	2619	62.95	34038	72.95	36712
42.85	360	52.20	452	63.75	949	74.00	160064
43.10	287	52.95	252	64.05	1902	75.00	467371
43.90	5476	53.70	275	64.95	671	76.05	39533
45.05	8618	54.95	2477	65.90	55	76.95	3987
46.00	817	56.00	15726	66.95	1610	77.70	441

Average of 13.757 to 13.764 min.: VL041065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	1840	90.10	127	104.80	983	114.80	320
78.90	27245	90.95	2719	105.00	705	115.10	367
79.95	7204	92.00	26957	105.90	3833	115.80	1287
80.90	24957	93.00	40635	106.95	737	115.95	1764
81.90	4995	94.00	108096	109.95	540	116.95	5572
82.95	727	95.00	861760	110.95	592	117.90	3235
84.20	174	96.05	55936	111.75	291	118.95	4515
86.05	334	96.95	2078	112.05	373	122.70	63
86.95	26723	102.60	338	112.70	541	123.10	96
87.95	24709	103.00	109	113.00	543	123.40	116
88.70	291	103.90	3697	114.55	388	123.85	576

Average of 13.757 to 13.764 min.: VL041065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.90	185	131.90	100	142.90	8636	152.85	395
125.80	274	134.00	120	143.90	1050	153.90	267
126.10	88	134.90	1457	144.95	876	154.70	583
126.80	406	135.80	56	145.85	1010	154.95	1287
127.95	3289	136.80	1538	146.85	616	155.80	574
128.70	429	138.50	88	147.80	1425	156.85	1097
128.95	1207	138.90	139	148.80	554	157.95	314
129.80	1068	139.75	312	149.85	1113	158.70	207
129.95	1948	140.00	266	150.90	55	158.95	770
130.70	346	140.95	9182	151.80	303	159.90	63
130.95	892	141.95	881	152.00	201	160.70	287

Average of 13.757 to 13.764 min.: VL041065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.95	581	170.90	71	181.70	61		
161.80	113	171.40	982	185.30	108		
166.90	71	171.70	566	199.80	107		
167.90	215	172.00	1647	201.20	76		
168.55	165	172.95	5668	234.30	89		
168.80	104	173.90	524949	234.80	67		
169.40	440	174.90	36651	250.90	80		
169.90	390	175.90	494912	257.40	79		
170.10	157	176.90	31075	266.70	81		
170.40	532	177.75	804	272.60	55		
170.70	282	178.00	605	286.70	59		