


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021622\
 Data File : VL038362.D
 Acq On : 16 Feb 2022 9:03
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Jan 24 14:12:48 2022
 Last Update : Mon Jan 24 14:12:48 2022

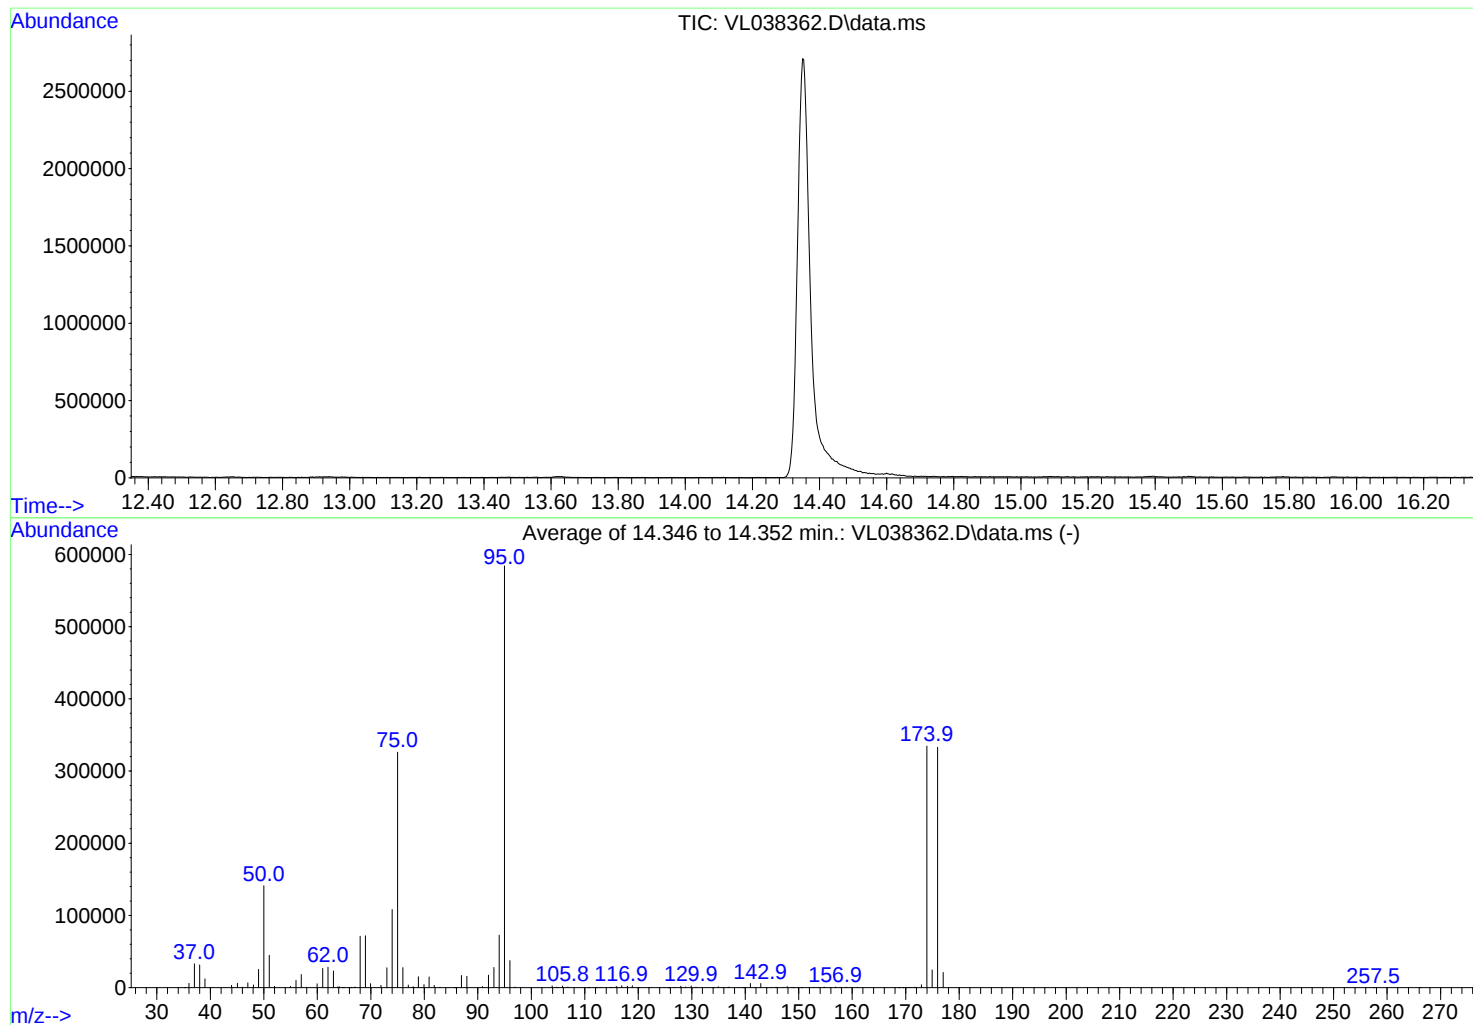

AutoFind: Scans 3595, 3596, 3597; Background Corrected with Scan 3573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	141141	PASS
75	95	30	66	55.8	325952	PASS
95	95	100	100	100.0	584256	PASS
96	95	5	9	6.4	37504	PASS
173	174	0.00	2	1.2	3910	PASS
174	95	50	120	57.3	334613	PASS
175	174	4	9	7.4	24723	PASS
176	174	93	101	99.5	332885	PASS
177	176	5	9	6.3	21035	PASS

Average of 14.346 to 14.352 min.: VL038362.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	52	47.00	6695	61.00	26533	68.00	7126
36.00	5930	48.05	3729	62.00	28397	69.00	7182
37.00	33141	49.00	25363	63.00	23072	69.95	554
38.00	31520	50.00	141141	63.80	828	71.90	308
39.00	12209	51.00	44888	64.10	1402	73.00	27541
39.95	483	52.00	1697	64.70	86	74.00	108157
40.20	286	54.95	1802	65.05	353	75.00	325952
42.85	344	56.00	10007	65.75	139	76.00	27703
43.95	3012	57.00	18221	66.30	104	77.00	3592
45.05	5996	58.00	690	66.90	646	77.90	1331
45.95	673	59.95	5268	67.05	778	78.10	557

Average of 14.346 to 14.352 min.: VL038362.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	15025	90.85	1685	106.85	766	116.90	2745
79.95	4346	92.00	17390	110.00	178	117.95	2034
80.90	14752	93.00	27920	110.70	84	118.90	2724
81.85	3151	94.00	72624	110.90	389	120.00	73
82.80	222	95.00	584256	111.75	265	122.00	60
83.00	396	96.00	37504	112.20	76	123.85	238
85.60	63	96.95	812	112.80	247	124.85	139
85.80	135	103.90	2357	113.00	177	125.60	60
86.05	441	104.75	630	114.80	471	125.80	101
86.95	16823	105.00	328	115.10	144	126.80	389
87.95	15754	105.85	2214	115.90	1778	127.95	2091

Average of 14.346 to 14.352 min.: VL038362.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.85	837	139.90	229	147.85	1473	156.90	965
129.90	2384	140.10	155	148.75	478	157.85	201
130.80	752	140.95	5671	149.00	66	158.75	363
134.00	69	141.80	501	149.85	472	159.00	442
134.95	1348	142.90	5686	150.50	98	160.95	534
135.70	181	144.00	249	151.85	239	167.85	134
135.90	160	144.80	298	152.85	367	168.70	50
136.70	228	145.00	134	153.75	241	169.00	162
136.95	817	145.75	643	154.70	457	169.50	65
138.90	236	146.00	145	154.85	745	170.00	74
139.50	60	146.95	267	155.80	224	170.50	287

Average of 14.346 to 14.352 min.: VL038362.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.70	316	257.50	61				
171.00	210	266.20	60				
171.40	197						
171.70	797						
171.90	286						
172.95	3910						
173.95	334613						
174.95	24723						
175.95	332885						
177.00	21035						
178.05	405						

Instrument :

MSVOA_L

ClientSampleId :

BFB