


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL021820\
Data File : VL034618.D
Acq On : 18 Feb 2020 9:19
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL013020AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 30 17:16:44 2020
Last Update : Thu Jan 30 17:16:44 2020

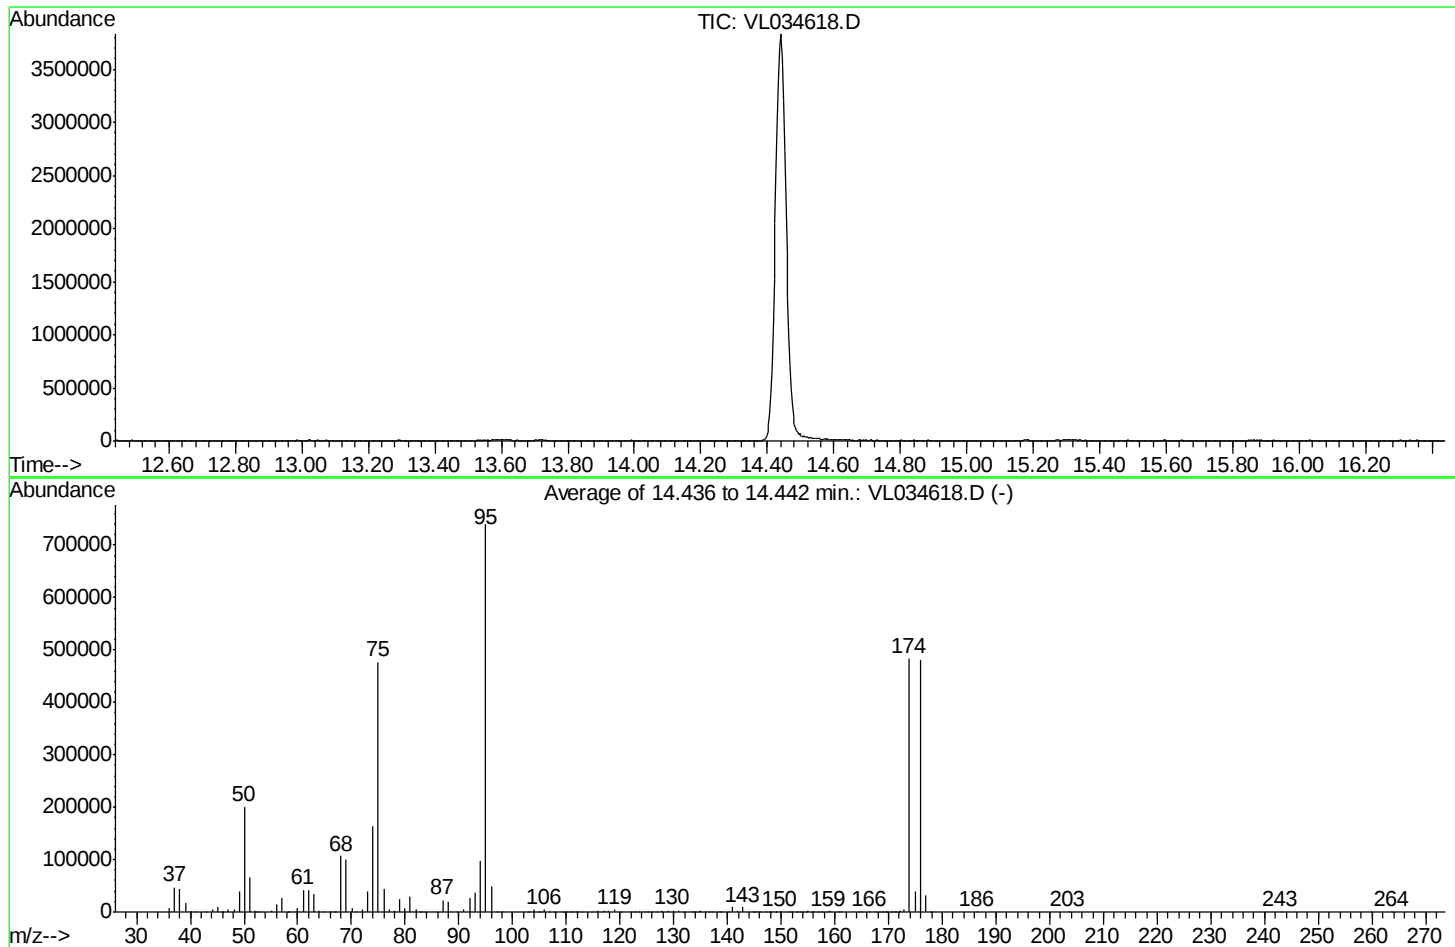

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.2	201087	PASS
75	95	30	66	64.4	476714	PASS
95	95	100	100	100.0	739776	PASS
96	95	5	9	6.6	48997	PASS
173	174	0.00	2	0.8	3988	PASS
174	95	50	120	65.4	483562	PASS
175	174	4	9	8.2	39445	PASS
176	174	93	101	99.7	482235	PASS
177	176	5	9	6.8	32658	PASS