
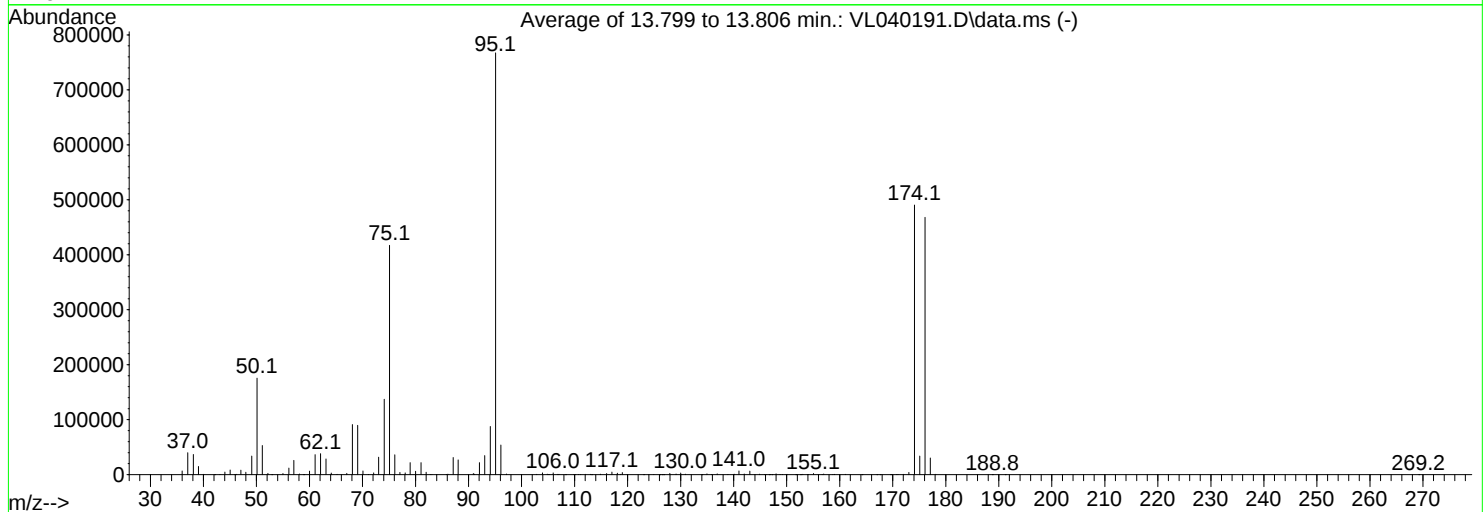


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022123\
Data File : VL040191.D
Acq On : 21 Feb 2023 9:33
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 22 03:17:31 2023

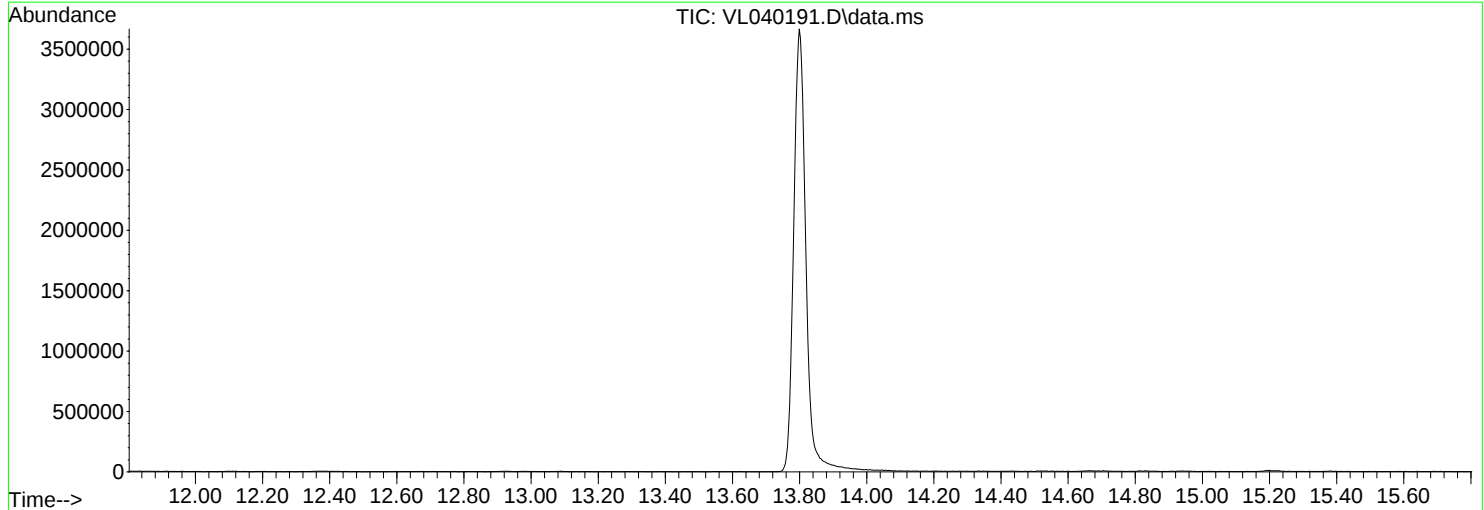

AutoFind: Scans 3482, 3483, 3484; Background Corrected with Scan 3459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	175616	PASS
75	95	30	66	54.4	417195	PASS
95	95	100	100	100.0	767339	PASS
96	95	5	9	7.0	54008	PASS
173	174	0.00	2	0.9	4192	PASS
174	95	50	120	63.9	490496	PASS
175	174	4	9	6.9	33827	PASS
176	174	93	101	95.4	468117	PASS
177	176	5	9	6.5	30413	PASS

Average of 13.799 to 13.806 min.: VL040191.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6865	47.05	8237	58.90	126	71.15	281
37.05	39936	48.00	4270	60.00	6431	72.10	324
38.10	36600	49.10	33688	61.05	36259	73.05	3176
39.05	14742	50.10	175616	62.10	38035	74.10	13707
40.05	586	51.10	53117	63.10	28515	75.10	417195
42.10	124	52.15	2265	64.10	3013	76.10	36229
43.10	312	52.90	111	65.20	605	77.05	4253
44.05	4744	55.00	1954	67.05	2261	78.05	3103
45.05	8362	56.10	11921	68.10	91259	79.00	21749
45.90	111	57.05	25797	69.10	89693	80.00	6147
46.20	546	58.10	1297	70.10	6875	81.05	21891

Average of 13.799 to 13.806 min.: VL040191.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.00	4347	93.05	34811	106.85	501	116.05	2139
82.80	160	94.10	87664	107.05	579	117.05	4725
83.10	416	95.10	767339	108.30	96	118.05	2620
84.00	227	96.10	54008	109.85	193	118.70	676
85.80	192	97.15	1328	110.15	225	119.00	3881
86.10	828	102.85	545	110.75	320	119.95	180
87.10	31224	103.95	3130	111.15	412	123.00	81
88.05	26845	104.85	892	112.05	720	124.00	385
90.90	2120	105.10	348	113.00	741	124.95	239
91.10	890	105.30	395	113.20	69	126.10	60
92.05	21736	105.95	3127	114.85	873	126.50	79

Average of 13.799 to 13.806 min.: VL040191.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.80	98	141.00	6874	148.75	351	156.05	164
127.95	2327	142.00	1056	149.20	196	156.70	227
129.15	1186	143.05	6477	149.90	193	157.00	1213
130.00	3025	144.00	355	150.05	489	158.70	234
130.90	1015	144.90	902	151.70	65	159.00	462
134.00	59	145.85	344	152.05	288	161.05	672
134.95	1402	146.10	419	152.60	90	164.20	82
135.85	209	146.70	67	153.05	622	167.00	140
136.90	1551	146.95	236	153.90	220	167.60	54
138.90	341	147.20	64	154.10	350	169.60	67
140.10	768	148.00	1593	155.05	2000	170.75	229

Average of 13.799 to 13.806 min.: VL040191.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.00	184						
172.05	559						
173.05	4192						
174.10	490496						
175.10	33827						
176.10	468117						
177.10	30413						
178.10	758						
188.80	101						
191.20	64						
269.20	53						