
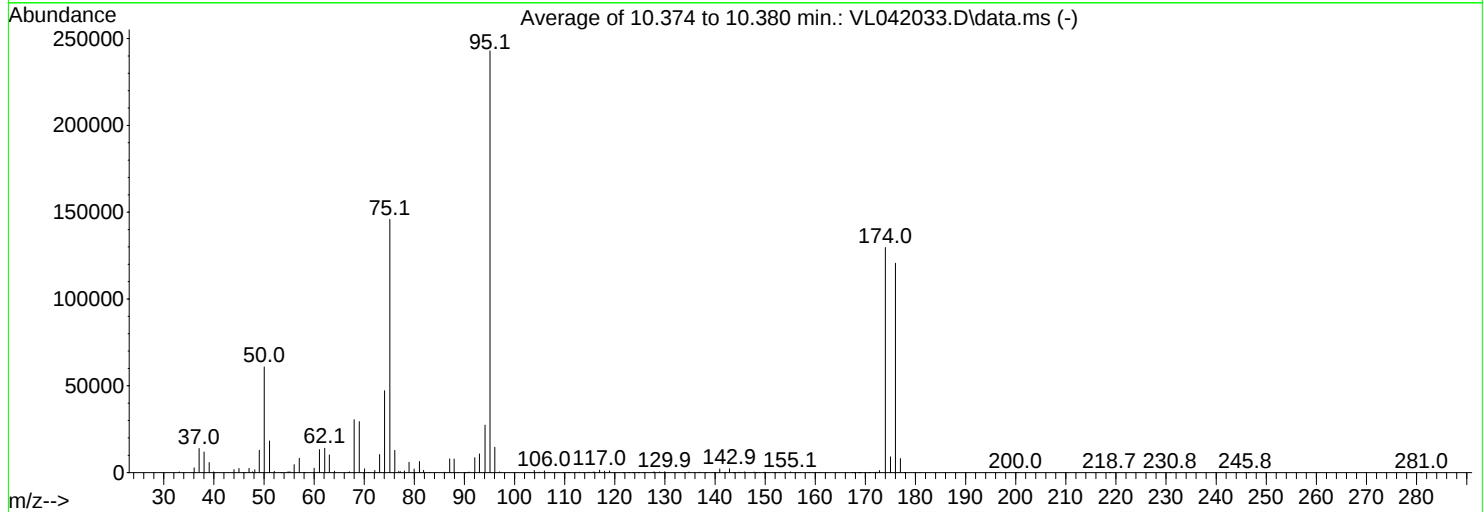


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022125\
Data File : VL042033.D
Acq On : 21 Feb 2025 08:58
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Feb 18 00:13:37 2025

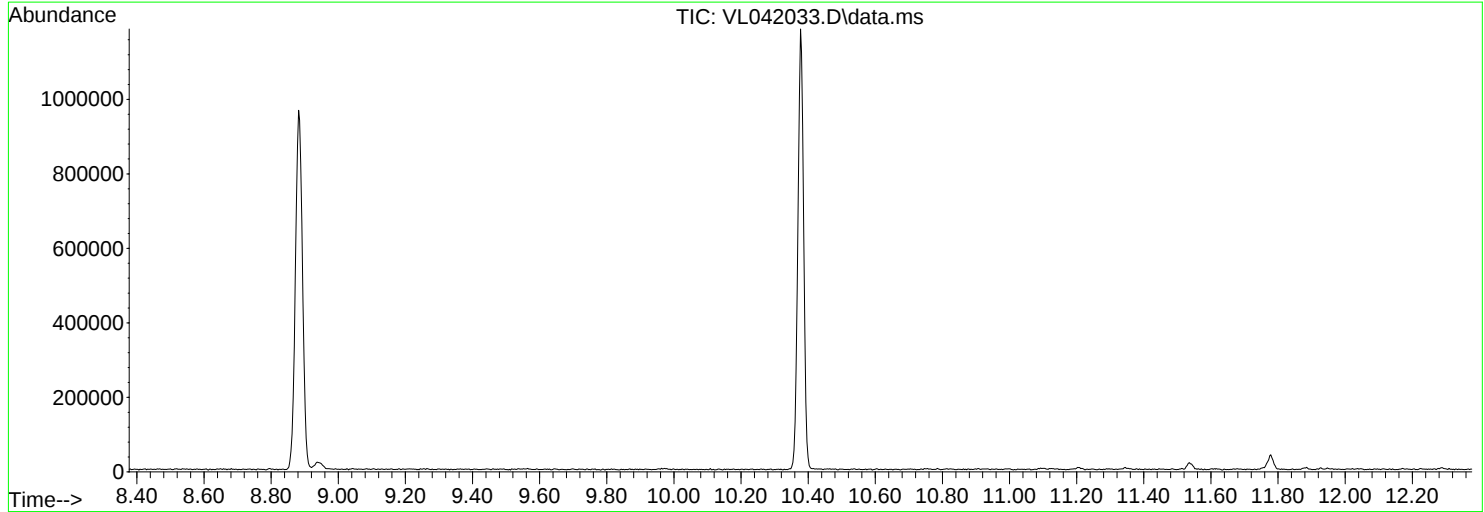

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.1	60904	PASS
75	95	30	66	60.0	145877	PASS
95	95	100	100	100.0	242944	PASS
96	95	5	9	6.0	14639	PASS
173	174	0.00	2	0.9	1176	PASS
174	95	50	120	53.4	129645	PASS
175	174	4	9	7.0	9089	PASS
176	174	93	101	93.0	120605	PASS
177	176	5	9	6.8	8145	PASS

Average of 10.374 to 10.380 min.: VL042033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	453	46.25	133	56.00	4649	68.00	3050
34.00	114	47.00	2453	57.05	8343	69.00	2937
36.05	2755	47.70	433	57.95	171	70.05	225
37.05	13901	48.15	1647	58.20	176	70.90	9
38.05	11869	49.05	12933	60.00	2579	72.10	1317
39.05	5840	50.05	60904	61.05	13271	73.05	10409
39.95	500	51.10	18227	62.10	14008	74.05	47237
42.90	127	52.05	731	63.05	10196	75.10	145877
44.00	1734	53.40	52	64.05	797	76.10	12775
45.00	2414	54.80	598	66.80	214	76.90	875
45.90	177	55.20	564	67.05	478	77.20	513

Average of 10.374 to 10.380 min.: VL042033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.00	987	90.70	168	105.95	1012	116.95	1486
78.95	6001	90.95	411	106.85	226	117.95	825
79.95	2117	92.05	8632	109.85	154	118.95	1056
81.00	6435	93.00	10748	110.70	65	121.70	45
81.85	1249	94.10	27368	110.95	106	122.80	38
83.10	189	95.10	242944	111.95	124	123.60	20
86.00	300	96.05	14639	112.95	242	123.85	84
87.05	7890	97.00	472	113.80	61	124.70	45
87.95	7798	103.00	107	114.85	295	125.75	187
88.70	81	103.95	1269	115.70	338	127.70	250
90.10	23	104.95	321	115.90	389	127.85	493

Average of 10.374 to 10.380 min.: VL042033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.95	507	143.70	17	153.00	186	168.70	29
129.95	574	144.10	138	153.80	125	169.00	48
133.90	128	144.75	248	155.05	496	170.05	172
134.80	328	145.10	238	156.05	80	170.70	39
136.90	322	145.85	463	156.70	95	170.95	209
138.35	94	147.00	143	157.05	138	171.70	181
139.95	131	147.80	402	158.85	147	172.00	187
140.95	2088	148.20	38	160.80	217	172.30	277
141.90	182	148.90	203	161.35	108	172.80	1176
142.10	203	149.95	291	167.30	32	174.00	129645
142.90	2185	151.95	46	167.80	28	175.00	9089

Average of 10.374 to 10.380 min.: VL042033.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	120605						
177.00	8145						
177.85	183						
180.90	102						
200.00	19						
218.70	40						
230.80	33						
245.80	92						
246.40	17						
281.00	22						