

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL022222\
 Data File : VL038399.D
 Acq On : 22 Feb 2022 22:10
 Operator : SY/AP
 Sample : N1607-06DL 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 MP-10DL

Quant Time: Mar 14 08:03:31 2022
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 QLast Update : Tue Feb 22 19:45:51 2022
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	904121	10.00	ppbv	0.02
33) 1,4-Difluorobenzene	7.18	114	2189616	10.00	ppbv	0.02
55) Chlorobenzene-d5	12.08	117	2046372	10.00	ppbv	0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.41	95	1663307	9.82	ppbv	0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.20%

Target Compounds


						Qvalue
3) Chlorodifluoromethane	3.04	51	22030	0.14	ppbv #	62
9) Propene	3.36	41	3828	0.07	ppbv	99
10) Heptane	8.12	43	307813	2.40	ppbv	99
13) Ethanol	3.62	45	12099	2.30	ppbv #	39
15) Acetone	3.87	43	193020	2.51	ppbv	97
16) 1,3-Butadiene	3.31	39	38743	0.75	ppbv #	17
17) tert-Butyl alcohol	4.31	59	12108	0.16	ppbv #	67
19) Isopropyl Alcohol	3.99	45	20794	0.47	ppbv #	93
20) Methylene Chloride	4.34	84	1926	0.05	ppbv #	73
25) Ethyl Acetate	5.69	43	78334	0.38	ppbv #	78
26) Hexane	5.69	57	48839	0.52	ppbv #	1
30) Cyclohexane	7.13	84	97651	1.28	ppbv #	76
34) 2-Butanone	5.26	43	28432	0.41	ppbv	99
36) Benzene	6.90	78	41507	0.22	ppbv #	93
39) 1,2-Dichloropropane	7.18	63	577913	7.53	ppbv #	25
42) Bromodichloromethane	7.78	83	6251	0.04	ppbv #	30
44) 2,2,4-Trimethylpentane	7.88	57	62480	0.19	ppbv #	42
51) 2-Hexanone	10.10	43	119759	2.20	ppbv #	30
53) Toluene	9.81	91	1642309	7.85	ppbv	99
58) Ethyl Benzene	12.71	91	351224	1.26	ppbv	91
59) m/p-Xylene	12.96	91	728000	3.03	ppbv	97
60) o-Xylene	13.69	91	314066	1.38	ppbv	99
62) Isopropylbenzene	14.66	105	77311	0.25	ppbv	98
64) n-propylbenzene	15.56	120	37600	0.50	ppbv	82
65) tert-Butylbenzene	16.76	119	35566	0.13	ppbv #	50
66) Benzyl Chloride	16.96	91	463	0.03	ppbv #	1
67) sec-Butylbenzene	17.29	105	60961	0.16	ppbv	97
69) p-Isopropyltoluene	17.65	119	25036	0.09	ppbv #	92
70) n-Butylbenzene	18.55	91	42934	0.14	ppbv #	48
71) 2-Chlorotoluene	15.83	91	20072	0.09	ppbv	68
72) 4-Ethyltoluene	15.83	105	157858	0.63	ppbv	96
73) 1,3,5-Trimethylbenzene	16.00	105	133593	0.59	ppbv	90
74) 1,2,4-Trimethylbenzene	16.76	105	365041	1.52	ppbv #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_L\DATA\VL022222\
Data File : VL038399.D
Acq On : 22 Feb 2022 22:10
Operator : SY/AP
Sample : N1607-06DL 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
MP-10DL

Quant Time: Mar 14 08:03:31 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

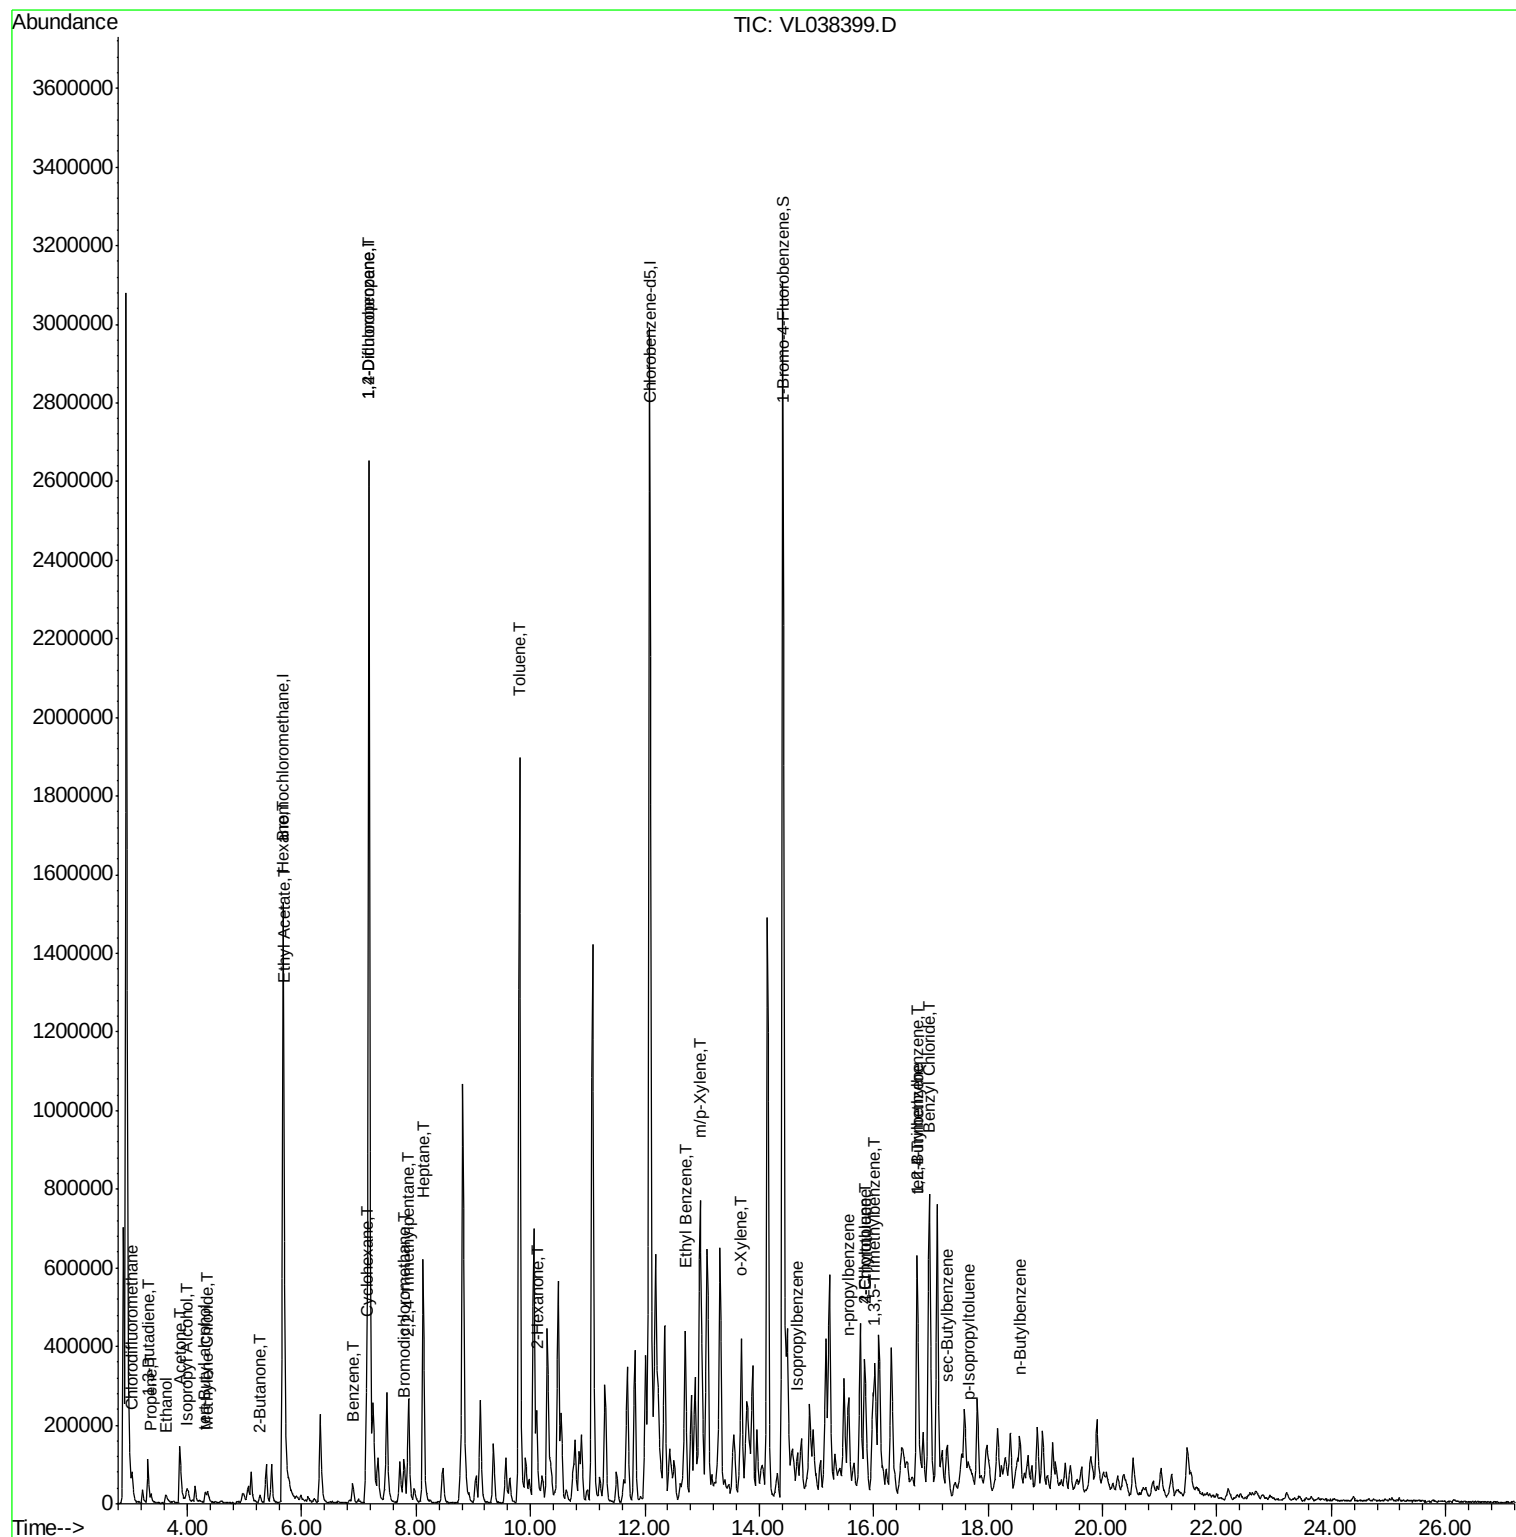

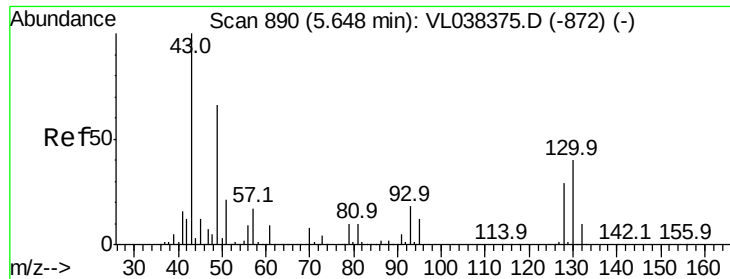

#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 5.67 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 22 Feb 2022 22:10


Tgt Ion: 49 Resp: 904121

Ion Ratio Lower Upper

49 100

128 47.3 24.3 72.9




130 60.6 30.1 90.5

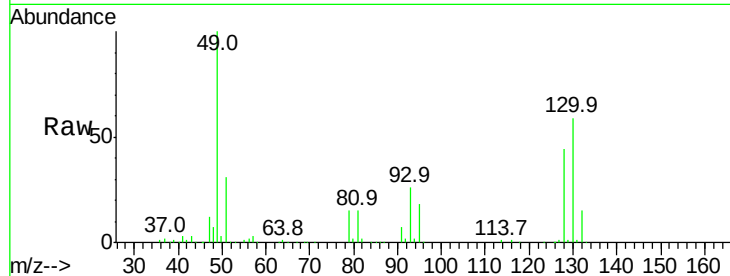

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

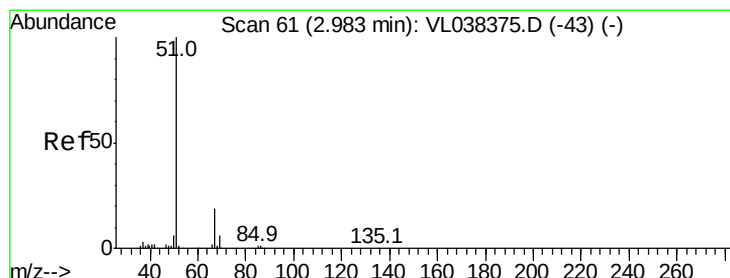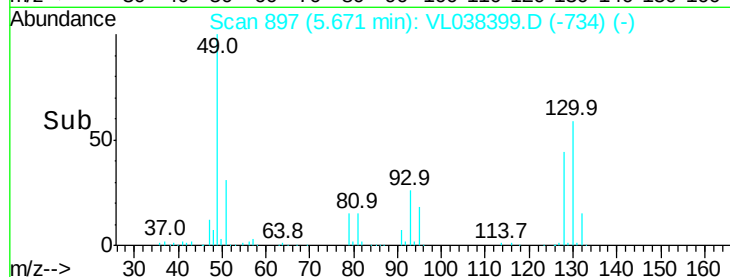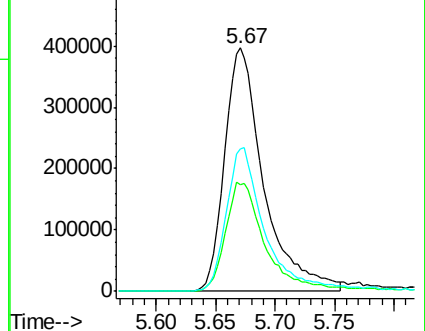

#3

Chlorodifluoromethane

Concen: 0.14 ppbv

RT: 3.04 min Scan# 78

Delta R.T. 0.05 min

Lab File: VL038399.D


Acq: 22 Feb 2022 22:10

Tgt Ion: 51 Resp: 22030

Ion Ratio Lower Upper



51 100


67 1.3 14.7 22.1#

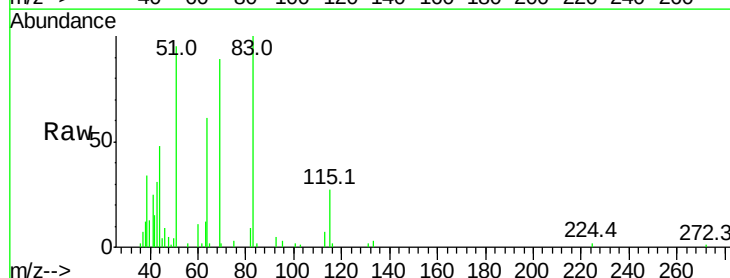

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

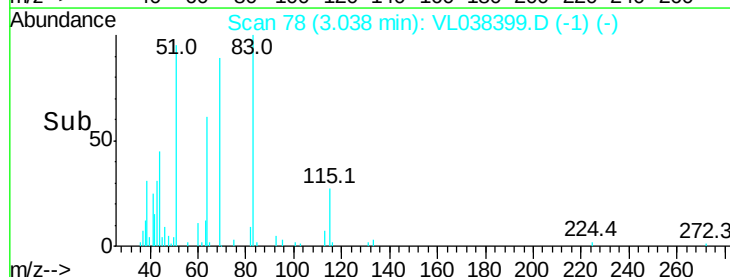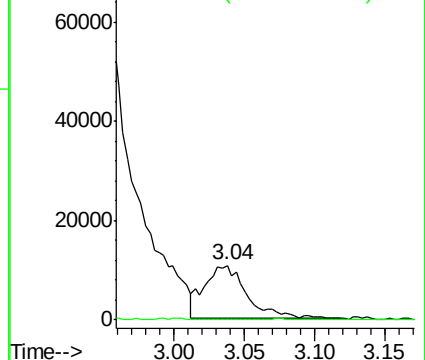

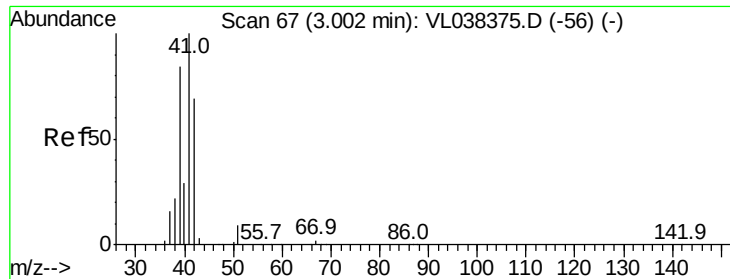

#9

Propene

Concen: 0.07 ppbv

RT: 3.36 Instrument:

Delta R.T. MSVOA_1

Lab File: ClientSampleId:





Acq: 22 Feb 2022 22:10

Tgt Ion: 41 Resp: 3828

Ion Ratio Lower Upper

41 100

42 67.1 54.6 82.0

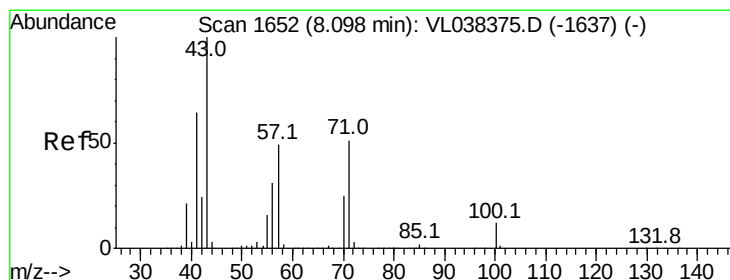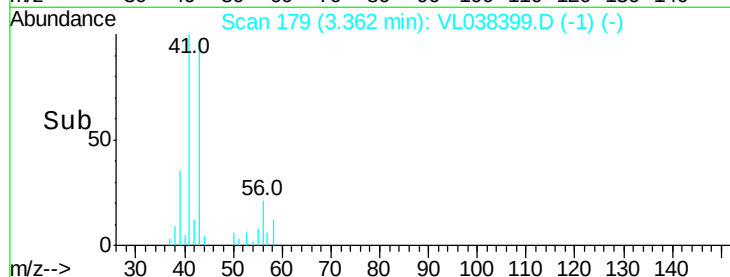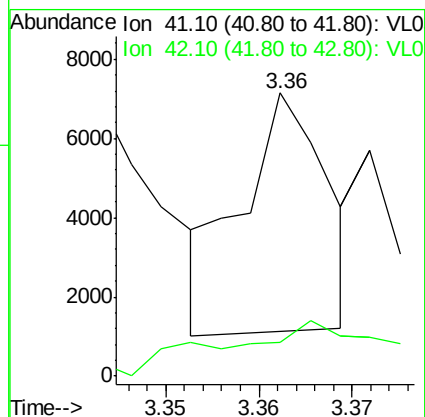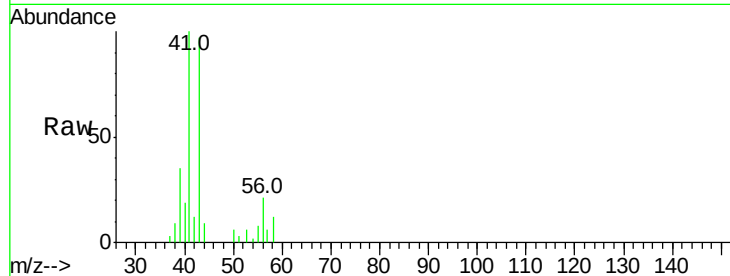

#10

Heptane

Concen: 2.40 ppbv

RT: 8.12 min Scan# 1660

Delta R.T. 0.03 min

Lab File: VL038399.D




Acq: 22 Feb 2022 22:10


Tgt Ion: 43 Resp: 307813

Ion Ratio Lower Upper

43 100





57 48.8 39.8 59.8

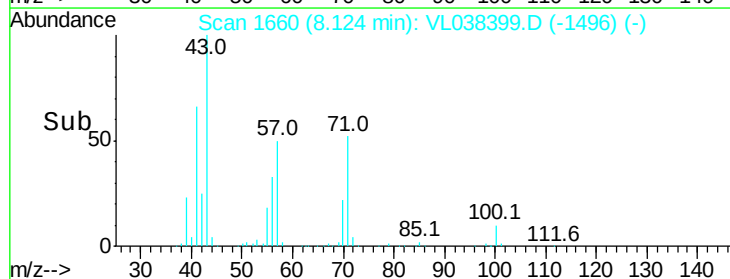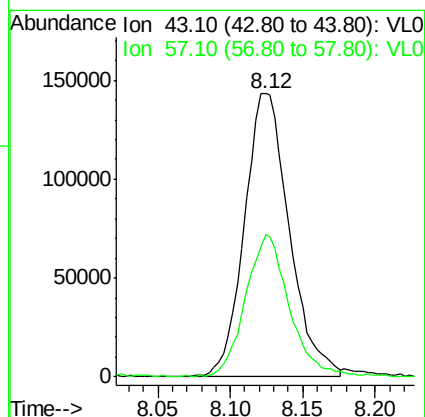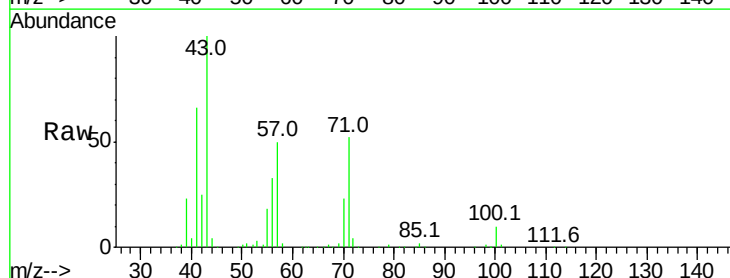

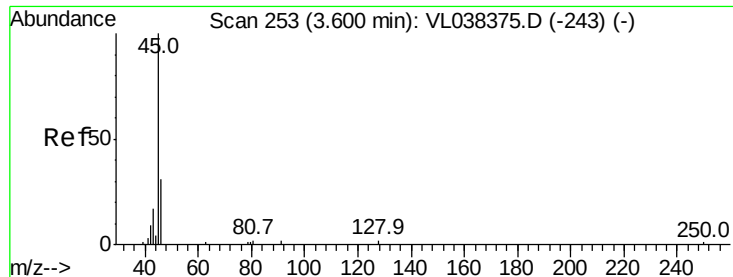




#13
 Ethanol
 Concen: 2.30 ppbv
 RT: 3.62
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 22 Feb 2022 22:10


Tgt Ion: 45 Resp: 12099
 Ion Ratio Lower Upper
 45 100
 46 85.7 18.2 72.8#

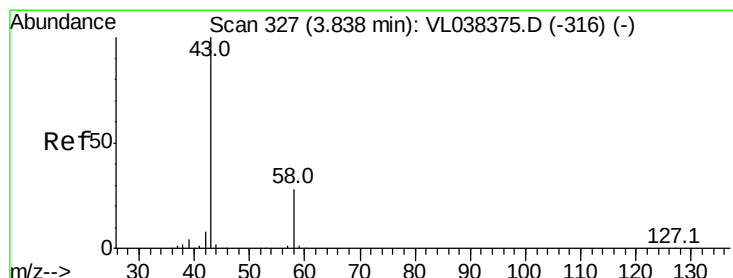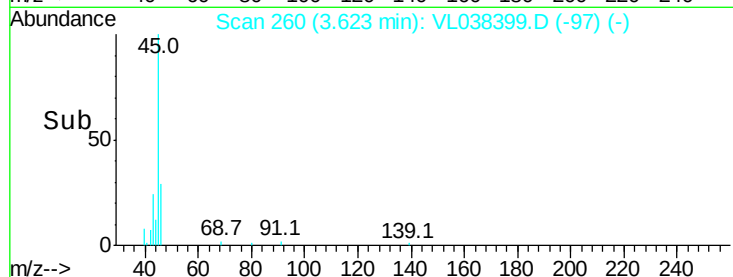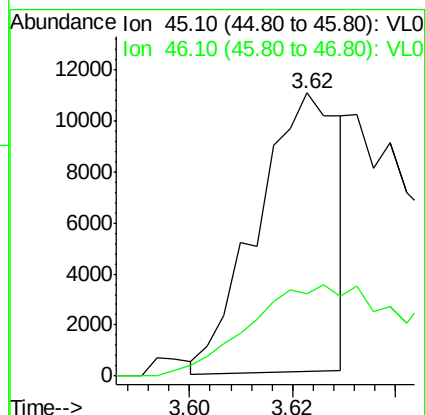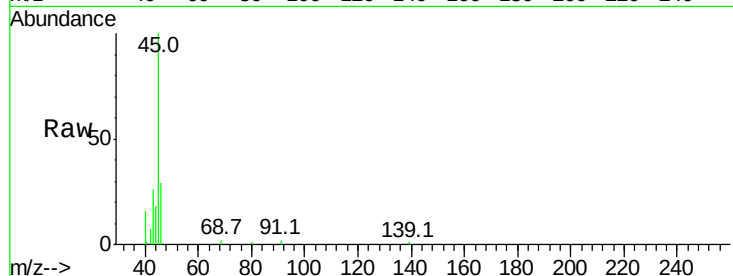

#15
 Acetone
 Concen: 2.51 ppbv
 RT: 3.87 min Scan# 336
 Delta R.T. 0.03 min
 Lab File: VL038399.D
 Acq: 22 Feb 2022 22:10





Tgt Ion: 43 Resp: 193020
 Ion Ratio Lower Upper
 43 100
 58 28.8 21.7 32.5

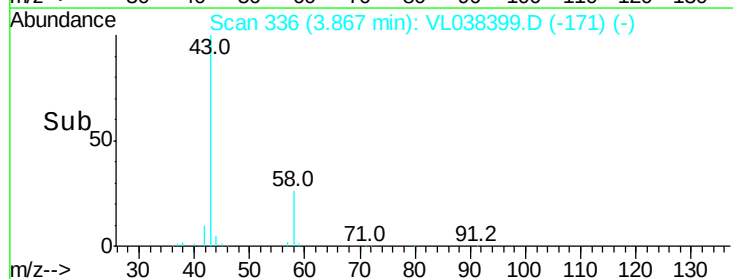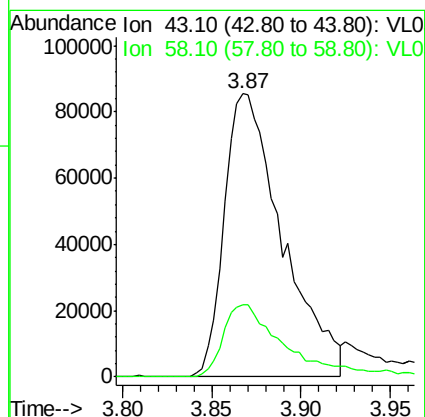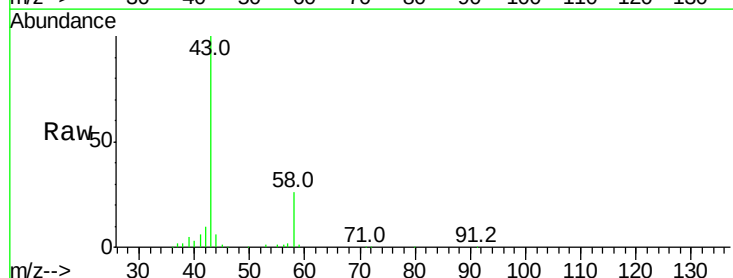

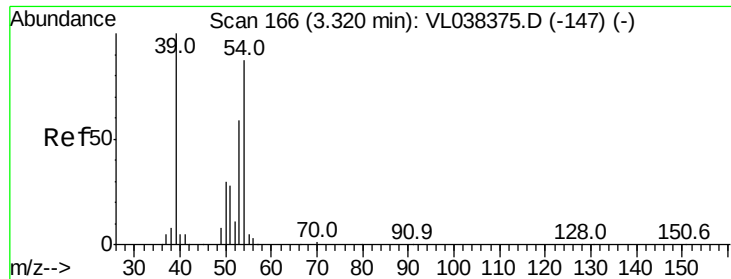




#16
 1,3-Butadiene
 Concen: 0.75 ppbv
 RT: 3.31
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 22 Feb 2022 22:10


Tgt Ion: 39 Resp: 38743
 Ion Ratio Lower Upper
 39 100
 54 4.8 60.3 90.5#

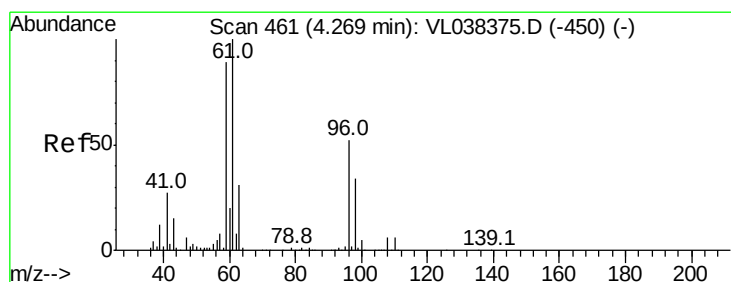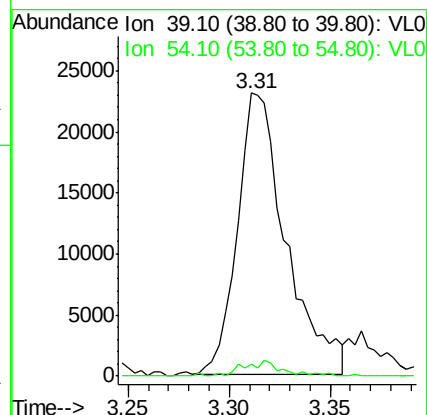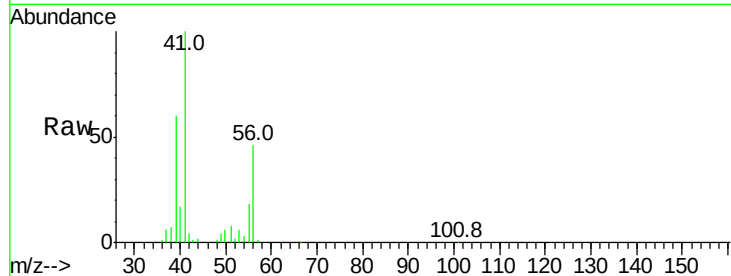

#17
 tert-Butyl alcohol
 Concen: 0.16 ppbv
 RT: 4.31 min Scan# 474
 Delta R.T. 0.04 min
 Lab File: VL038399.D
 Acq: 22 Feb 2022 22:10

Tgt Ion: 59 Resp: 12108
 Ion Ratio Lower Upper
 59 100
 57 22.8 8.4 12.6#

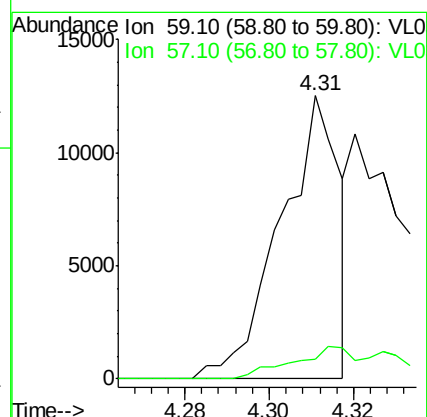

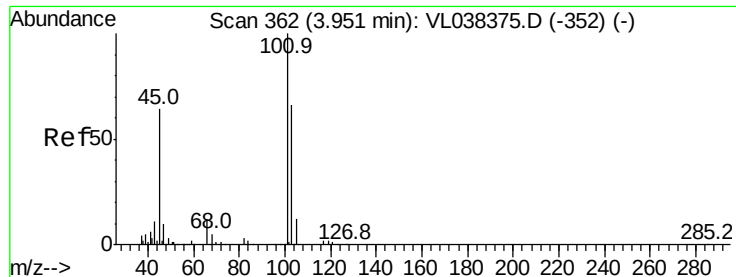

#19

Isopropyl Alcohol

Concen: 0.47 ppbv

RT: 3.99 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:





Acq: 22 Feb 2022 22:10

Tgt Ion: 45 Resp: 20794

Ion Ratio Lower Upper

45 100

58 0.0 1.8 2.8#

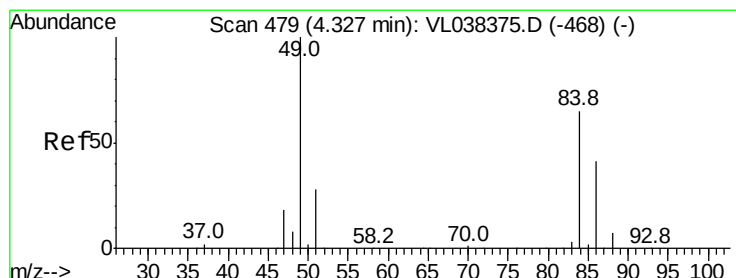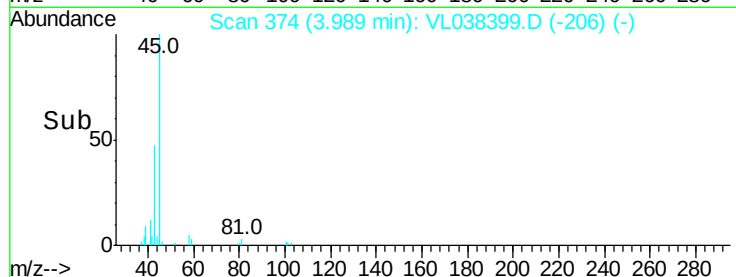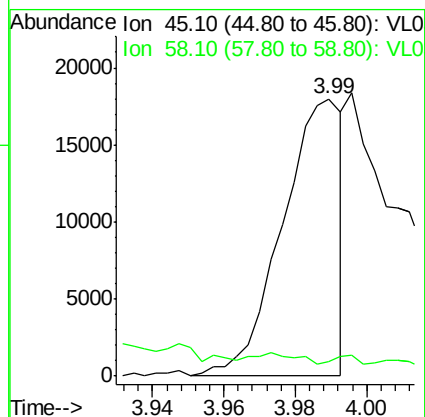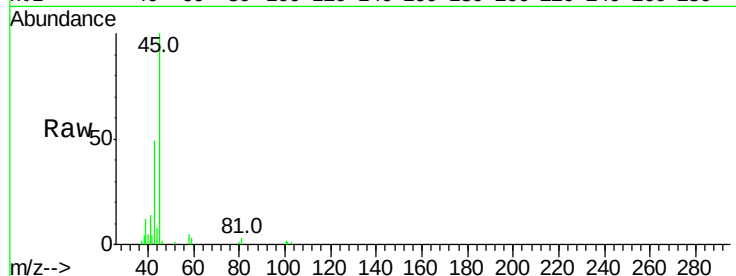

#20

Methylene Chloride

Concen: 0.05 ppbv

RT: 4.34 min Scan# 483

Delta R.T. 0.01 min

Lab File: VL038399.D

Acq: 22 Feb 2022 22:10

Tgt Ion: 84 Resp: 1926




Ion Ratio Lower Upper


84 100

49 116.2 122.4 183.6#

51 26.9 33.3 49.9#





86 43.7 50.7 76.1#

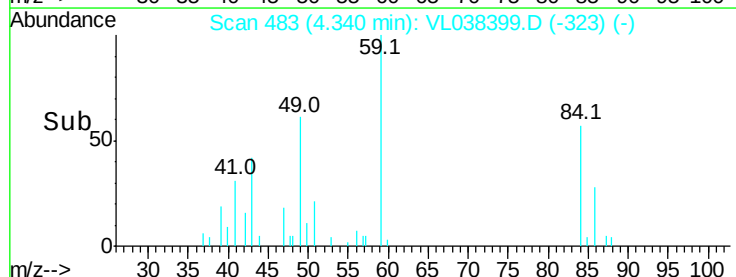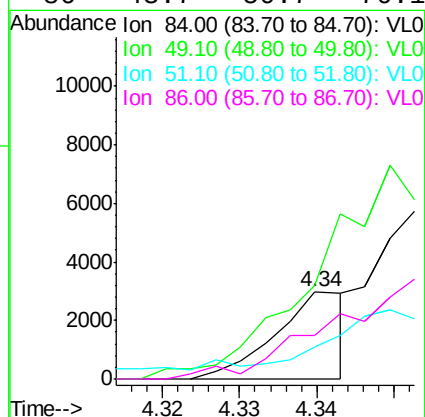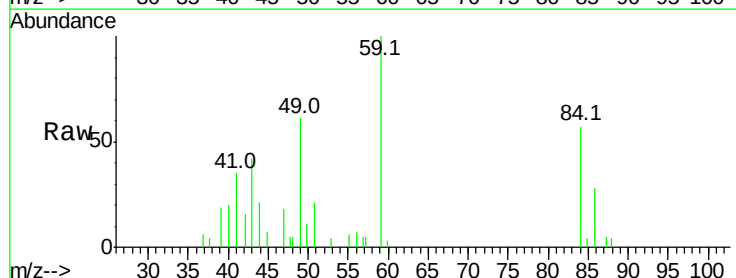

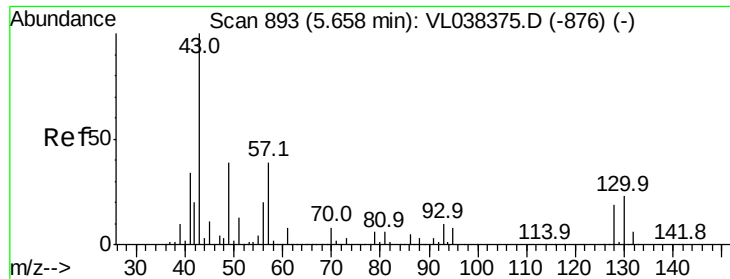




#25
Ethyl Acetate
Concen: 0.38 ppbv
RT: 5.69
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
MP-10DL
Acq: 22 Feb 2022 22:10


Tgt Ion:	43	Resp:	78334
Ion	Ratio	Lower	Upper
43	100		
45	0.8	7.8	11.6#
61	0.0	7.5	11.3#
70	1.5	5.4	8.0#

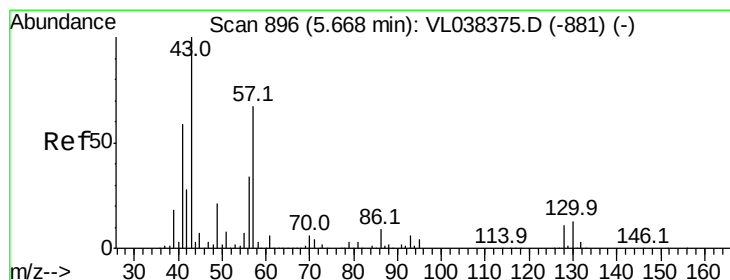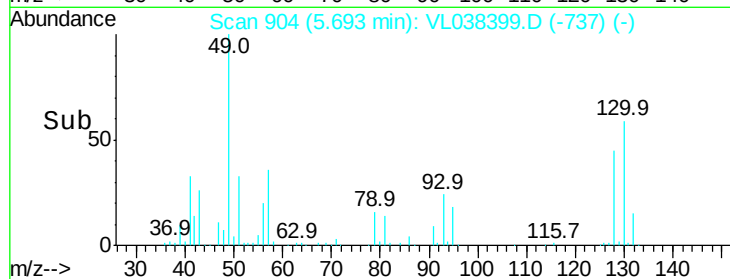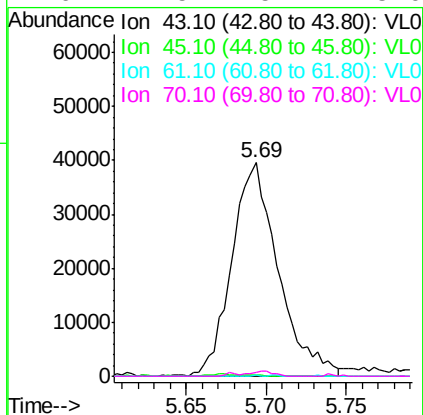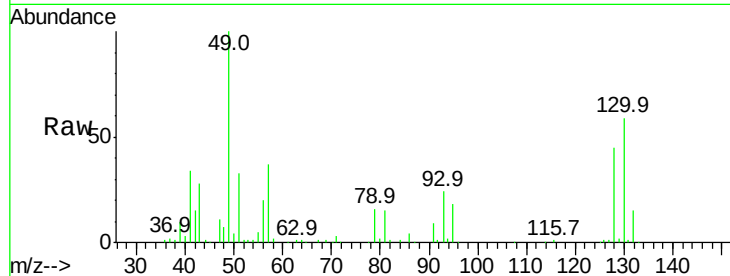

#26
Hexane
Concen: 0.52 ppbv
RT: 5.69 min Scan# 902
Delta R.T.: 0.02 min
Lab File: VL038399.D
Acq: 22 Feb 2022 22:10





Tgt Ion:	57	Resp:	48839
Ion	Ratio	Lower	Upper
57	100		
41	0.0	73.1	109.7#
43	0.0	181.0	271.4#
56	0.0	43.4	65.0#

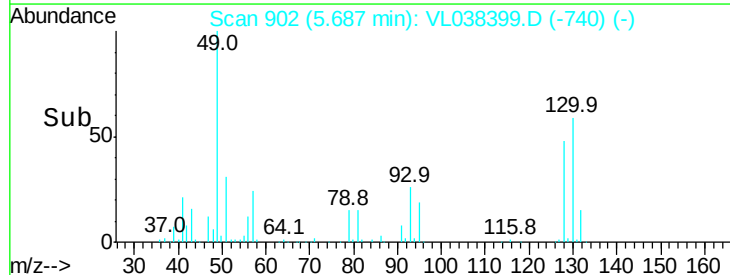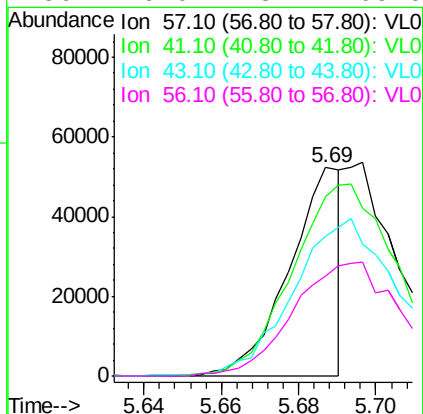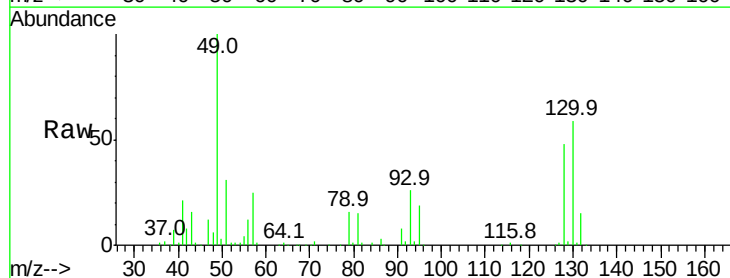

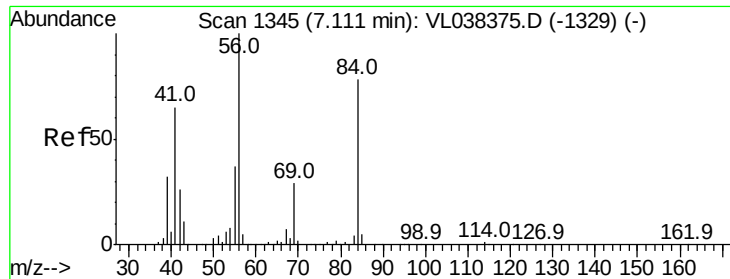




#30
Cyclohexane
Concen: 1.28 ppbv
RT: 7.13
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 22 Feb 2022 22:10


Tgt Ion	Ratio	Lower	Upper
84	100		
56	190.9	116.2	174.4#
41	95.9	74.3	111.5

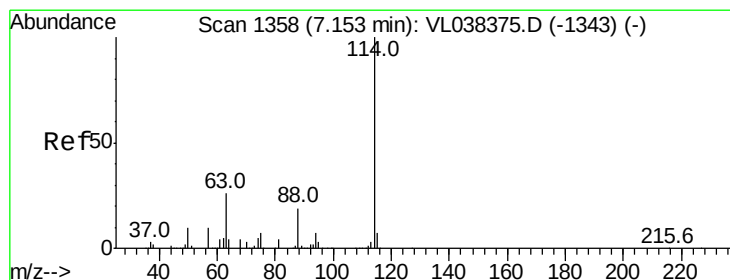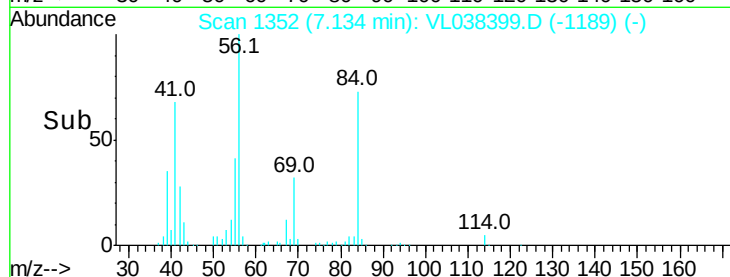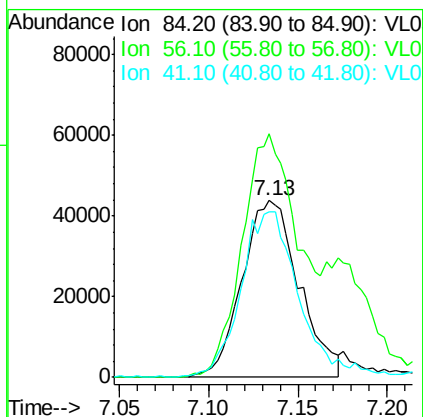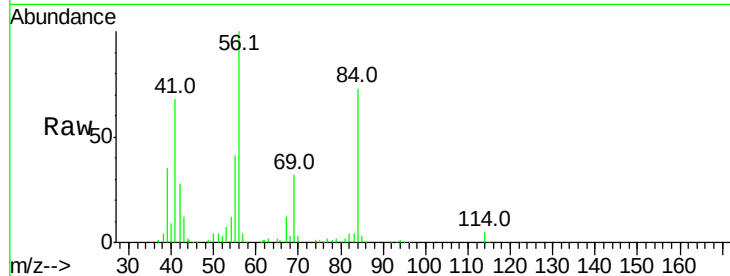

#33
1,4-Difluorobenzene
Concen: 10.00 ppbv
RT: 7.18 min Scan# 1365
Delta R.T. 0.02 min
Lab File: VL038399.D
Acq: 22 Feb 2022 22:10





Tgt Ion	Ratio	Lower	Upper
114	100		
63	27.6	22.2	33.2
88	19.1	15.2	22.8

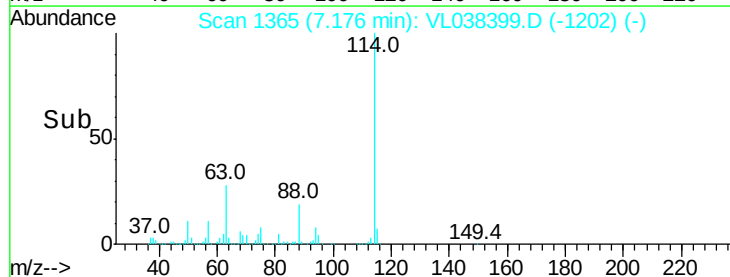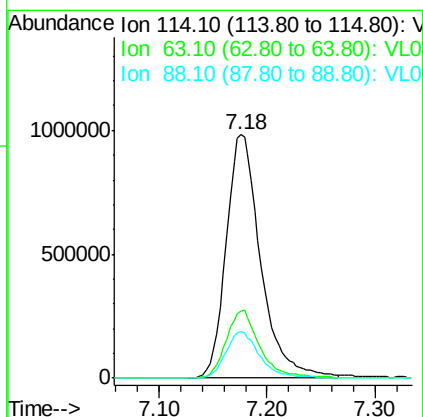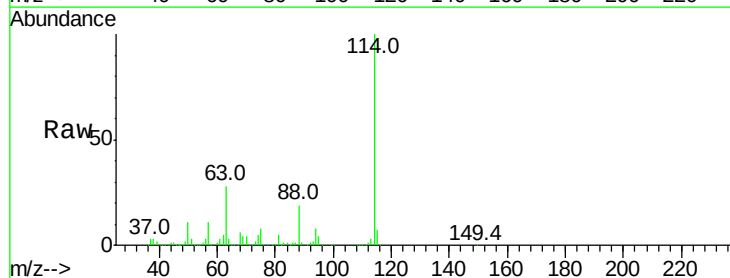

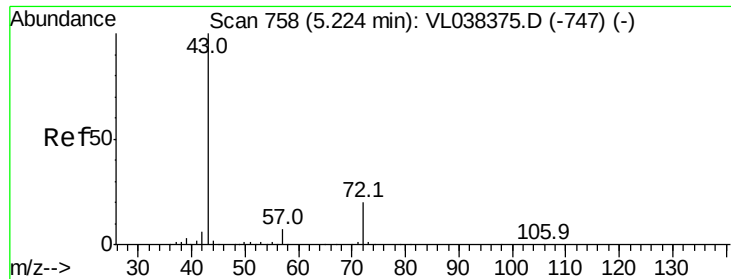




#34
2-Butanone
Concen: 0.41 ppbv
RT: 5.26
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
MP-10DL
Acq: 22 Feb 2022 22:10


Tgt Ion: 43 Resp: 28432
Ion Ratio Lower Upper
43 100
72 21.5 17.4 26.2

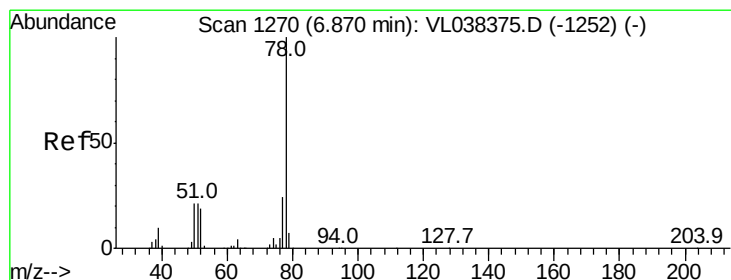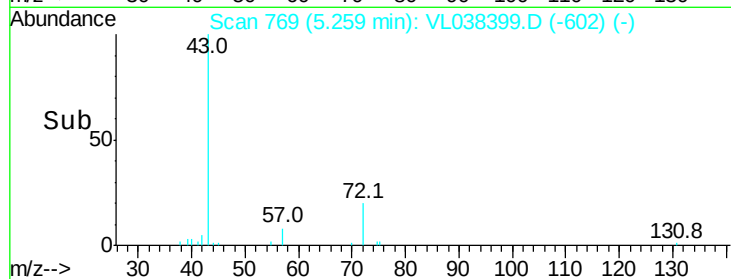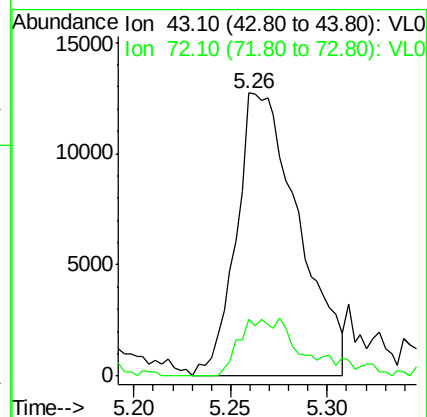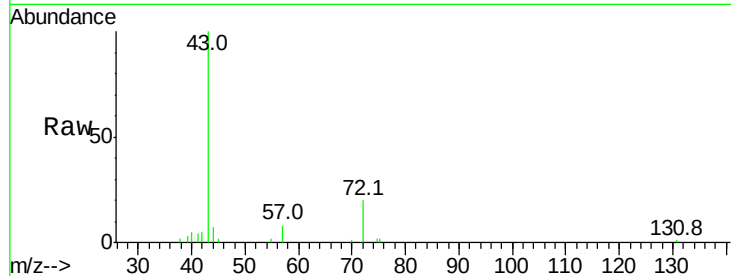

#36
Benzene
Concen: 0.22 ppbv
RT: 6.90 min Scan# 1278
Delta R.T. 0.03 min
Lab File: VL038399.D
Acq: 22 Feb 2022 22:10

Tgt Ion: 78 Resp: 41507
Ion Ratio Lower Upper
78 100
77 22.0 19.0 28.6
50 15.4 16.6 24.8#

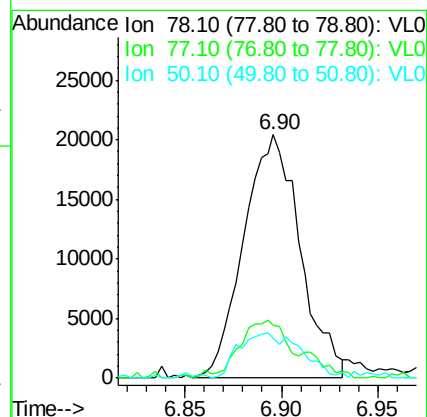

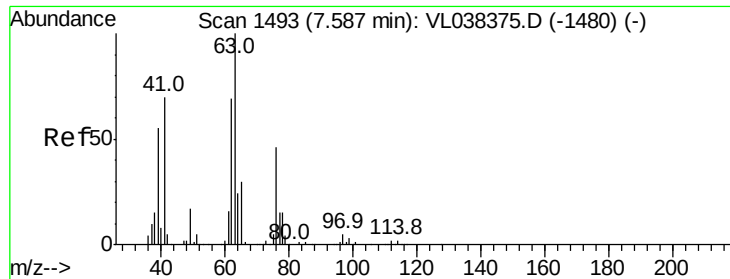

#39

1,2-Dichloropropane

Concen: 7.53 ppbv

RT: 7.18 Instrument:

Delta R.T. MSVOA_1

Lab File: ClientSampleId:

Acq: 22 Feb 2022 22:10


Tgt Ion: 63 Resp: 577913

Ion Ratio Lower Upper

63 100

41 0.0 56.1 84.1#




62 16.2 55.5 83.3#

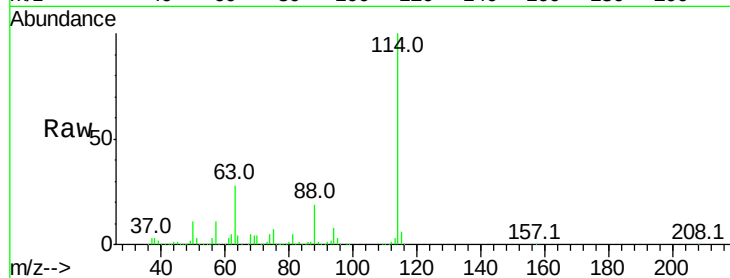

Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

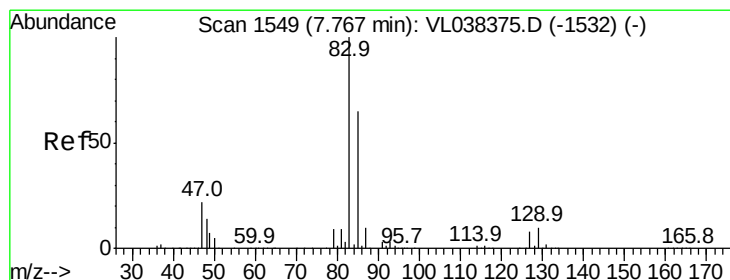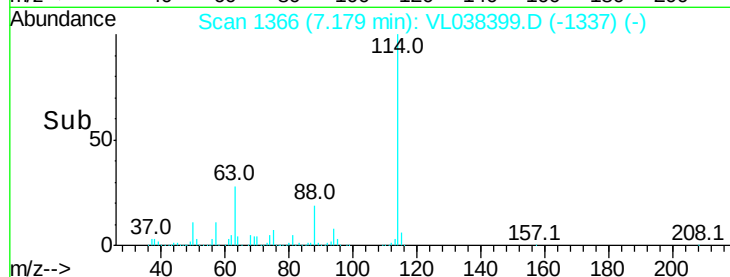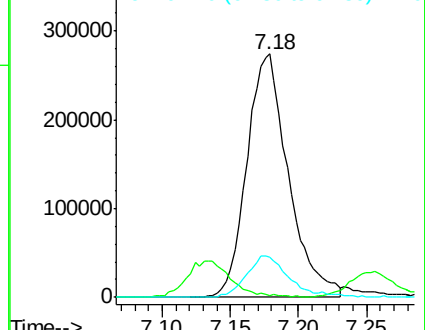

#42

Bromodichloromethane

Concen: 0.04 ppbv

RT: 7.78 min Scan# 1554

Delta R.T. 0.02 min

Lab File: VL038399.D

Acq: 22 Feb 2022 22:10


Tgt Ion: 83 Resp: 6251

Ion Ratio Lower Upper

83 100

85 5.4 52.2 78.4#



127 0.0 6.2 9.4#

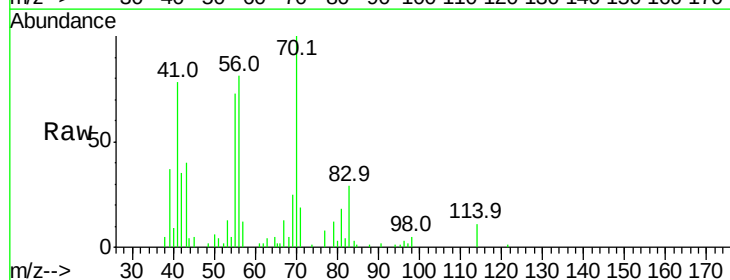


Abundance Ion 83.00 (82.70 to 83.70): VL0

Ion 85.00 (84.70 to 85.70): VL0





Ion 126.90 (126.60 to 127.60): V

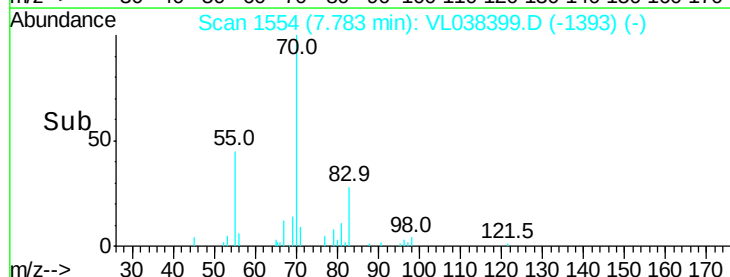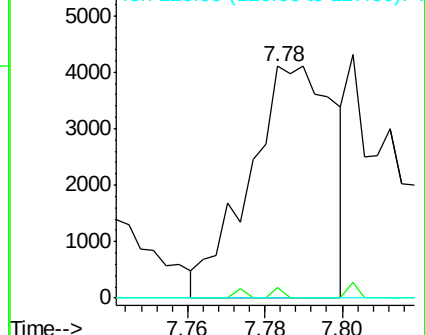

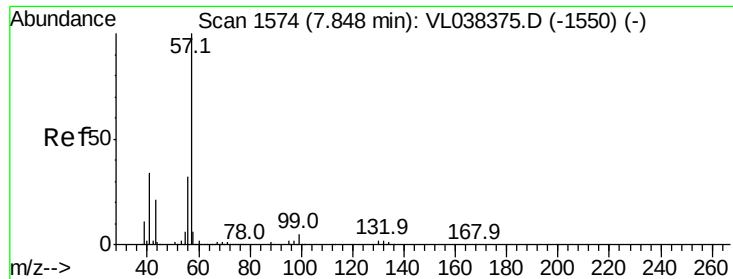




#44
 2,2,4-Trimethylpentane
 Concen: 0.19 ppbv
 RT: 7.88
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 MP-10DL
 Acq: 22 Feb 2022 22:10


Tgt Ion: 57 Resp: 62480
 Ion Ratio Lower Upper
 57 100
 41 0.0 26.6 39.8#
 56 0.0 25.0 37.6#

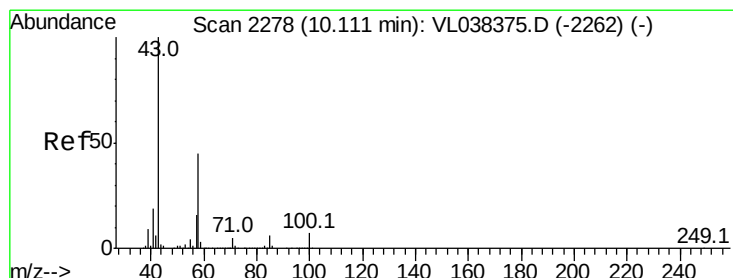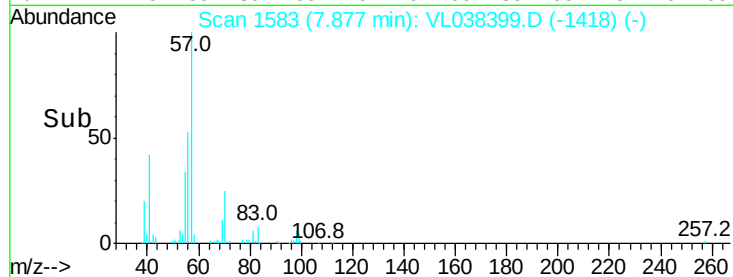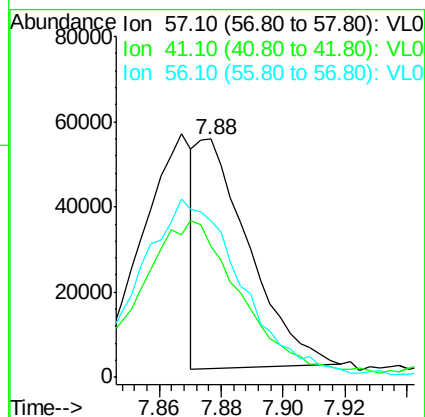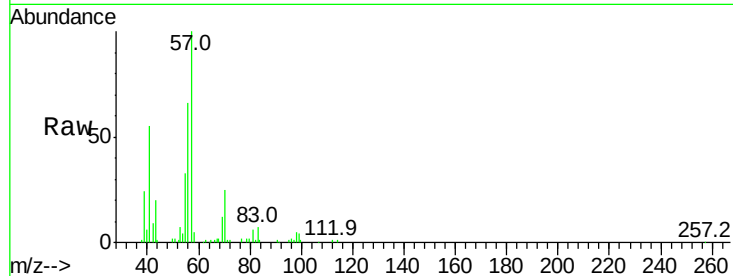

#51
 2-Hexanone
 Concen: 2.20 ppbv
 RT: 10.10 min Scan# 2276
 Delta R.T. -0.01 min
 Lab File: VL038399.D
 Acq: 22 Feb 2022 22:10

Tgt Ion: 43 Resp: 119759
 Ion Ratio Lower Upper
 43 100
 58 0.0 37.4 56.0#
 98 1.9 0.1 0.1#

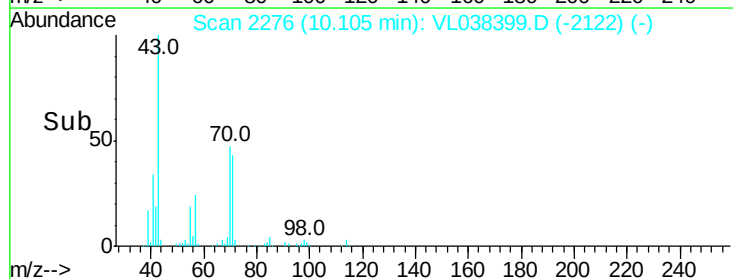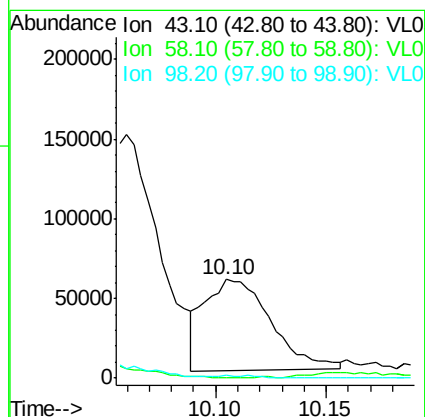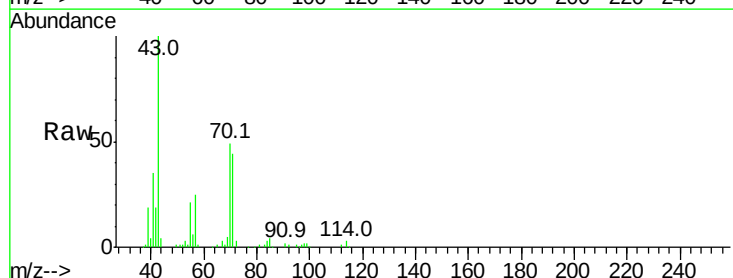

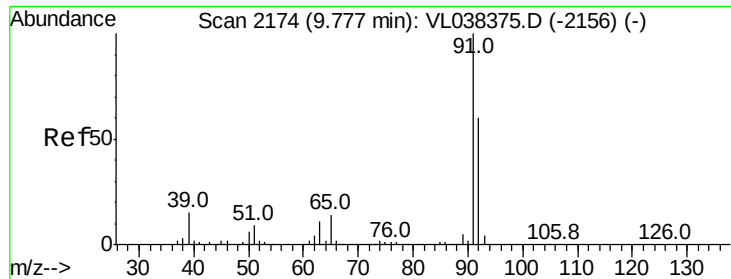

#53

Toluene

Concen: 7.85 ppbv

RT: 9.81 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:





Acq: 22 Feb 2022 22:10 MP-10DL

Tgt Ion: 91 Resp: 1642309

Ion Ratio Lower Upper

91 100

92 59.8 48.2 72.4

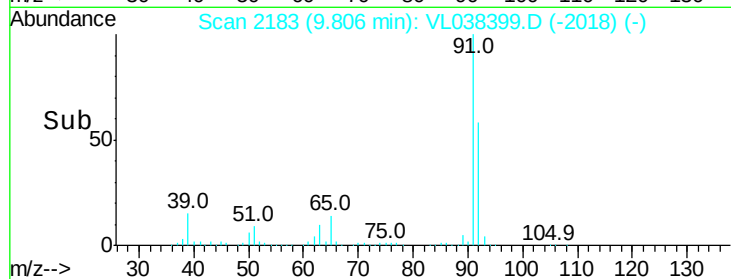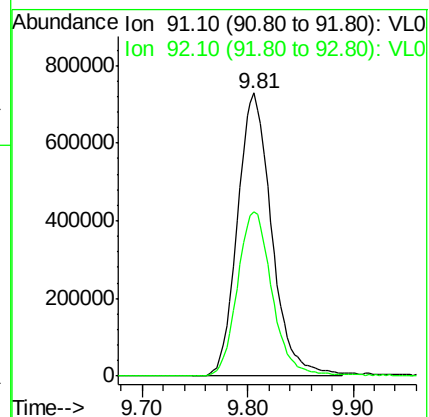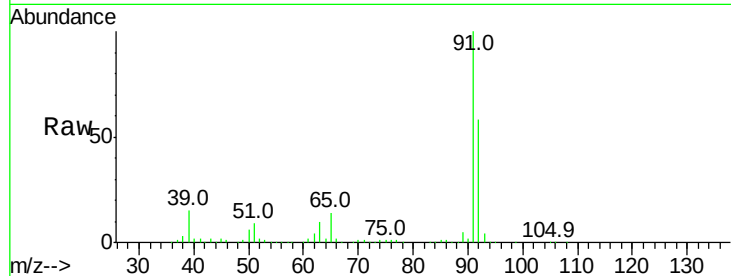

#55

Chlorobenzene-d5

Concen: 10.00 ppbv

RT: 12.08 min Scan# 2891

Delta R.T. 0.03 min

Lab File: VL038399.D

Acq: 22 Feb 2022 22:10




Tgt Ion: 117 Resp: 2046372


Ion Ratio Lower Upper

117 100

82 66.8 54.9 82.3

119 34.5 46.1 69.1#

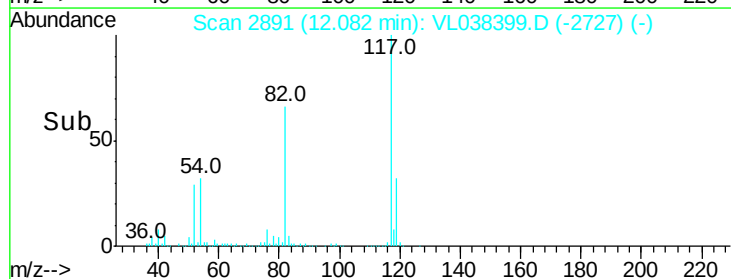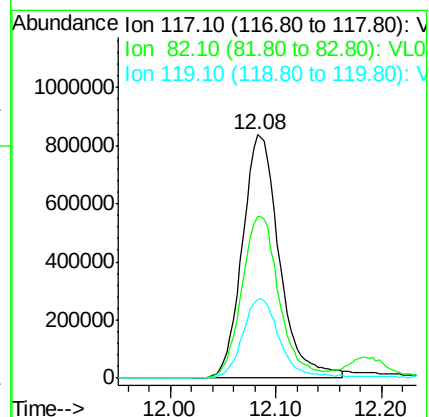

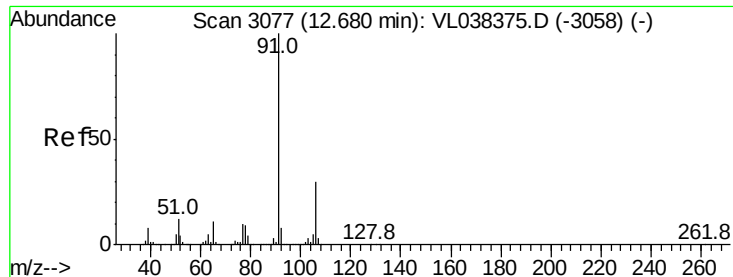

#58

Ethyl Benzene

Concen: 1.26 ppbv

RT: 12.71

Delta R.T. MSVOA_L

Lab File: ClientSampleId :





Acq: 22 Feb 2022 22:10

Tgt Ion: 91 Resp: 351224

Ion Ratio Lower Upper

91 100

106 25.2 24.0 36.0

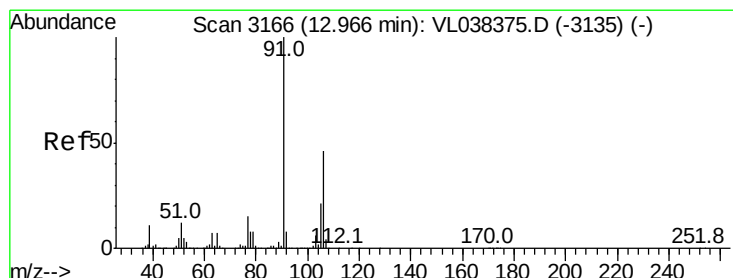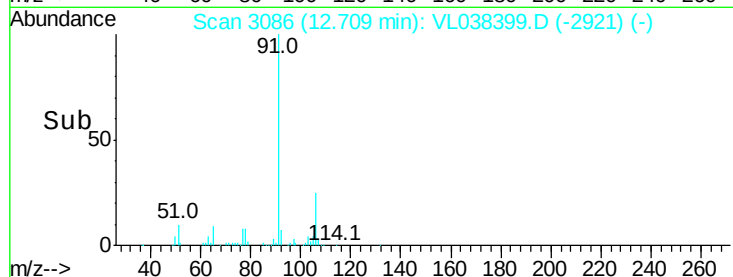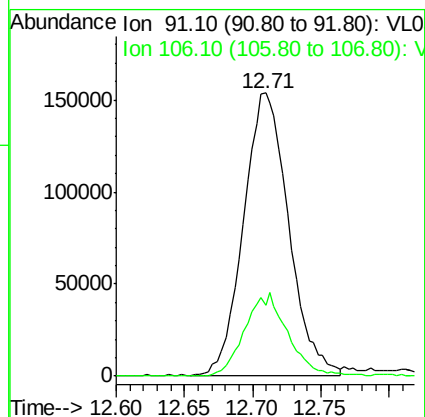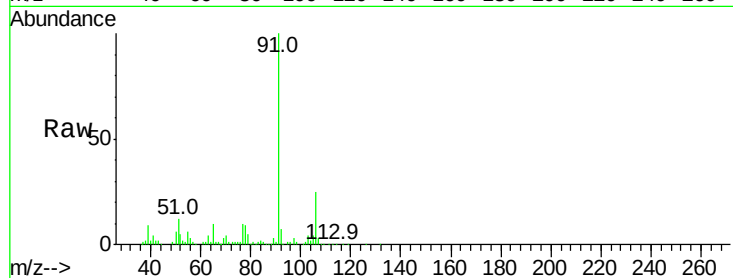

#59

m/p-Xylene

Concen: 3.03 ppbv

RT: 12.96 min Scan# 3165

Delta R.T. -0.00 min

Lab File: VL038399.D




Acq: 22 Feb 2022 22:10


Tgt Ion: 91 Resp: 728000

Ion Ratio Lower Upper

91 100





106 45.1 34.4 51.6

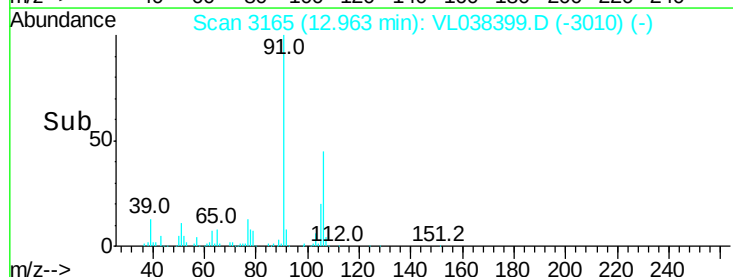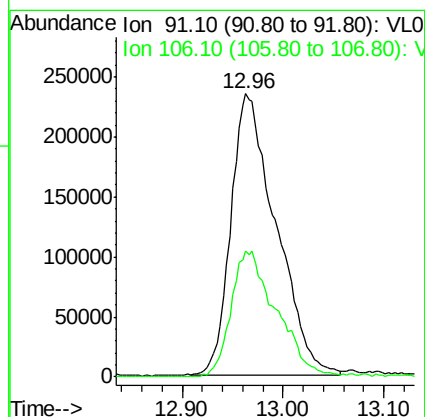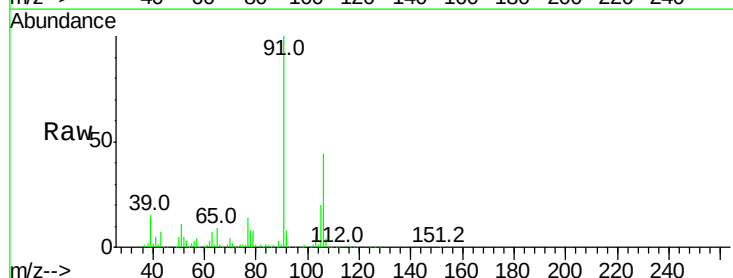






#60
o-Xylene
Concen: 1.38 ppbv
RT: 13.69
Delta R.T. MSVOA_1
Lab File: ClientSampleId :
MP-10DL
Acq: 22 Feb 2022 22:10


Tgt Ion: 91 Resp: 314066
Ion Ratio Lower Upper
91 100
106 44.3 21.9 65.5

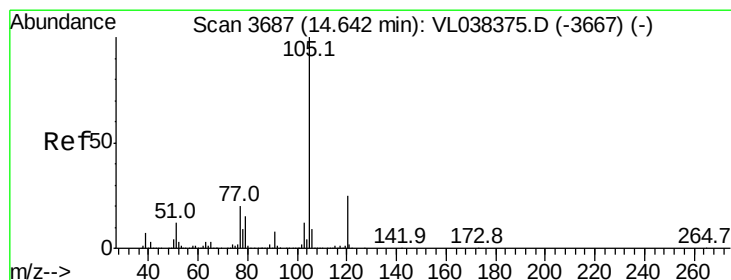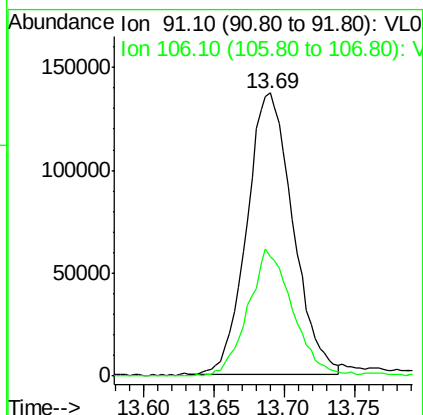

#62
Isopropylbenzene
Concen: 0.25 ppbv
RT: 14.66 min Scan# 3694
Delta R.T. 0.02 min
Lab File: VL038399.D
Acq: 22 Feb 2022 22:10

Tgt Ion: 105 Resp: 77311
Ion Ratio Lower Upper
105 100
120 26.6 20.6 30.8

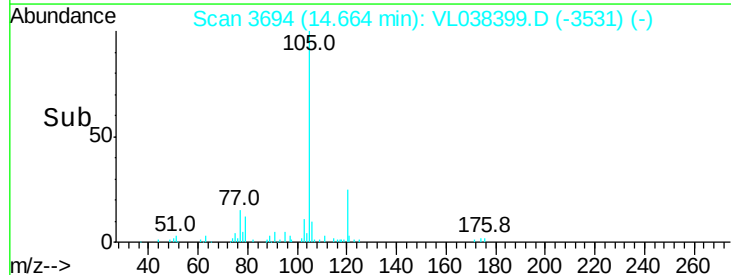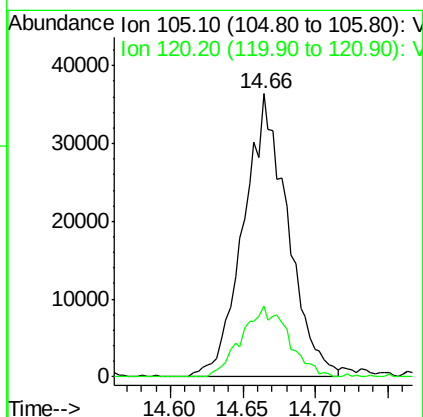



#64

n-propylbenzene

Concen: 0.50 ppbv

RT: 15.56

Delta R.T. MSVOA_L

Lab File: ClientSampleId :


Acq: 22 Feb 2022 22:10

Tgt Ion:120 Resp: 37600

Ion Ratio Lower Upper




120 100

91 534.1 388.1 582.1

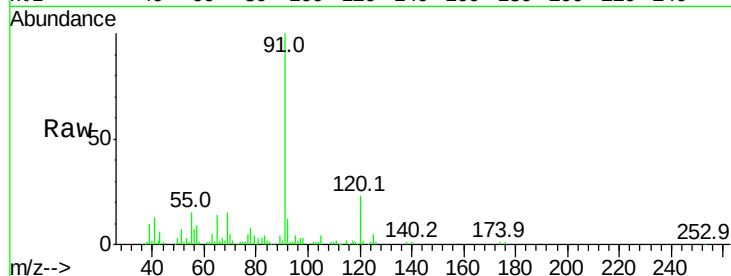

Abundance Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

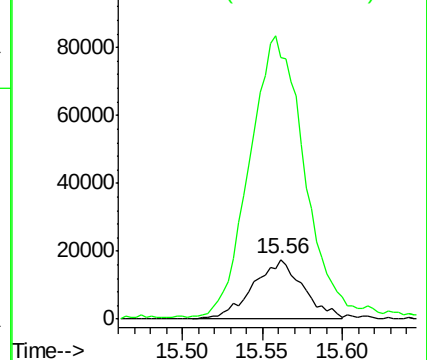

#65

tert-Butylbenzene

Concen: 0.13 ppbv

RT: 16.76 min Scan# 4345

Delta R.T. 0.04 min

Lab File: VL038399.D

Acq: 22 Feb 2022 22:10


Tgt Ion:119 Resp: 35566

Ion Ratio Lower Upper

119 100

91 132.0 68.0 102.0#



134 0.0 15.8 23.8#




Abundance Ion 119.20 (118.90 to 119.90): V

Ion 91.10 (90.80 to 91.80): VL0





Ion 134.20 (133.90 to 134.90): V

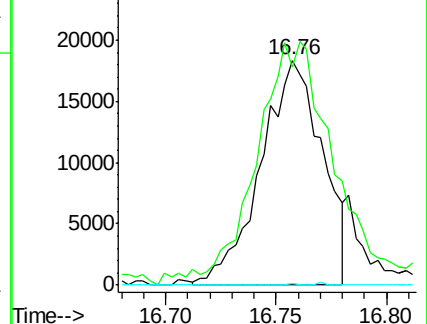

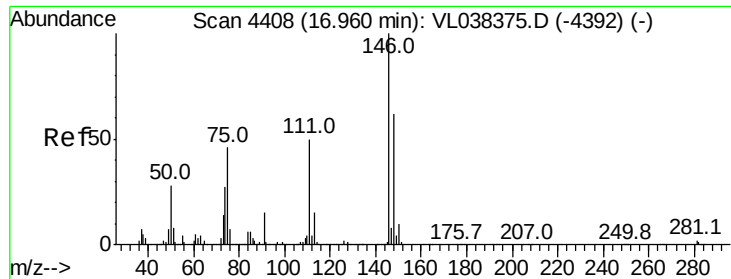




#66
Benzyl Chloride
Concen: 0.03 ppbv
RT: 16.96 min
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 22 Feb 2022 22:10


Tgt Ion: 91 Resp: 463
Ion Ratio Lower Upper
91 100
126 707.3 12.3 18.5#
128 24.8 4.2 6.4#

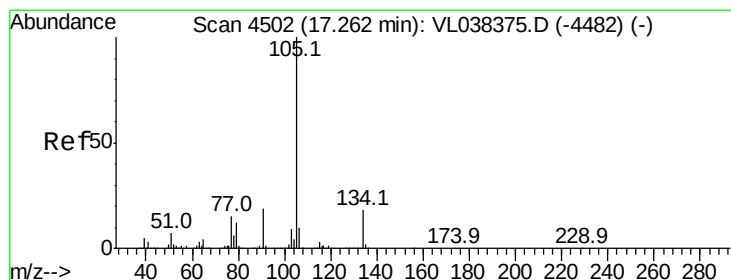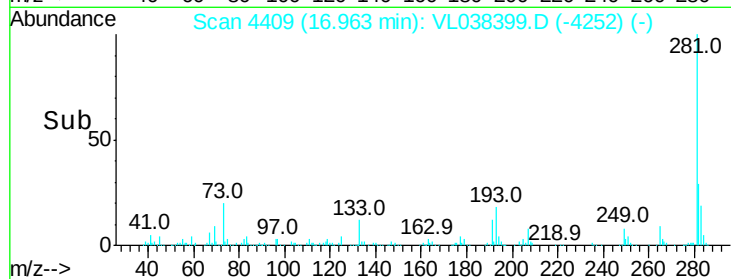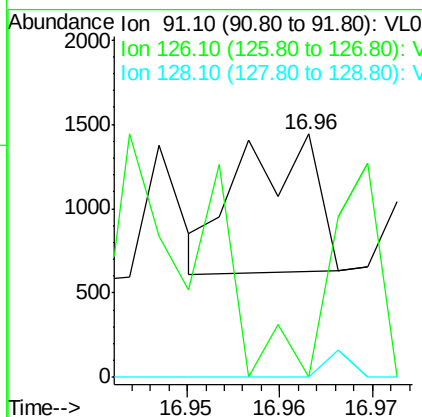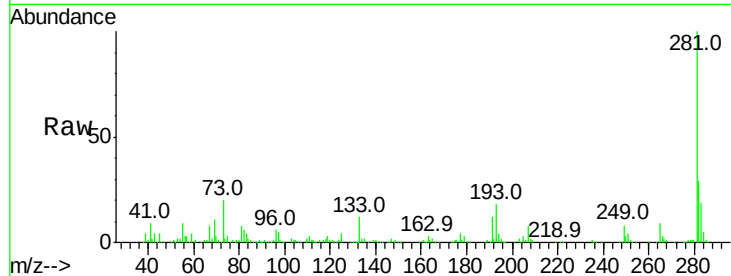

#67
sec-Butylbenzene
Concen: 0.16 ppbv
RT: 17.29 min Scan# 4511
Delta R.T. 0.03 min
Lab File: VL038399.D
Acq: 22 Feb 2022 22:10

Tgt Ion: 105 Resp: 60961
Ion Ratio Lower Upper
105 100
134 19.6 14.6 21.8

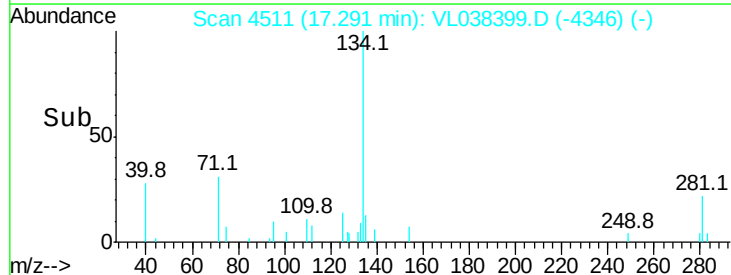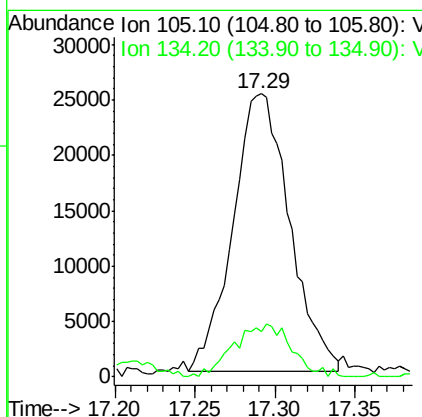

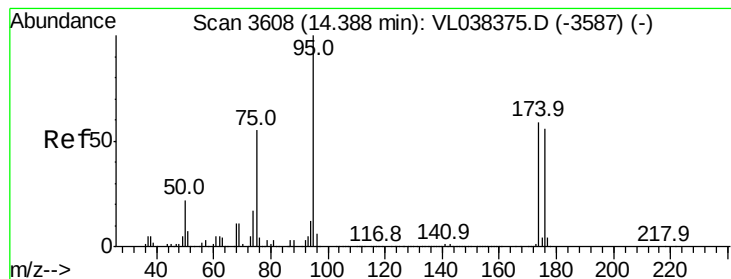

#68

1-Bromo-4-Fluorobenzene

Concen: 9.82 ppbv

RT: 14.41

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 22 Feb 2022 22:10


Tgt Ion: 95 Resp: 1663307

Ion Ratio Lower Upper

95 100

174 63.2 49.0 73.4




175 4.6 3.6 5.4



Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

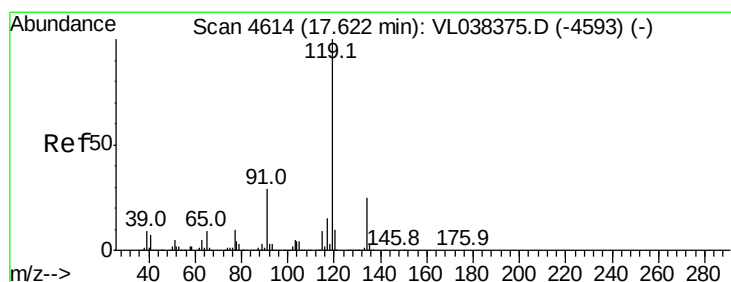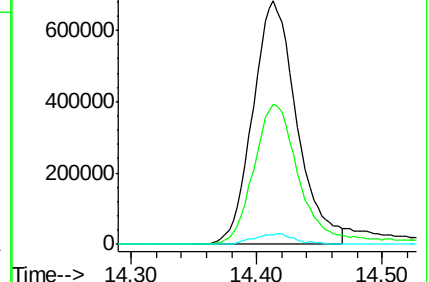

#69

p-Isopropyltoluene

Concen: 0.09 ppbv

RT: 17.65 min Scan# 4622

Delta R.T. 0.03 min

Lab File: VL038399.D

Acq: 22 Feb 2022 22:10


Tgt Ion: 119 Resp: 25036

Ion Ratio Lower Upper

119 100

134 24.3 20.4 30.6



91 36.8 23.8 35.8#

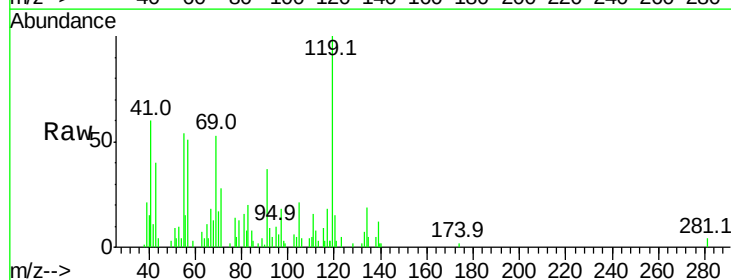


Abundance Ion 119.10 (118.80 to 119.80): V

Ion 134.20 (133.90 to 134.90): V





Ion 91.10 (90.80 to 91.80): VL0

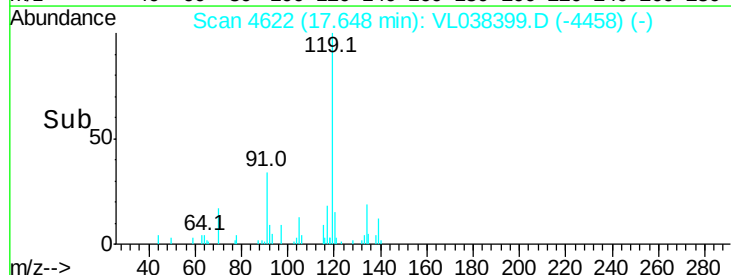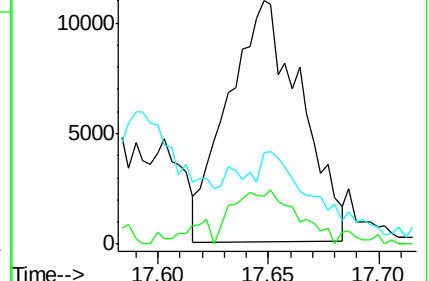






#70
n-Butylbenzene
Concen: 0.14 ppbv
RT: 18.55 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
MP-10DL
Acq: 22 Feb 2022 22:10


Tgt Ion: 91 Resp: 42934
Ion Ratio Lower Upper
91 100
92 57.9 43.1 64.7
134 100.5 17.4 26.0#

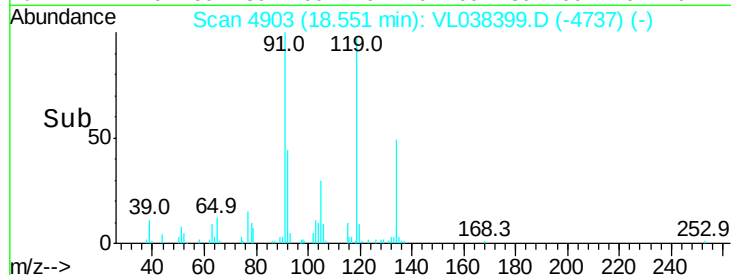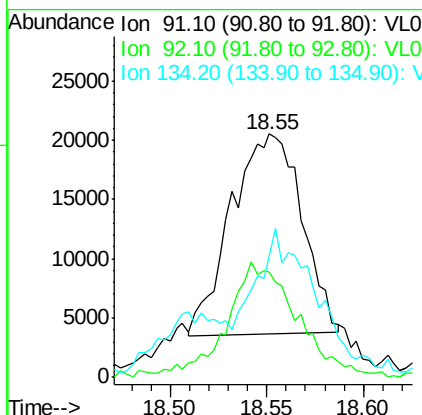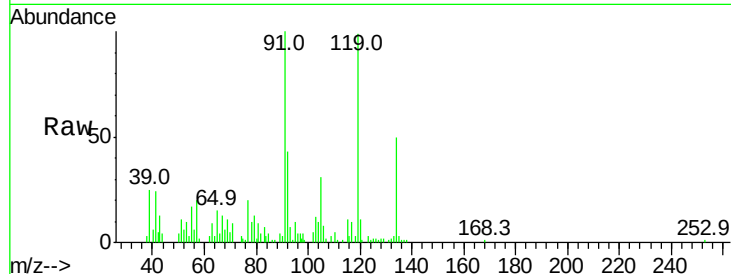

#71
2-Chlorotoluene
Concen: 0.09 ppbv
RT: 15.83 min Scan# 4057
Delta R.T.: 0.41 min
Lab File: VL038399.D
Acq: 22 Feb 2022 22:10

Tgt Ion: 91 Resp: 20072
Ion Ratio Lower Upper
91 100
126 12.6 11.9 47.7

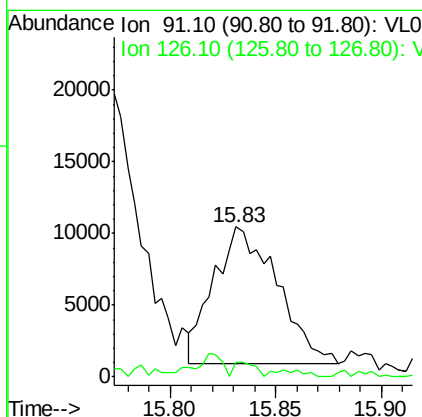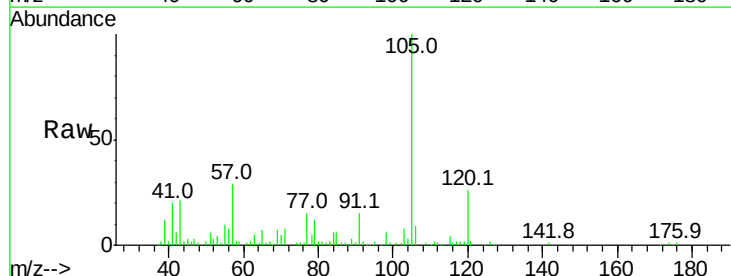



#72

4-Ethyltoluene

Concen: 0.63 ppbv

RT: 15.83

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 22 Feb 2022 22:10

Tgt Ion:105 Resp: 157858


Ion Ratio Lower Upper

105 100

120 31.1 23.4 35.2

91 15.2 10.4 15.6

77 16.8 11.6 17.4






Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

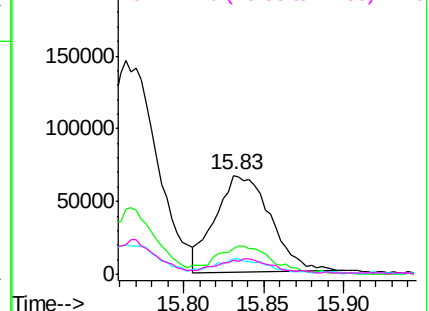

#73

1,3,5-Trimethylbenzene

Concen: 0.59 ppbv

RT: 16.00 min Scan# 4108

Delta R.T. 0.03 min

Lab File: VL038399.D


Acq: 22 Feb 2022 22:10

Tgt Ion:105 Resp: 133593

Ion Ratio Lower Upper



105 100


120 39.2 36.6 55.0



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

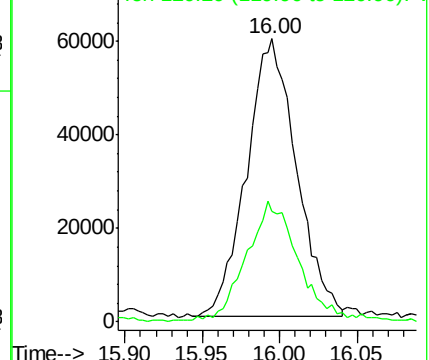



#74
 1,2,4-Trimethylbenzene
 Concen: 1.52 ppbv
 RT: 16.76
 Delta R.T: MSVOA_1
 Lab File: ClientSampleId :
 Acq: 22 Feb 2022 22:10

Tgt Ion:	105	Resp:	365041
Ion Ratio	Lower	Upper	
105	100		
120	41.7	38.2	57.4
91	12.4	42.7	64.1#
77	16.9	18.5	27.7#

