


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL022222\
 Data File : VL038374.D
 Acq On : 22 Feb 2022 3:32
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 Last Update : Tue Feb 22 19:45:51 2022

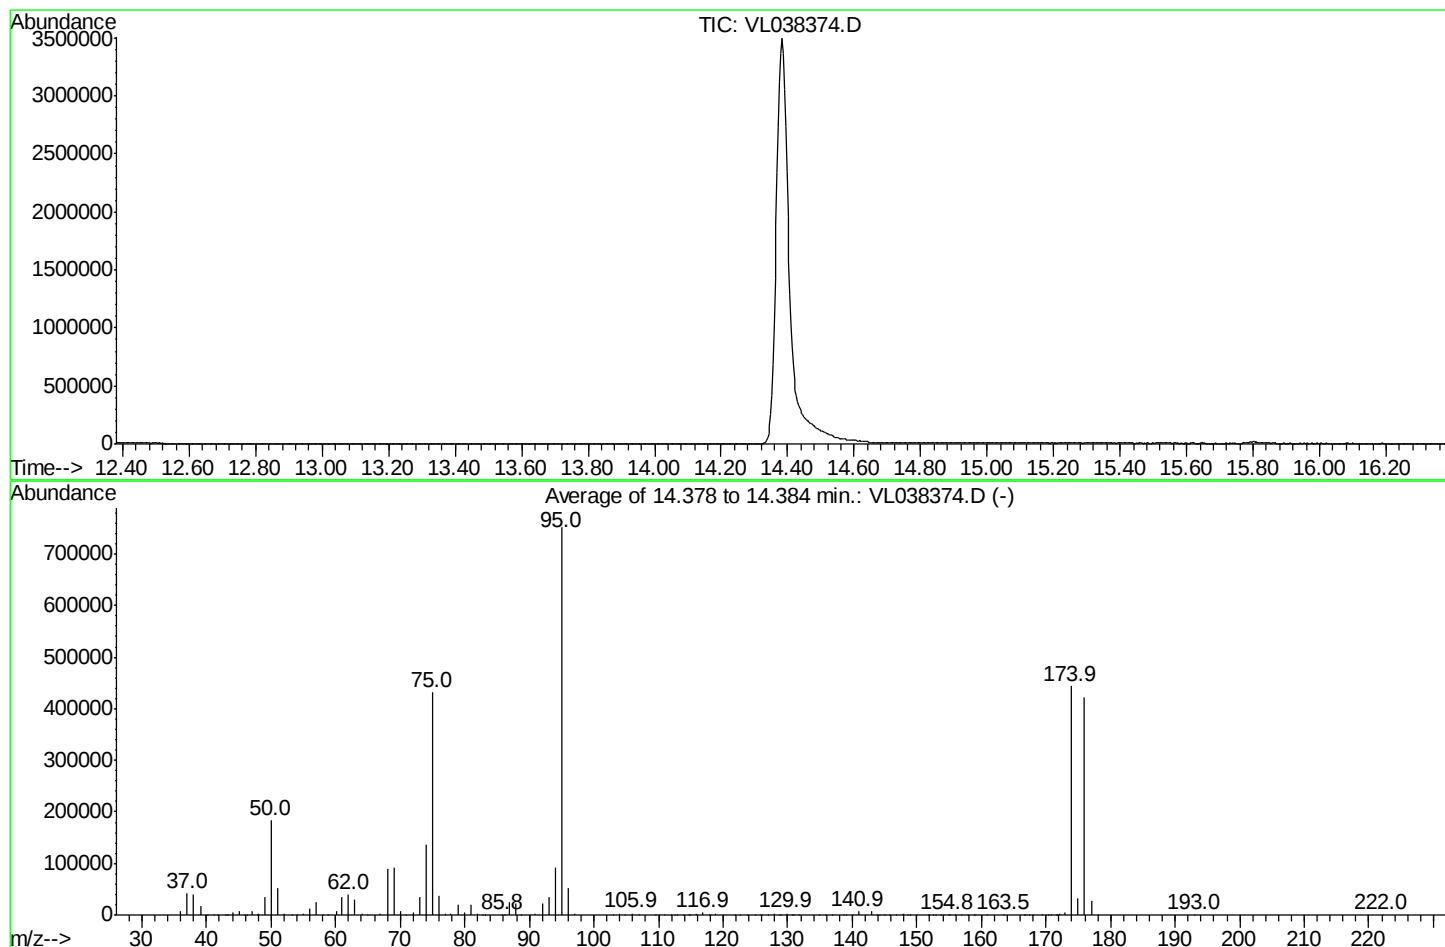

AutoFind: Scans 3605, 3606, 3607; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	183189	PASS
75	95	30	66	57.4	431168	PASS
95	95	100	100	100.0	751680	PASS
96	95	5	9	7.0	52421	PASS
173	174	0.00	2	1.1	4744	PASS
174	95	50	120	59.0	443392	PASS
175	174	4	9	7.3	32402	PASS
176	174	93	101	95.2	422101	PASS
177	176	5	9	6.5	27605	PASS