


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022222\
 Data File : VL038374.D
 Acq On : 22 Feb 2022 3:32
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 Last Update : Tue Feb 22 19:45:51 2022

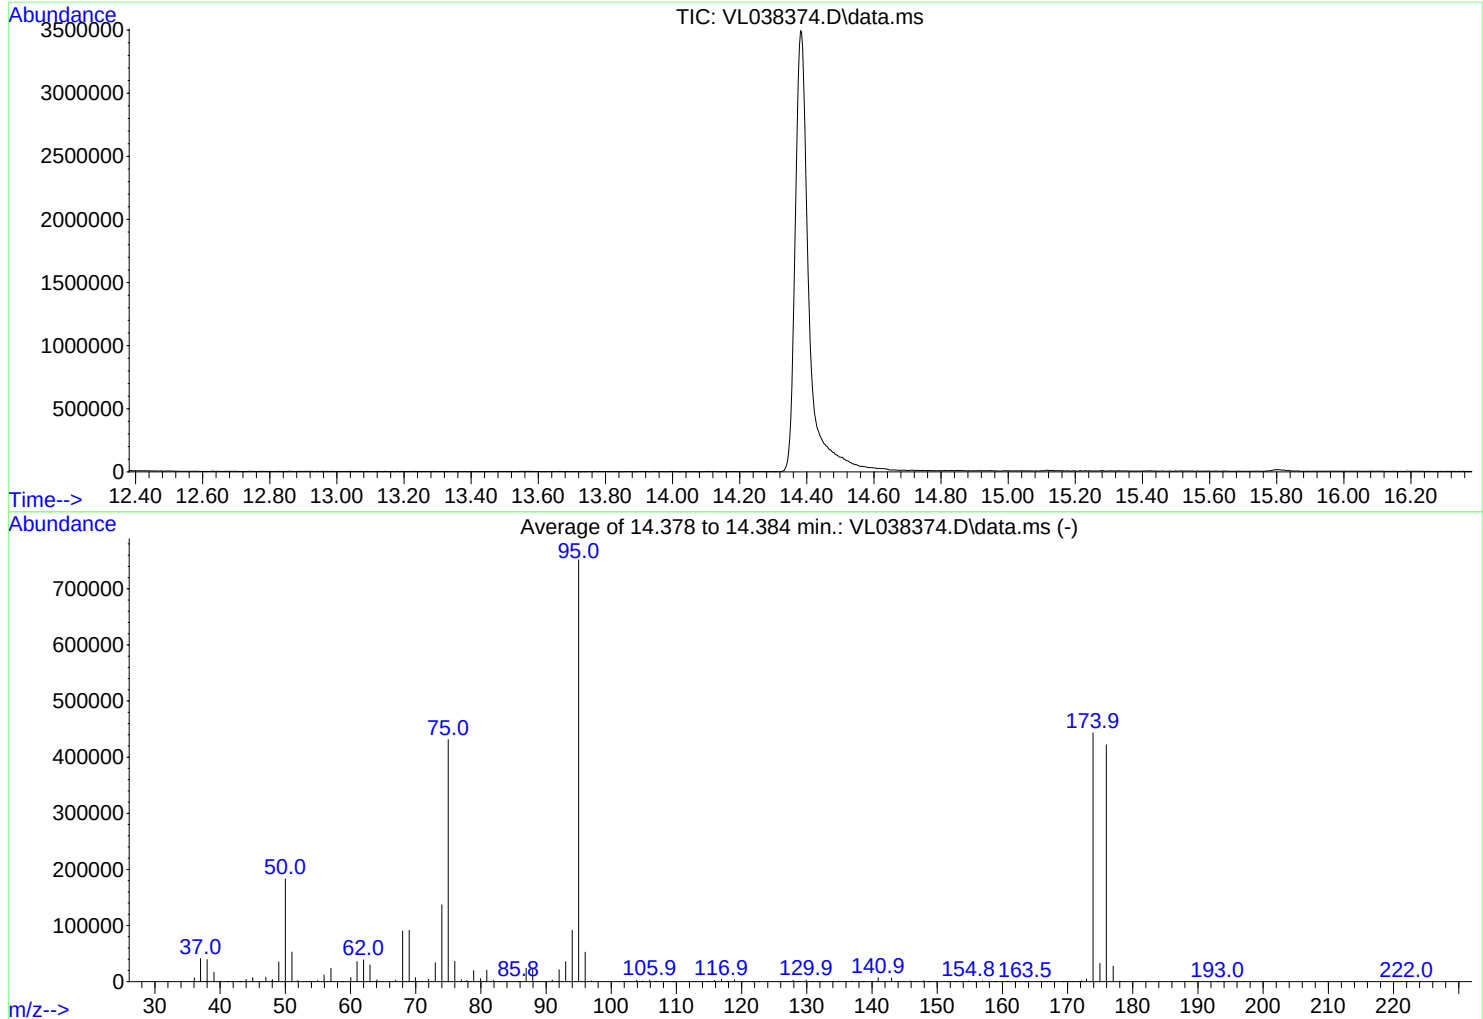

AutoFind: Scans 3605, 3606, 3607; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	183189	PASS
75	95	30	66	57.4	431168	PASS
95	95	100	100	100.0	751680	PASS
96	95	5	9	7.0	52421	PASS
173	174	0.00	2	1.1	4745	PASS
174	95	50	120	59.0	443392	PASS
175	174	4	9	7.3	32403	PASS
176	174	93	101	95.2	422101	PASS
177	176	5	9	6.5	27605	PASS

Average of 14.378 to 14.384 min.: VL038374.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7005	45.00	7253	53.90	54	64.95	711
37.00	41176	45.95	416	54.95	2120	66.90	255
38.00	39237	46.20	155	55.95	11984	68.00	9047
39.05	16949	47.00	8126	57.00	23808	69.00	9155
40.05	897	47.90	1333	58.05	990	69.95	7184
41.10	144	48.05	3300	58.80	66	70.90	411
41.80	99	49.00	34976	60.05	7307	71.95	4234
42.85	317	50.00	183189	61.00	35544	73.00	33677
43.00	147	51.00	52717	62.00	38827	74.00	136992
43.20	148	51.95	1987	63.00	29941	75.00	431168
44.00	4113	53.25	216	64.05	3158	76.00	36117

Average of 14.378 to 14.384 min.: VL038374.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	3401	87.95	22592	104.80	1061	114.85	637
77.85	2257	88.70	320	105.90	2947	115.85	2221
78.90	19688	90.95	2892	106.90	655	116.90	3914
79.95	5387	92.00	21451	109.50	132	117.80	1285
80.90	20597	93.00	35520	110.00	519	118.00	769
81.90	2684	94.00	91549	110.85	573	118.90	3189
82.80	462	95.00	751680	111.85	634	119.95	148
83.20	168	96.00	52421	112.50	176	121.70	75
85.75	585	96.95	1527	112.95	546	122.65	123
86.10	228	102.95	183	113.90	63	123.80	478
86.95	23875	103.90	2687	114.70	270	124.90	207

Average of 14.378 to 14.384 min.: VL038374.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	97	135.90	274	145.85	1038	153.70	101
126.00	180	136.90	1185	146.75	534	154.00	323
126.95	331	138.60	53	147.80	532	154.80	1141
127.90	2380	139.00	292	147.95	1621	155.10	478
128.80	351	139.95	585	148.60	69	155.85	235
128.95	840	140.95	7250	148.90	398	156.95	1034
129.90	2785	142.00	1012	149.90	679	157.90	222
130.80	395	143.00	6389	151.70	149	158.80	539
131.00	707	143.85	480	152.00	113	159.10	452
131.70	126	144.20	60	152.60	205	160.85	789
134.85	873	144.90	649	153.00	248	163.50	56

Average of 14.378 to 14.384 min.: VL038374.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
166.50	168	172.90	4745				
166.80	90	173.90	443392				
167.30	94	174.95	32403				
168.05	196	175.95	422101				
169.30	133	177.00	27605				
169.90	251	178.00	937				
170.25	359	193.00	66				
170.80	480	222.00	81				
171.50	378						
171.80	386						
172.15	1401						

Instrument :

MSVOA_L

ClientSampleId :

BFB