


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022520\
 Data File : VL034666.D
 Acq On : 25 Feb 2020 10:38
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022520AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 25 12:01:27 2020
 Last Update : Tue Feb 25 12:01:27 2020

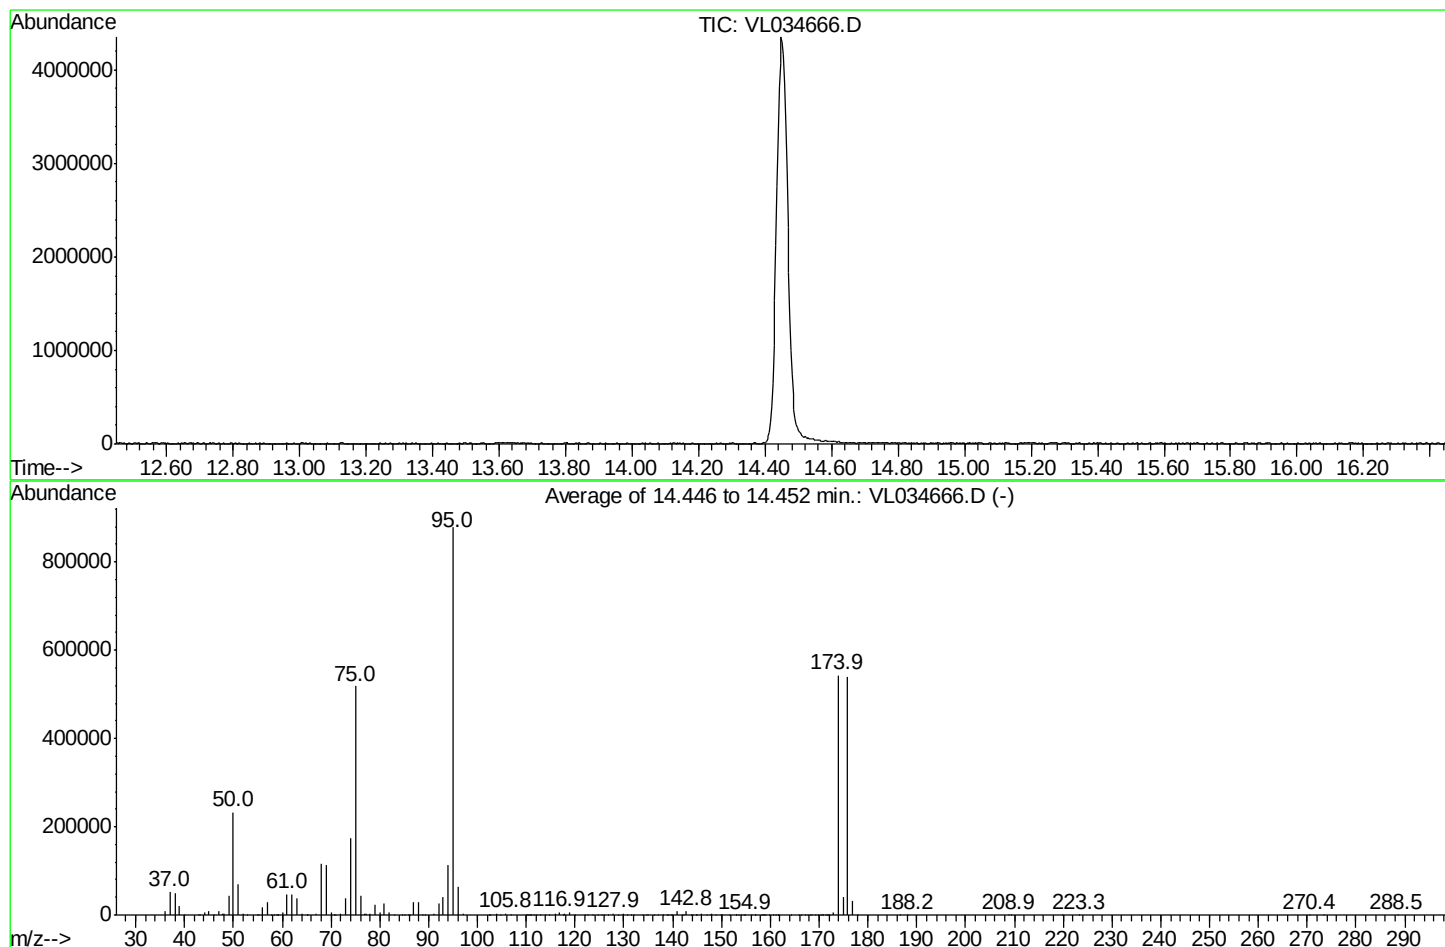

AutoFind: Scans 3626, 3627, 3628; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.5	233009	PASS
75	95	30	66	59.0	517971	PASS
95	95	100	100	100.0	878549	PASS
96	95	5	9	7.2	63024	PASS
173	174	0.00	2	1.1	6134	PASS
174	95	50	120	61.9	543530	PASS
175	174	4	9	7.5	40944	PASS
176	174	93	101	99.5	540864	PASS
177	176	5	9	6.1	32938	PASS