

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022723\
 Data File : VL040236.D
 Acq On : 27 Feb 2023 15:14
 Operator : SY/MD
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Feb 28 00:19:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Feb 28 00:12:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.189	49	972666	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.651	114	2448470	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.471	117	2062465	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	13.783	95	1629524	9.608	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022723\
Data File : VL040236.D
Acq On : 27 Feb 2023 15:14
Operator : SY/MD
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Feb 28 00:19:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Feb 28 00:12:21 2023
Response via : Initial Calibration




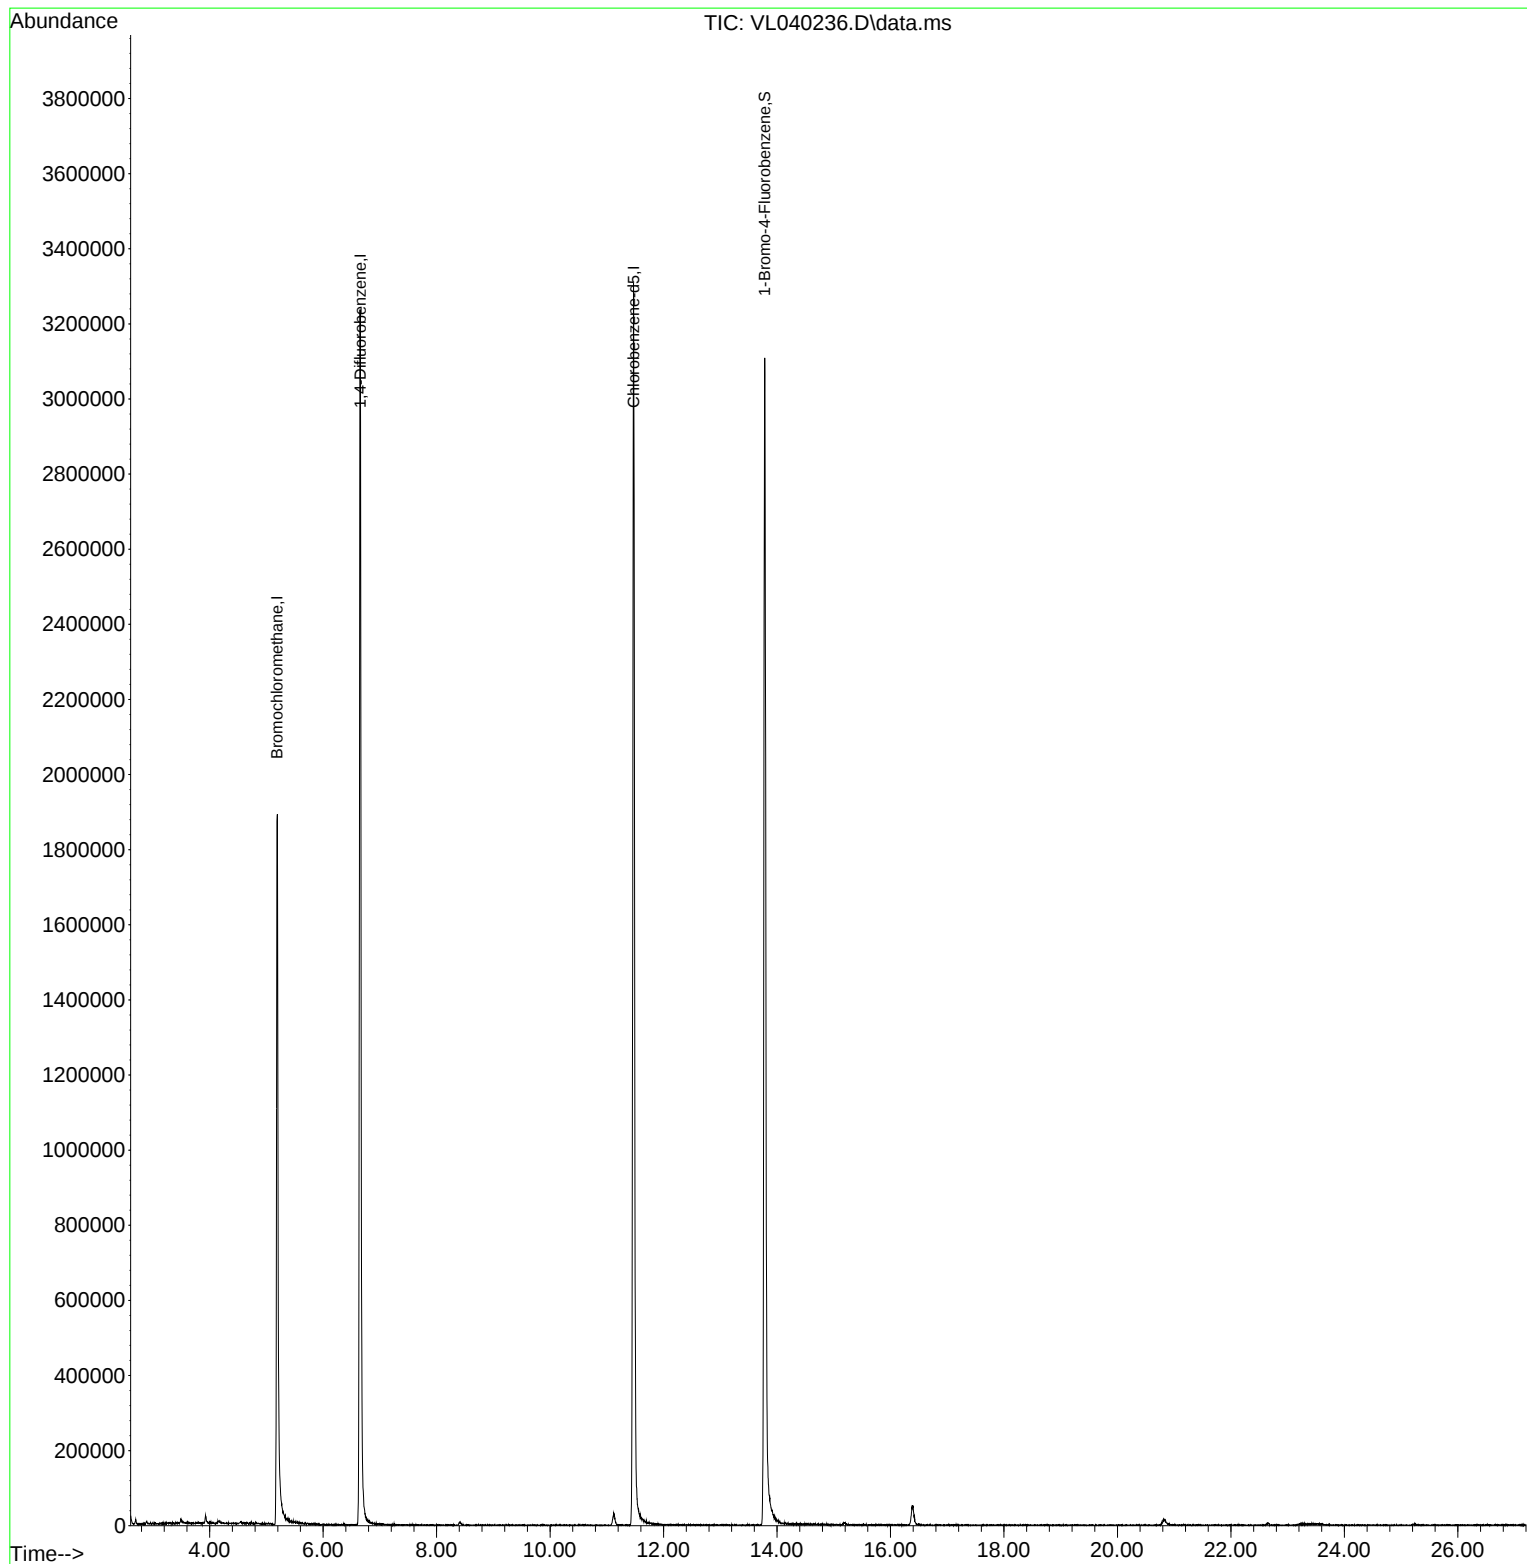


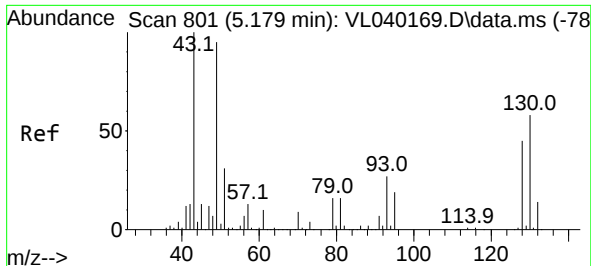

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.189 min Scan# 801
Delta R.T. 0.007 min
Lab File: VL040236.D
Acq: 27 Feb 2023 15:14




Instrument :
MSVOA_L
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 972666
Ion Ratio Lower Upper
49 100
128 47.6 24.1 72.3
130 61.6 30.9 92.8

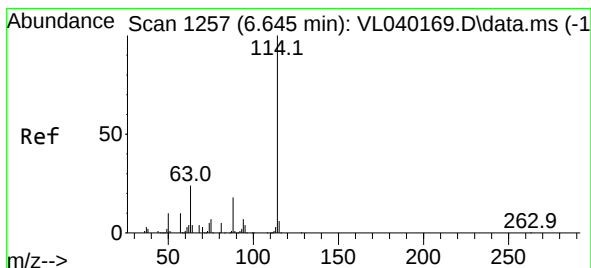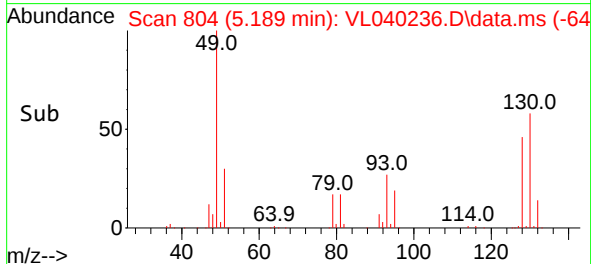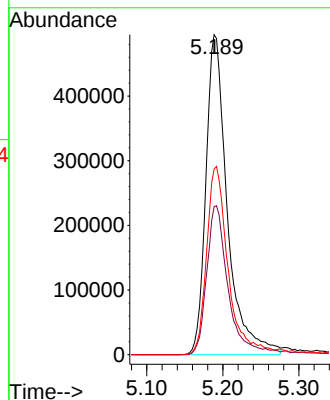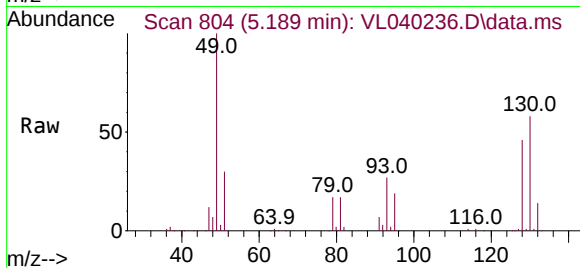

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.651 min Scan# 1259
Delta R.T. 0.003 min
Lab File: VL040236.D
Acq: 27 Feb 2023 15:14

Tgt Ion: 114 Resp: 2448470
Ion Ratio Lower Upper
114 100
63 25.7 20.4 30.6
88 18.1 14.3 21.5


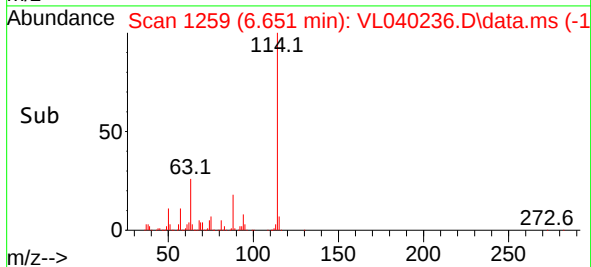
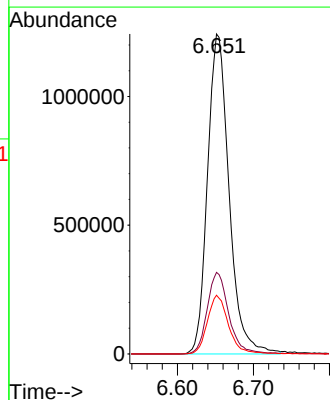
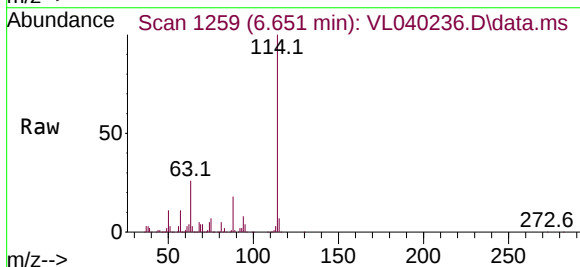


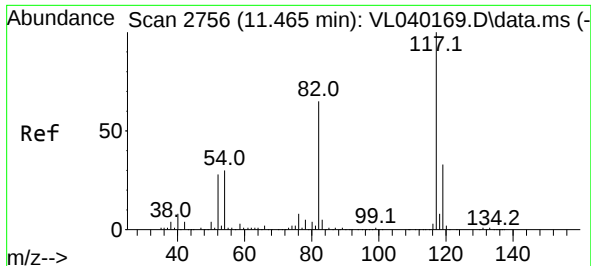

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.471 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL040236.D
Acq: 27 Feb 2023 15:14

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 2062465
Ion Ratio Lower Upper
117 100
82 68.5 53.3 79.9
119 32.8 24.6 37.0

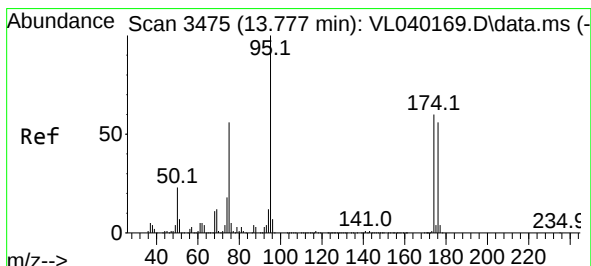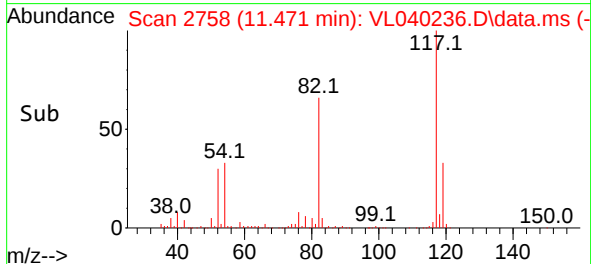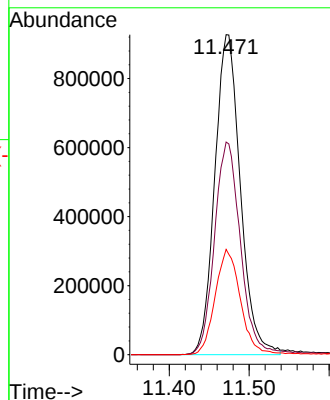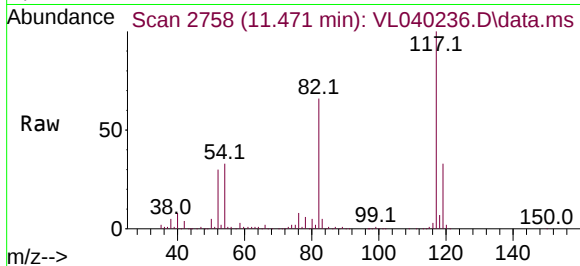

#68
1-Bromo-4-Fluorobenzene
Concen: 9.608 ppbv
RT: 13.783 min Scan# 3477
Delta R.T. 0.007 min
Lab File: VL040236.D
Acq: 27 Feb 2023 15:14

Tgt Ion: 95 Resp: 1629524
Ion Ratio Lower Upper
95 100
174 58.7 48.2 72.2
175 4.2 3.4 5.2

