
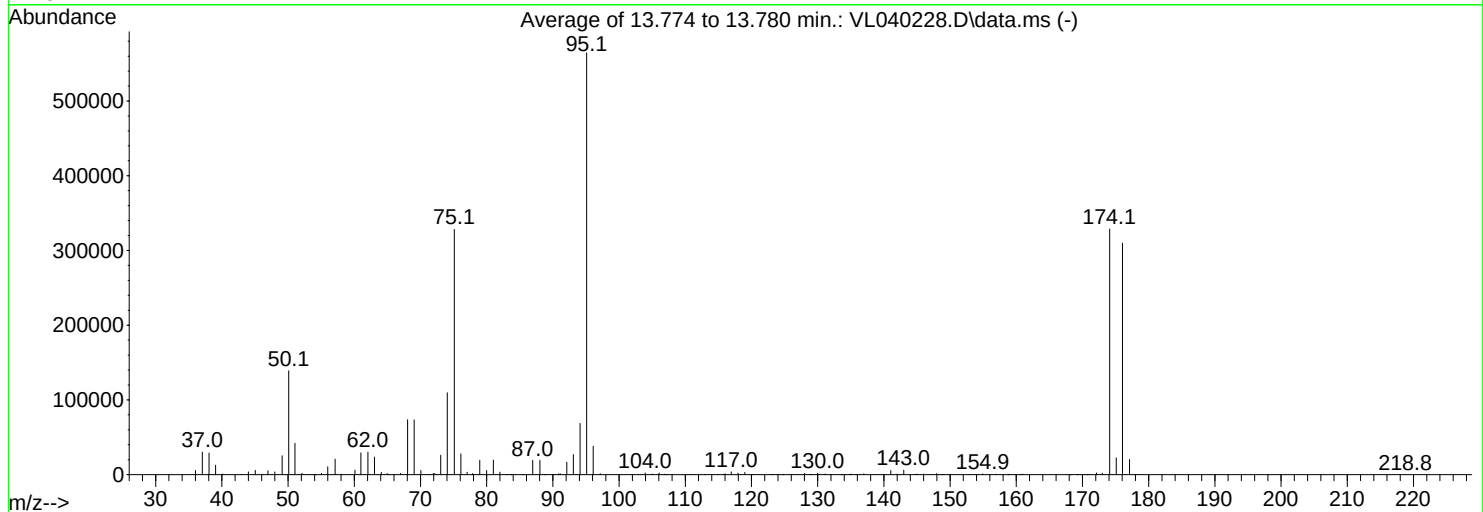


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022723\
Data File : VL040228.D
Acq On : 27 Feb 2023 9:04
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Feb 28 00:12:21 2023

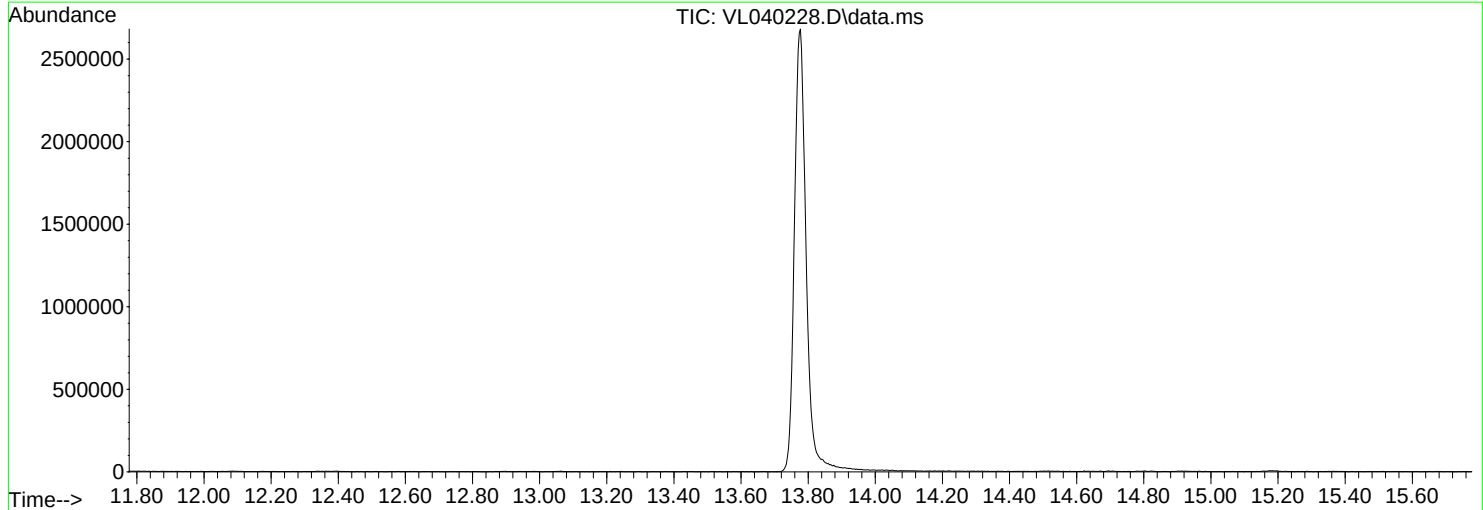

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.6	138883	PASS
75	95	30	66	58.2	328299	PASS
95	95	100	100	100.0	564459	PASS
96	95	5	9	6.8	38149	PASS
173	174	0.00	2	0.6	2046	PASS
174	95	50	120	58.2	328597	PASS
175	174	4	9	6.9	22573	PASS
176	174	93	101	94.3	309845	PASS
177	176	5	9	6.6	20365	PASS

Average of 13.774 to 13.780 min.: VL040228.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	5514	48.00	3684	58.05	720	69.05	7327
37.05	30189	49.10	25373	60.10	5976	70.05	5561
38.05	28856	50.10	138883	61.00	29091	71.30	35
39.05	12634	51.05	41986	62.05	30165	71.95	171
40.10	836	52.10	1681	63.05	23541	72.15	1484
42.90	384	52.95	210	64.10	2992	73.05	25976
44.00	3740	53.80	143	64.95	1423	74.05	109757
45.05	5850	54.10	59	65.20	509	75.10	328299
46.00	582	55.05	1753	66.15	273	76.10	27829
46.20	219	56.00	10532	67.00	1692	77.05	3168
46.95	5064	57.10	20707	68.05	73429	77.90	1541

Average of 13.774 to 13.780 min.: VL040228.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	19373	88.05	19349	102.90	278	113.10	202
80.00	5563	88.80	114	103.95	2313	114.95	462
81.00	19501	90.20	207	105.00	847	115.80	665
82.00	3426	90.85	1111	106.05	2082	116.05	1140
82.90	196	91.10	1305	106.85	549	116.95	3765
83.15	368	92.10	16646	107.10	126	117.95	2197
83.70	104	93.10	26845	109.90	96	119.00	3035
84.30	320	94.10	68589	110.20	186	120.00	57
85.40	126	95.10	564459	110.85	389	123.10	69
86.05	455	96.10	38149	112.05	701	123.85	273
86.95	19008	97.15	1403	112.90	420	124.70	117

Average of 13.774 to 13.780 min.: VL040228.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.05	155	135.05	930	145.00	828	154.95	1160
126.90	152	135.80	185	146.00	886	156.05	152
128.05	1738	136.95	1184	147.15	203	156.95	617
128.85	610	138.95	250	147.95	1327	158.70	75
129.10	234	139.90	439	148.70	95	159.00	416
130.00	2026	141.05	5538	149.05	260	159.80	126
131.10	809	141.95	569	149.80	184	160.60	52
131.90	65	142.20	241	150.05	652	161.00	561
133.60	100	143.00	6035	151.95	255	168.10	114
134.00	82	143.85	137	152.95	342	169.20	68
134.80	352	144.70	162	153.80	175	169.90	97

Average of 13.774 to 13.780 min.: VL040228.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.30	209	218.80	172				
170.70	74						
171.10	170						
172.10	2448						
173.00	2046						
174.10	328597						
175.10	22573						
176.05	309845						
177.10	20365						
178.00	445						
178.20	247						

Instrument :

MSVOA_L

ClientSampleId :

BFB