
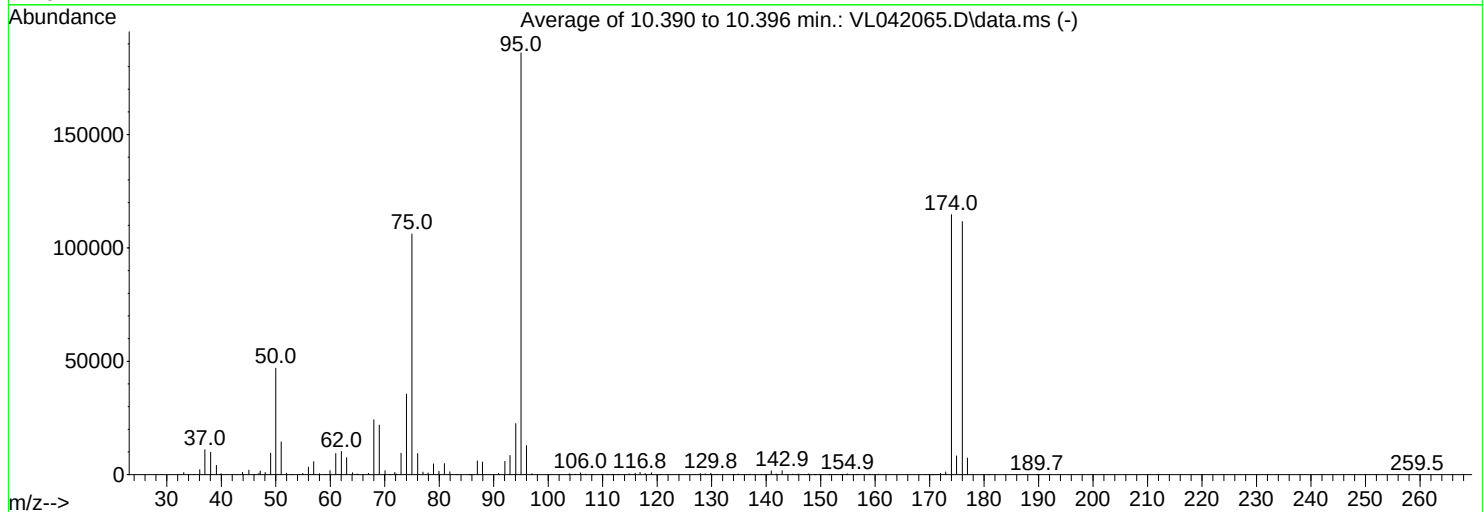


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022725\
Data File : VL042065.D
Acq On : 27 Feb 2025 07:55
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 26 01:08:36 2025

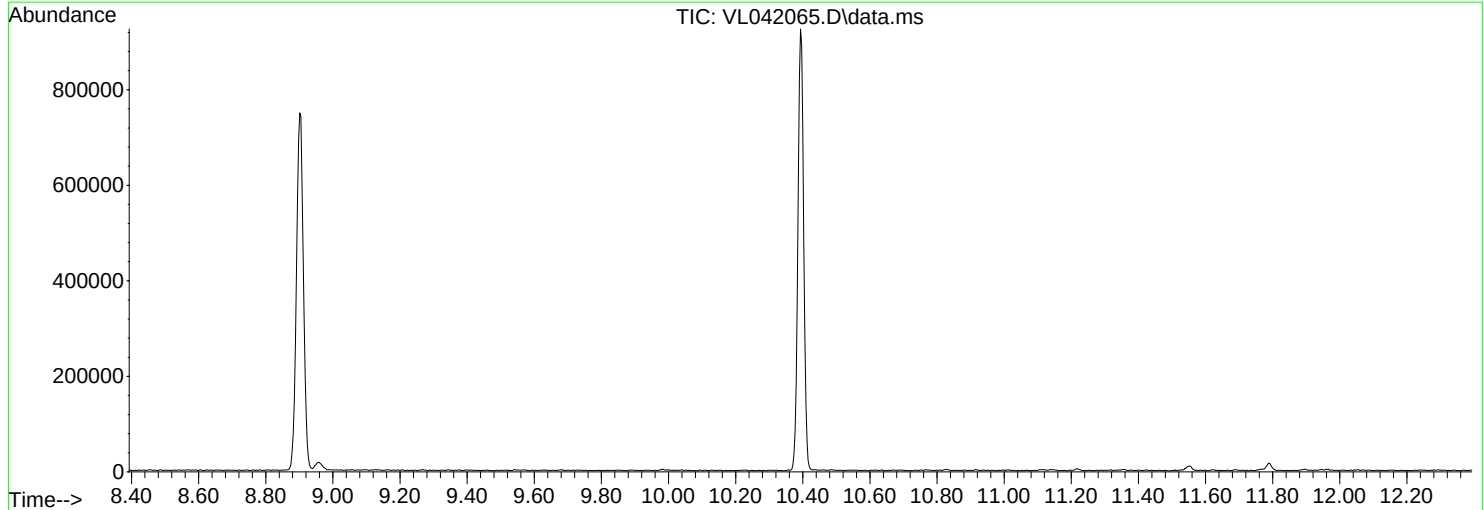

AutoFind: Scans 3183, 3184, 3185; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	46912	PASS
75	95	30	66	57.1	106163	PASS
95	95	100	100	100.0	186069	PASS
96	95	5	9	6.9	12845	PASS
173	174	0.00	2	1.1	1218	PASS
174	95	50	120	61.7	114731	PASS
175	174	4	9	7.2	8269	PASS
176	174	93	101	97.3	111685	PASS
177	176	5	9	6.6	7357	PASS

Average of 10.390 to 10.396 min.: VL042065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	911	46.05	123	56.00	3296	66.10	81
35.05	56	46.90	617	56.95	5753	67.00	55
36.05	2212	47.15	1657	58.00	414	68.00	2418
37.00	10986	48.05	1014	59.10	44	69.00	2185
38.05	9918	49.05	9438	59.95	1789	70.05	1751
39.10	4101	50.00	46912	61.00	9346	71.00	91
39.95	435	51.00	14498	62.05	10216	71.85	987
42.10	44	51.95	661	63.00	7511	72.10	274
42.85	104	53.05	52	64.10	841	73.00	9487
43.90	1002	54.40	77	64.90	264	74.00	35483
45.05	1991	54.95	552	65.10	215	75.00	106163

Average of 10.390 to 10.396 min.: VL042065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	9344	87.95	5586	104.95	185	116.85	975
77.00	1118	90.90	594	105.95	798	117.80	489
77.95	750	92.05	5868	106.90	200	118.95	851
78.95	4751	93.00	8492	108.00	21	120.50	19
79.95	1460	94.05	22533	109.80	54	121.80	46
80.95	4844	95.00	186069	110.90	173	124.00	223
81.95	1295	96.00	12845	111.70	58	126.95	89
83.15	82	97.00	405	112.05	94	127.90	509
85.60	39	100.00	19	112.85	157	128.80	364
85.90	106	103.80	150	114.85	321	129.85	636
87.00	6074	103.95	391	115.95	634	130.95	124

Average of 10.390 to 10.396 min.: VL042065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
134.00	29	142.95	1800	151.60	21	160.60	188
134.70	43	143.75	119	152.65	75	169.20	74
134.90	302	144.85	188	152.95	133	169.85	86
136.40	85	145.60	27	153.70	68	170.50	34
136.80	111	146.00	283	153.95	56	170.70	58
137.00	191	147.05	48	154.80	87	171.00	71
137.80	54	147.60	156	154.95	379	171.20	88
139.10	50	147.80	322	156.05	81	171.60	96
139.80	47	148.90	26	156.60	130	172.00	574
140.95	1704	149.15	59	156.85	161	172.95	1218
141.85	301	149.75	232	159.00	239	174.00	114731

Average of 10.390 to 10.396 min.: VL042065.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.95	8269						
176.00	111685						
176.95	7357						
177.95	236						
180.80	39						
189.70	17						
251.90	23						
259.50	66						

Instrument :

MSVOA_L

ClientSampleId :

BFB