


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL030221\
 Data File : VL036423.D
 Acq On : 2 Mar 2021 9:09
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL021021AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 10 16:04:02 2021
 Last Update : Wed Feb 10 16:04:02 2021

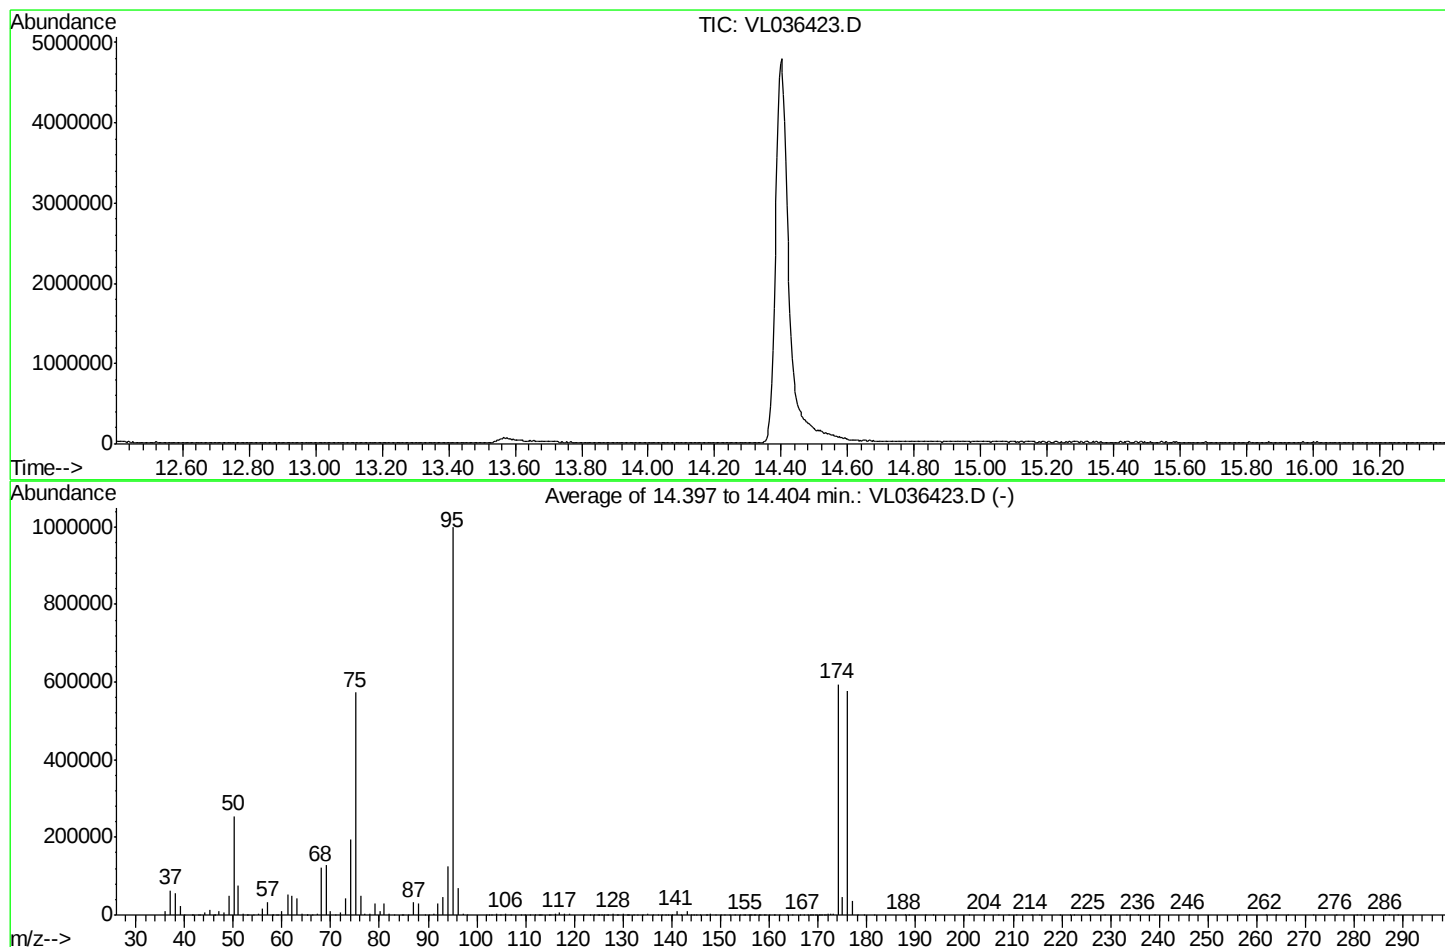

AutoFind: Scans 3611, 3612, 3613; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	254037	PASS
75	95	30	66	57.4	573139	PASS
95	95	100	100	100.0	998485	PASS
96	95	5	9	6.9	68600	PASS
173	174	0.00	2	0.6	3692	PASS
174	95	50	120	59.5	594581	PASS
175	174	4	9	7.7	45525	PASS
176	174	93	101	97.3	578496	PASS
177	176	5	9	6.5	37728	PASS