


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030321\
 Data File : VL036432.D
 Acq On : 3 Mar 2021 8:55
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030321AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 10 16:04:02 2021
 Last Update : Wed Feb 10 16:04:02 2021

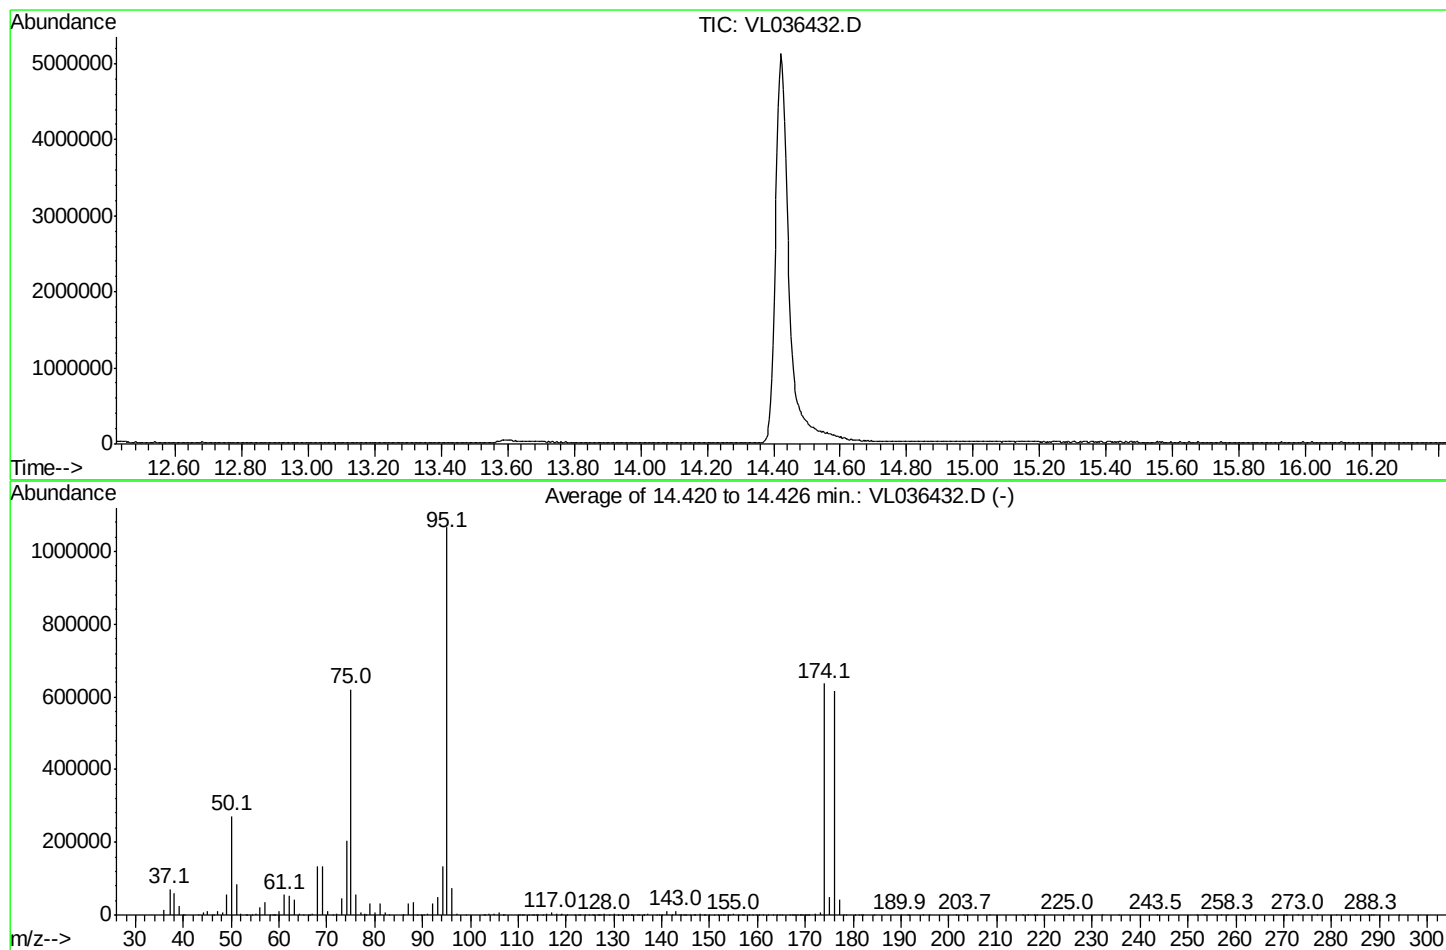

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.5	272341	PASS
75	95	30	66	58.2	620118	PASS
95	95	100	100	100.0	1066240	PASS
96	95	5	9	6.8	72682	PASS
173	174	0.00	2	1.3	8276	PASS
174	95	50	120	59.7	636352	PASS
175	174	4	9	7.7	49290	PASS
176	174	93	101	96.9	616469	PASS
177	176	5	9	7.2	44106	PASS