


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030520\
 Data File : VL034789.D
 Acq On : 5 Mar 2020 9:00
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030420AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Mar 04 06:36:39 2020
 Last Update : Wed Mar 04 06:36:39 2020

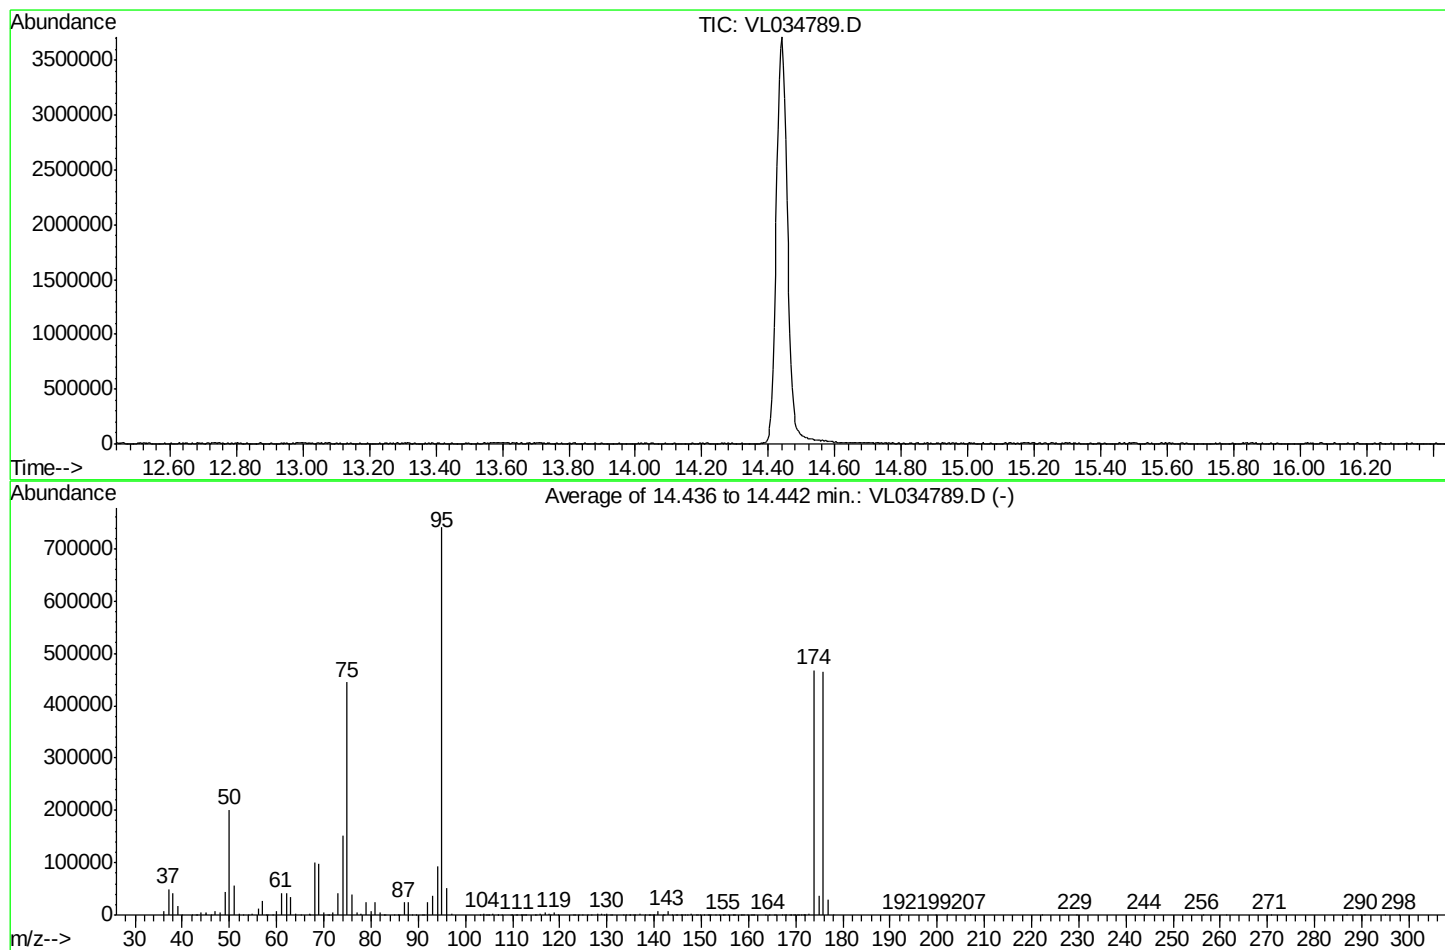

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.2	201173	PASS
75	95	30	66	60.1	445019	PASS
95	95	100	100	100.0	740906	PASS
96	95	5	9	6.9	51330	PASS
173	174	0.00	2	0.7	3452	PASS
174	95	50	120	63.1	467328	PASS
175	174	4	9	7.7	36091	PASS
176	174	93	101	99.5	464810	PASS
177	176	5	9	6.4	29970	PASS