


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030619\
Data File : VL033239.D
Acq On : 6 Mar 2019 1:19
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030619AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Mar 06 08:43:44 2019
Last Update : Wed Mar 06 08:43:44 2019

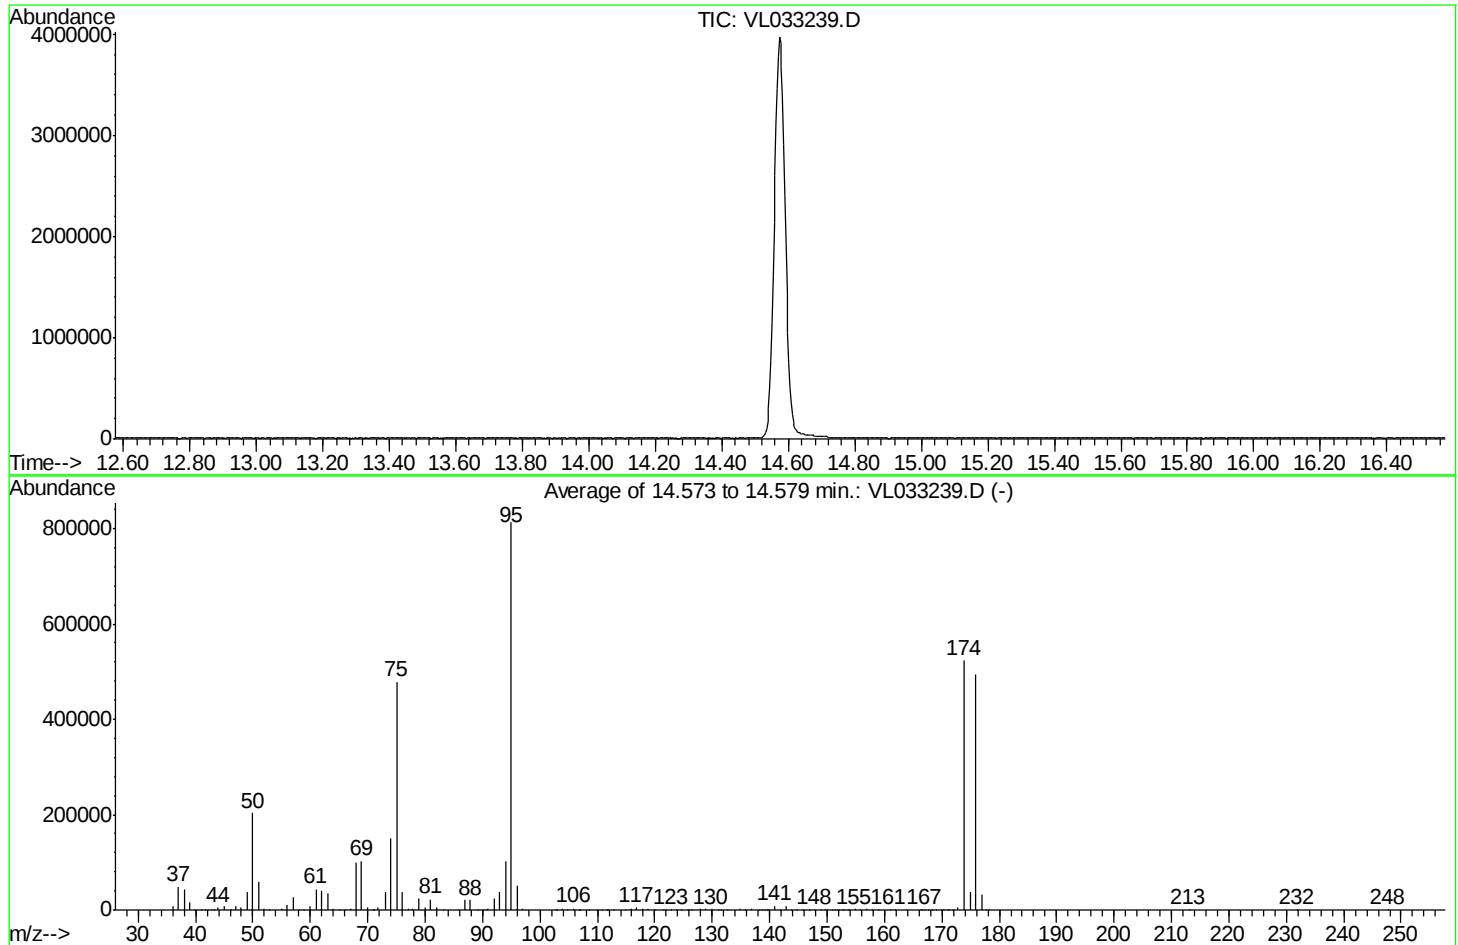

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	203178	PASS
75	95	30	66	58.9	478784	PASS
95	95	100	100	100.0	813056	PASS
96	95	5	9	6.4	51720	PASS
173	174	0.00	2	0.9	4828	PASS
174	95	50	120	64.2	522346	PASS
175	174	4	9	7.1	37248	PASS
176	174	93	101	94.4	492842	PASS
177	176	5	9	6.5	31925	PASS