


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031119\
 Data File : VV009583.D
 Acq On : 11 Mar 2019 08:45
 Operator : SY/MD
 Sample : BFB74
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
 Title : VOC Analysis
 Last Update : Mon Mar 11 04:48:46 2019

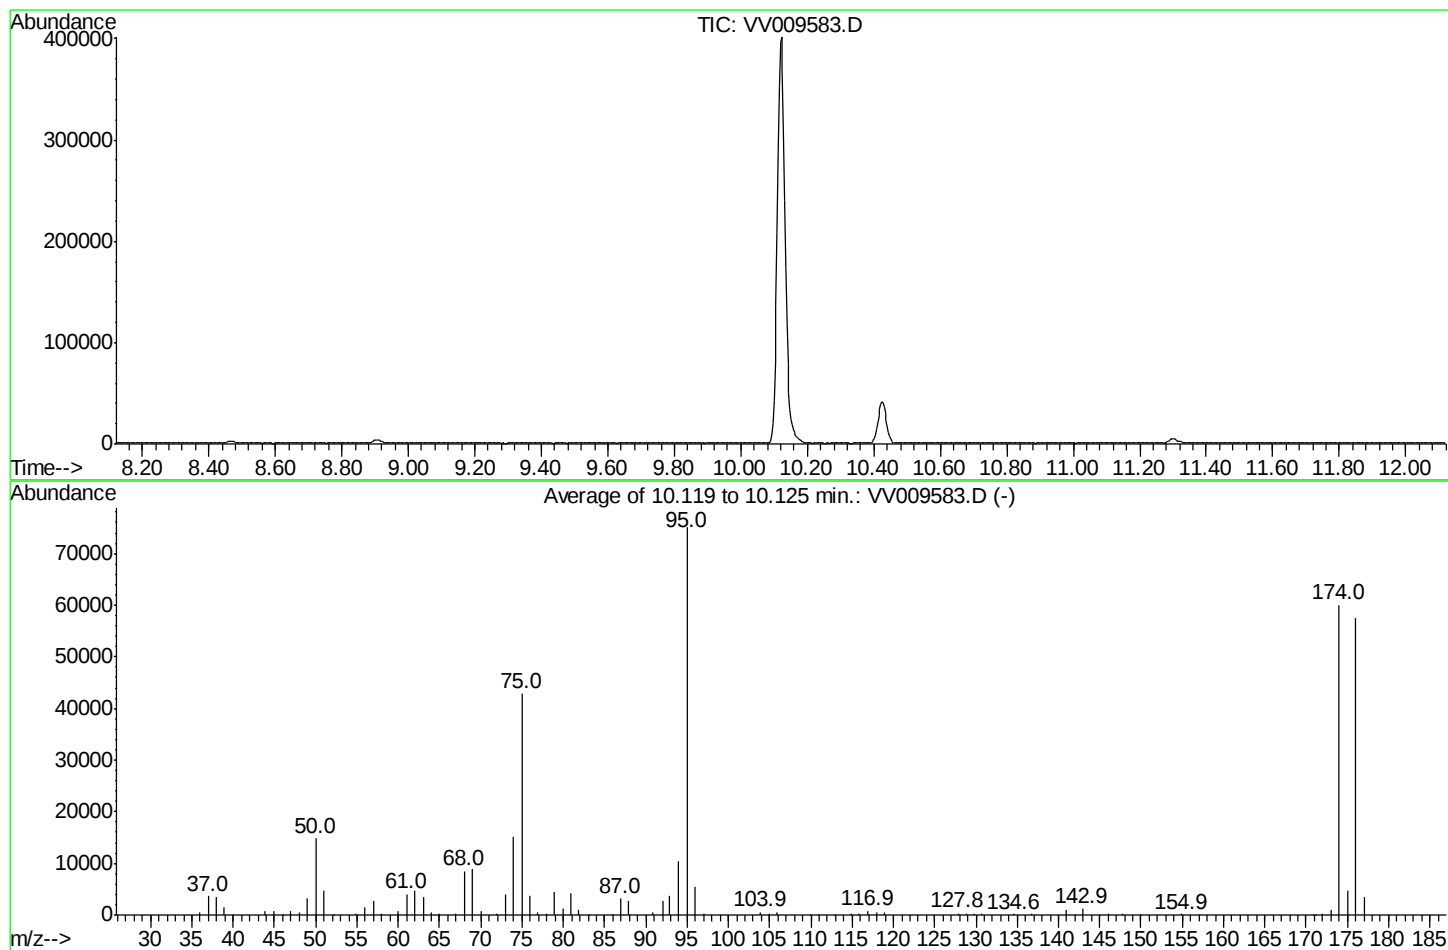

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	14828	PASS
75	95	30	80	57.0	42786	PASS
95	95	100	100	100.0	75074	PASS
96	95	5	9	7.3	5466	PASS
173	174	0.00	2	1.7	1043	PASS
174	95	50	120	79.9	60010	PASS
175	174	5	9	7.9	4723	PASS
176	174	95	101	95.9	57565	PASS
177	176	5	9	6.1	3505	PASS