


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030819\
 Data File : VL033255.D
 Acq On : 8 Mar 2019 12:08
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030819AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Sat Mar 09 03:32:03 2019
 Last Update : Sat Mar 09 03:32:03 2019

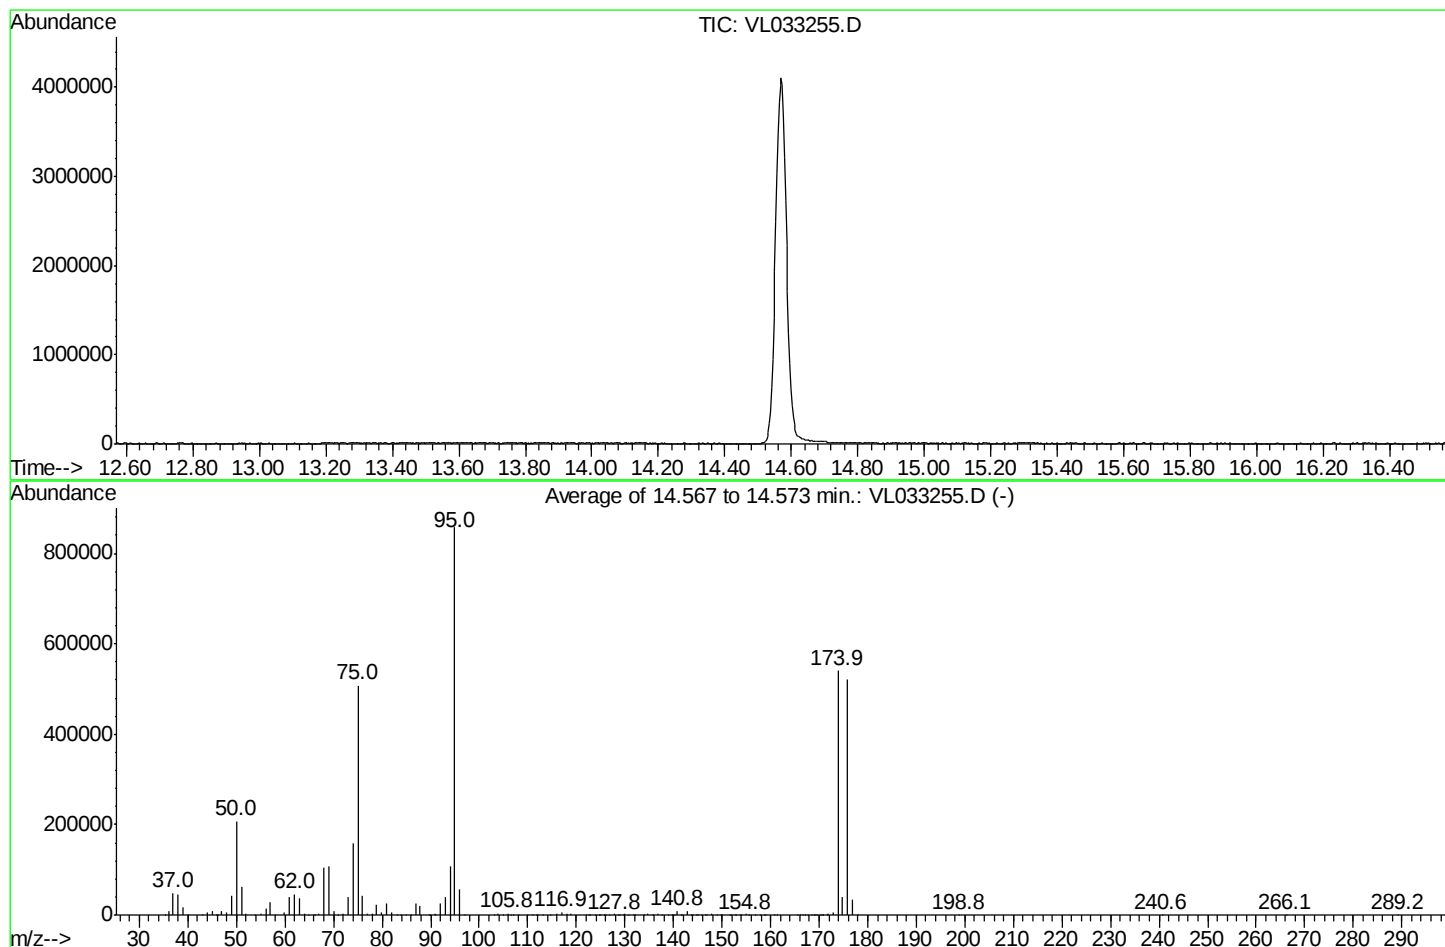

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	207061	PASS
75	95	30	66	59.1	507242	PASS
95	95	100	100	100.0	857621	PASS
96	95	5	9	6.8	58072	PASS
173	174	0.00	2	0.9	4652	PASS
174	95	50	120	63.1	540842	PASS
175	174	4	9	7.2	38800	PASS
176	174	93	101	96.2	520106	PASS
177	176	5	9	6.5	33952	PASS