


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030822\
 Data File : VL038552.D
 Acq On : 8 Mar 2022 10:30
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030822AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 Last Update : Tue Feb 22 19:45:51 2022

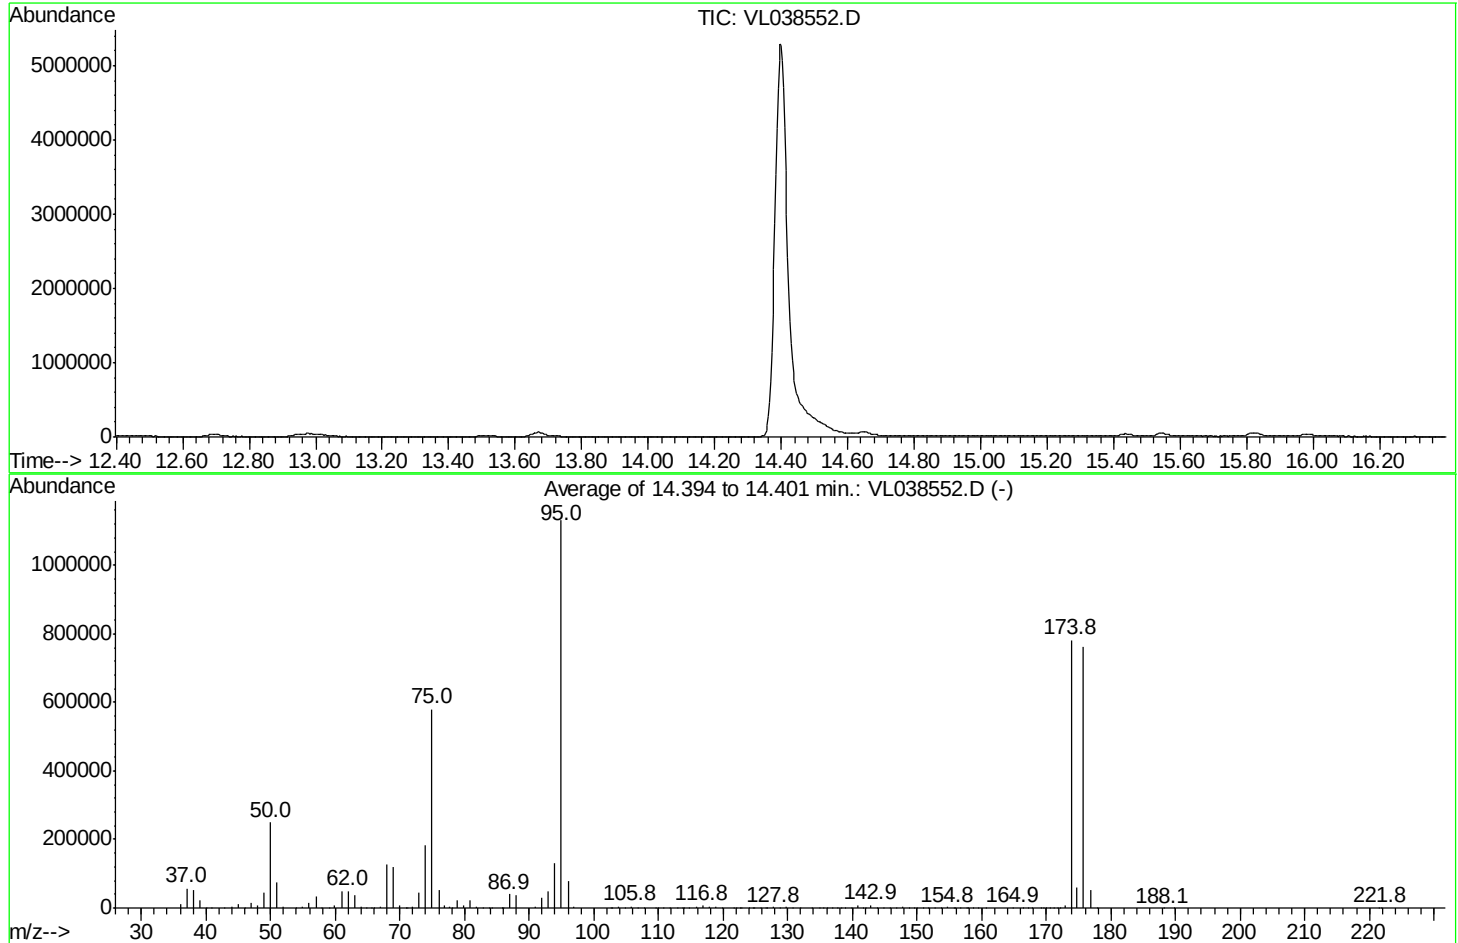

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	248960	PASS
75	95	30	66	51.3	580352	PASS
95	95	100	100	100.0	1131178	PASS
96	95	5	9	6.9	77826	PASS
173	174	0.00	2	1.1	8794	PASS
174	95	50	120	69.1	781994	PASS
175	174	4	9	7.8	60685	PASS
176	174	93	101	97.3	760512	PASS
177	176	5	9	6.8	51488	PASS