
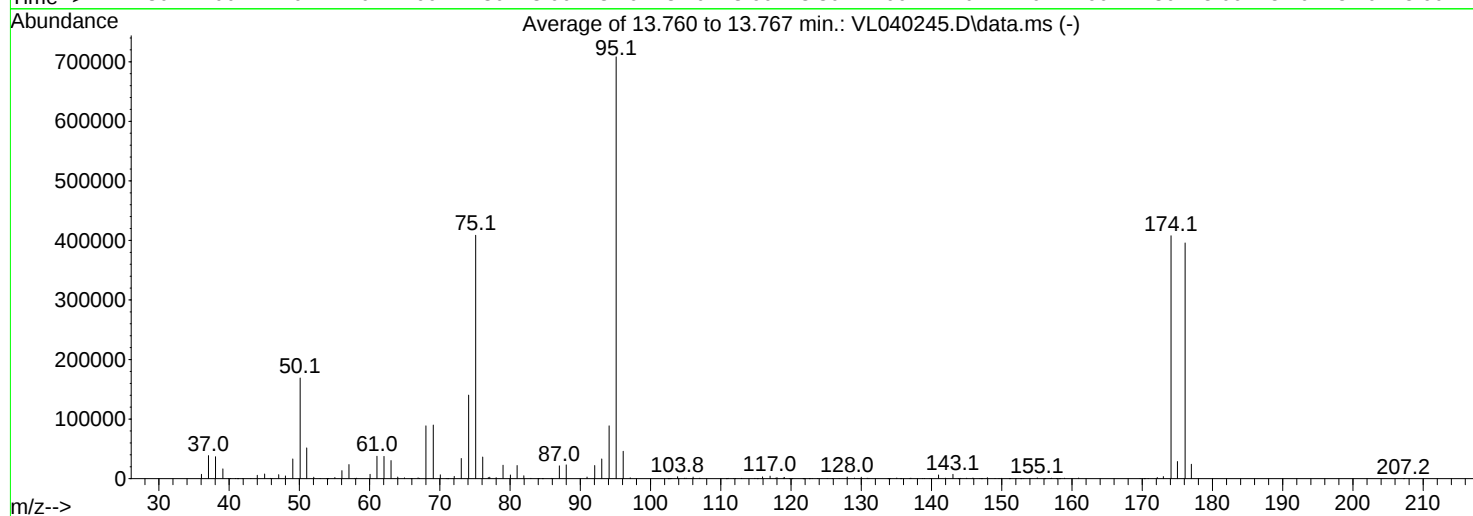


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030823\
Data File : VL040245.D
Acq On : 8 Mar 2023 8:40
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Mar 01 04:21:39 2023

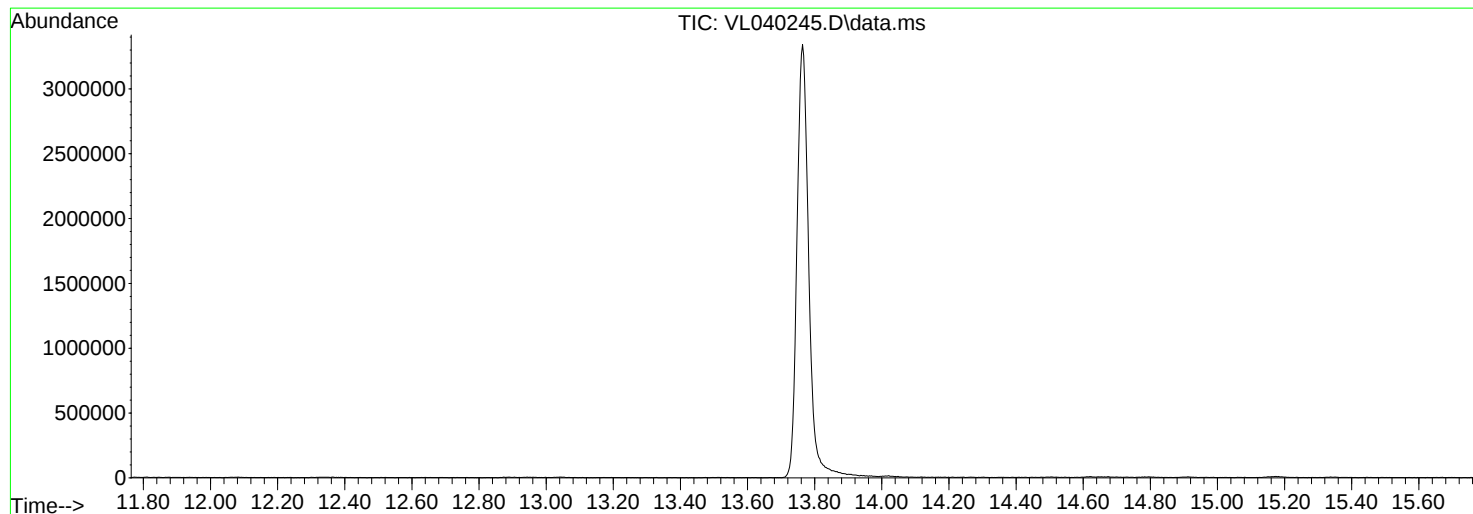

AutoFind: Scans 3470, 3471, 3472; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	168960	PASS
75	95	30	66	57.7	408576	PASS
95	95	100	100	100.0	708309	PASS
96	95	5	9	6.5	45832	PASS
173	174	0.00	2	0.9	3503	PASS
174	95	50	120	57.6	407936	PASS
175	174	4	9	7.0	28643	PASS
176	174	93	101	97.0	395691	PASS
177	176	5	9	6.1	24299	PASS

Average of 13.760 to 13.767 min.: VL040245.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7244	45.05	7857	54.05	115	64.95	1361
37.05	38824	45.90	623	55.05	1927	65.90	91
38.05	36752	46.10	207	56.05	13484	66.90	132
39.10	16487	47.05	6810	57.05	23803	67.10	65
39.90	394	48.00	4602	57.90	540	68.00	88557
40.20	315	49.05	33181	58.15	705	69.05	90109
40.90	210	50.10	168960	60.05	7182	70.05	6491
41.20	66	51.05	51587	61.05	37525	70.90	179
41.95	205	52.05	2330	62.05	37467	71.10	134
43.10	352	52.95	227	63.05	30368	72.05	3757
44.00	5630	53.90	117	64.00	2801	73.05	33824

Average of 13.760 to 13.767 min.: VL040245.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.10	140352	84.00	125	96.10	45832	110.80	152
75.10	408576	84.60	63	97.10	1287	111.05	523
76.10	36187	85.85	639	102.50	55	111.85	297
76.90	2028	86.10	287	102.70	132	112.10	214
77.10	2314	87.00	21427	103.00	223	112.95	566
78.00	1590	88.00	23040	103.85	3157	114.85	595
79.00	22464	90.95	2761	104.80	712	115.20	117
80.05	6168	92.05	22149	105.05	919	115.95	2934
81.00	22160	93.05	32963	106.05	2737	117.00	4266
81.95	4790	94.10	88733	107.00	711	117.80	853
82.95	419	95.10	708309	110.00	406	118.00	1927

Average of 13.760 to 13.767 min.: VL040245.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.90	1243	126.85	321	137.05	777	146.90	226
119.05	2237	128.00	2826	138.75	218	147.10	150
119.80	89	129.05	1020	139.00	203	147.95	1654
120.10	94	130.00	2336	139.80	201	149.05	392
121.70	64	130.85	710	141.00	6324	149.60	172
121.85	126	131.10	470	142.00	757	149.95	592
122.60	80	133.80	54	143.05	7199	151.10	68
123.00	257	134.00	112	143.80	76	152.05	388
123.80	392	135.05	1005	144.10	471	152.70	97
125.15	212	135.60	55	145.00	878	153.15	162
125.90	323	136.90	329	145.90	1105	154.00	667

Average of 13.760 to 13.767 min.: VL040245.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.05	1403	172.15	1830				
156.10	57	173.00	3503				
156.90	174	174.10	407936				
157.10	940	175.00	28643				
157.80	58	176.10	395691				
158.20	67	177.00	24299				
158.95	775	178.05	369				
160.95	1095	207.20	140				
169.70	345						
170.30	107						
170.85	267						