


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL030922\
 Data File : VL038570.D
 Acq On : 9 Mar 2022 9:44
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030822AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Mar 08 21:18:44 2022
 Last Update : Tue Mar 08 21:18:44 2022

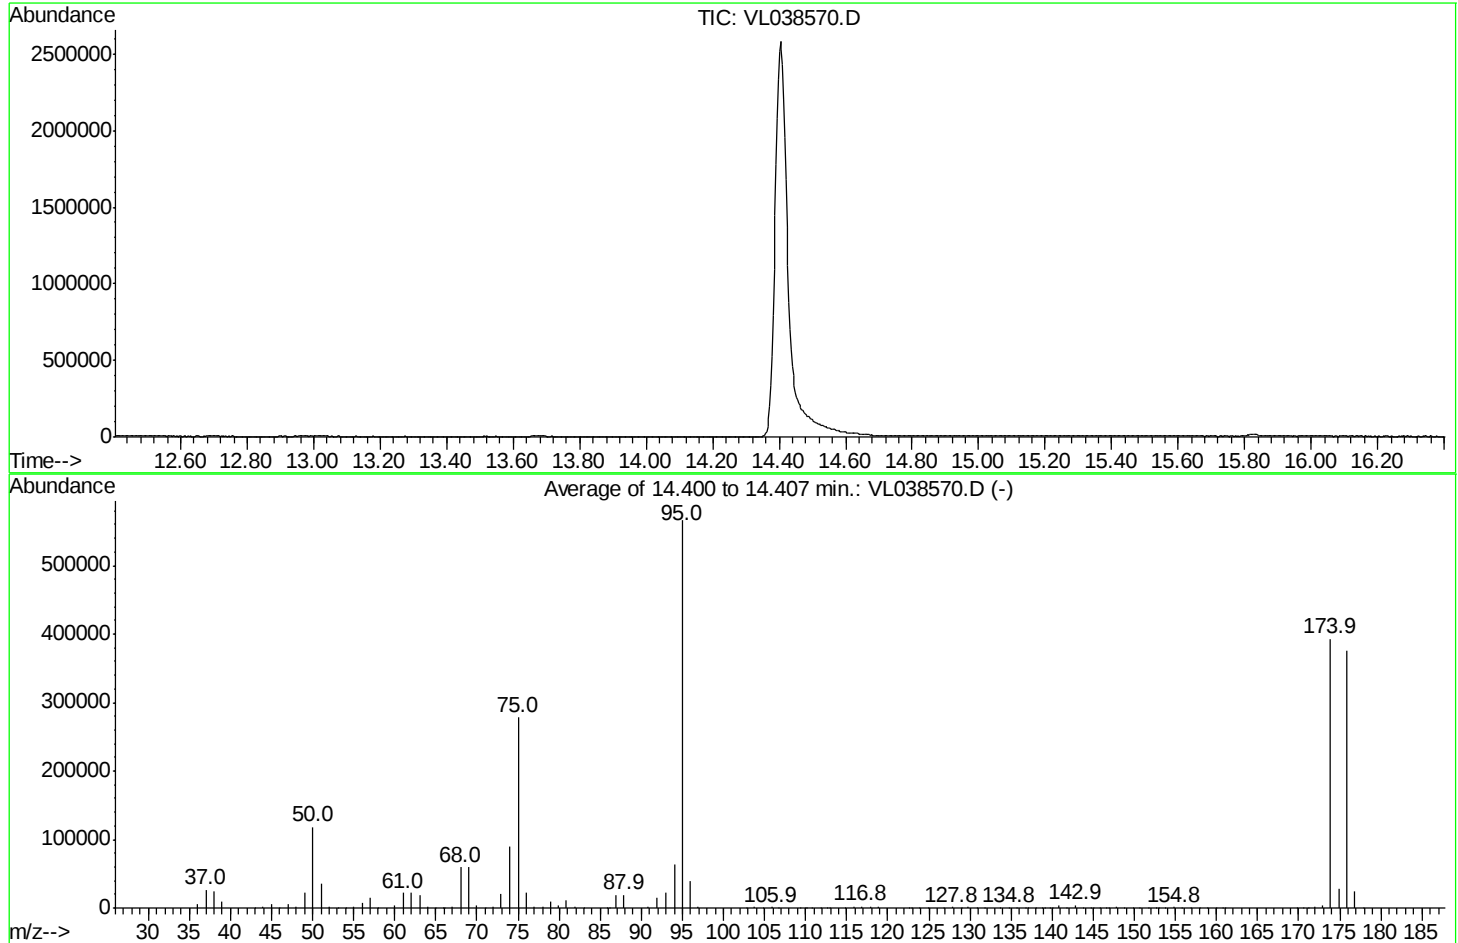

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.9	118354	PASS
75	95	30	66	49.2	278293	PASS
95	95	100	100	100.0	566058	PASS
96	95	5	9	7.0	39848	PASS
173	174	0.00	2	0.9	3460	PASS
174	95	50	120	69.5	393429	PASS
175	174	4	9	7.4	29045	PASS
176	174	93	101	95.6	375957	PASS
177	176	5	9	6.7	25146	PASS