
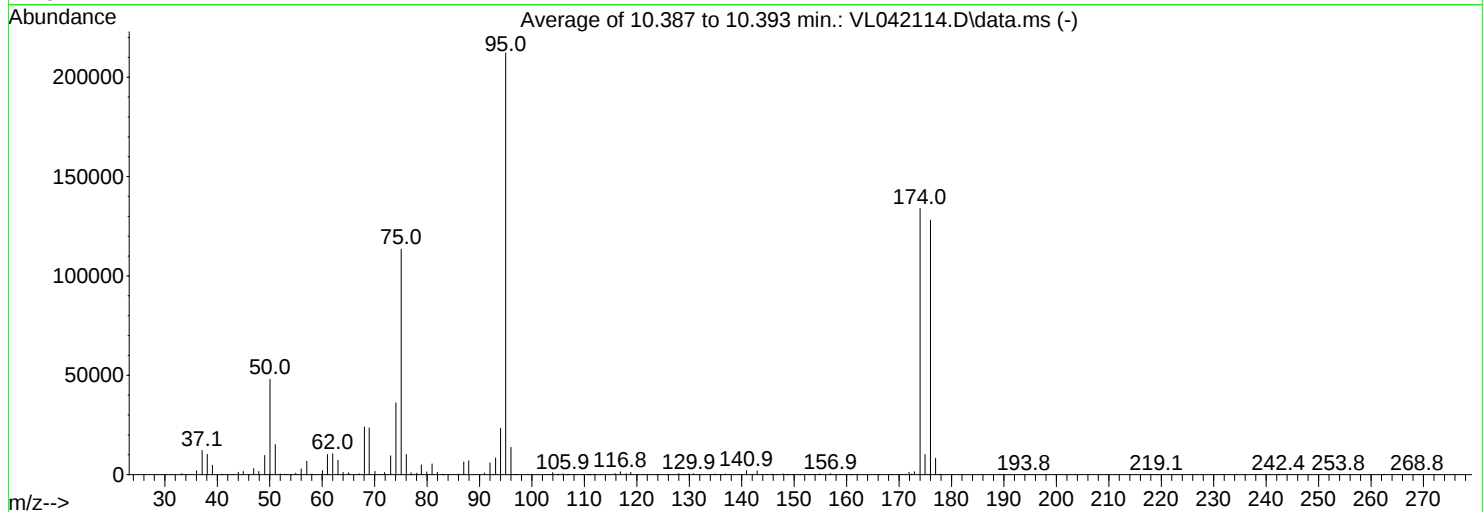


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031025\
Data File : VL042114.D
Acq On : 10 Mar 2025 08:22
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 26 01:08:36 2025

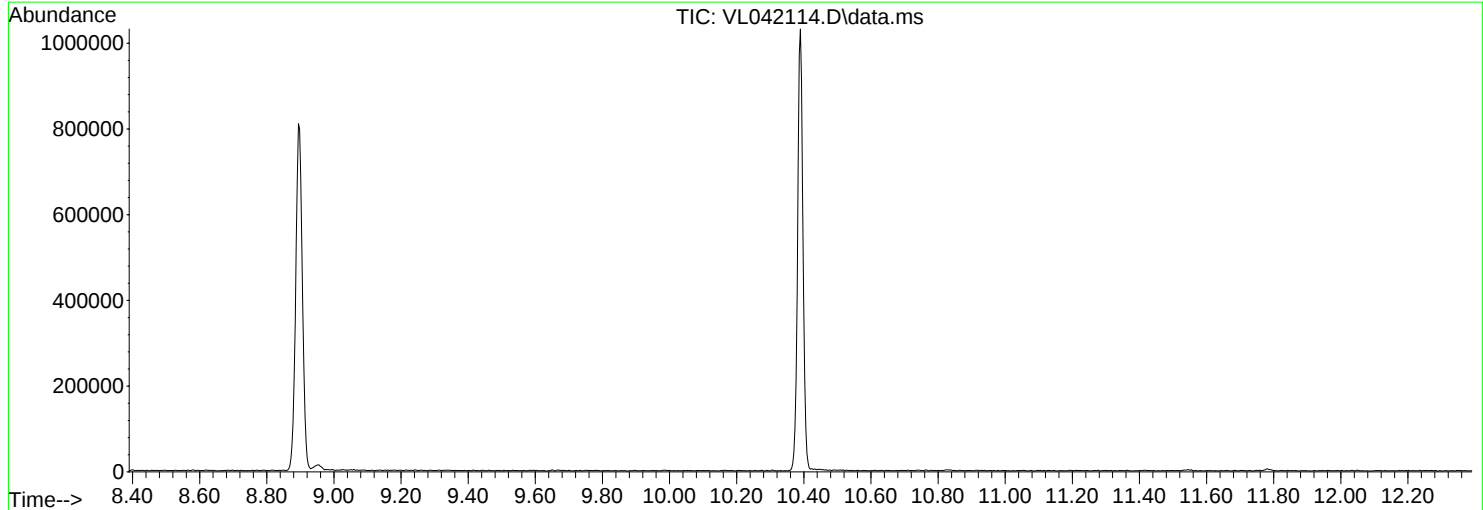

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.6	47960	PASS
75	95	30	66	53.4	113432	PASS
95	95	100	100	100.0	212267	PASS
96	95	5	9	6.5	13780	PASS
173	174	0.00	2	1.1	1482	PASS
174	95	50	120	63.1	133968	PASS
175	174	4	9	7.6	10185	PASS
176	174	93	101	95.6	128123	PASS
177	176	5	9	6.5	8273	PASS

Average of 10.387 to 10.393 min.: VL042114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.20	465	44.95	1598	54.00	39	64.00	116
34.05	168	46.15	119	54.95	693	65.00	88
36.05	1968	46.95	3029	56.00	2870	65.20	34
37.10	12192	47.90	1628	57.05	6764	65.95	10
38.10	10213	49.05	9673	57.80	118	66.80	118
39.05	4743	50.05	47960	58.05	226	67.10	378
40.80	18	51.05	15126	58.85	49	68.05	24019
41.10	66	52.00	396	60.05	2001	68.95	23553
41.95	154	52.20	112	61.00	10067	70.05	1668
43.10	145	52.85	191	62.00	10530	70.90	109
44.00	1208	53.10	145	63.00	7241	71.90	1051

Average of 10.387 to 10.393 min.: VL042114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	9509	82.90	135	95.00	212267	106.70	37
74.05	36173	83.10	42	96.00	13780	107.00	181
75.05	113432	84.05	65	96.90	114	108.00	24
76.05	10118	85.85	220	97.05	154	108.20	48
76.95	1002	86.10	67	98.00	63	109.85	130
77.50	106	87.00	6347	102.65	71	110.60	31
78.05	842	87.95	6894	103.00	48	111.00	42
78.90	4958	90.95	841	103.95	1039	111.90	210
79.95	1412	92.00	5925	104.80	28	113.05	100
80.95	5386	93.05	8354	105.05	277	114.60	109
81.95	1178	94.00	23376	105.90	499	115.85	554

Average of 10.387 to 10.393 min.: VL042114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.85	1451	129.05	243	142.10	123	149.90	100
117.95	597	129.80	213	142.95	1873	151.10	29
118.85	1147	129.95	425	143.80	165	151.75	56
120.00	23	130.85	484	144.70	83	152.85	117
123.60	47	134.00	39	144.95	114	153.60	57
124.05	51	134.95	380	145.85	313	154.00	140
125.80	27	135.90	17	146.70	63	154.85	437
127.90	416	136.90	317	147.90	409	155.90	113
128.10	302	138.00	62	148.70	32	156.70	127
128.60	62	139.95	106	148.85	114	156.95	508
128.80	108	140.90	2004	149.70	103	158.85	115

Average of 10.387 to 10.393 min.: VL042114.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.80	24	172.40	289	242.40	30		
160.70	32	172.95	1482	253.80	72		
160.95	114	174.00	133968	262.30	18		
166.10	44	174.95	10185	268.80	68		
168.50	164	176.00	128123	269.20	26		
169.00	60	176.95	8273				
169.65	52	177.80	239				
170.10	55	178.00	55				
170.55	133	193.80	42				
171.20	216	209.40	18				
171.90	1192	219.10	27				