
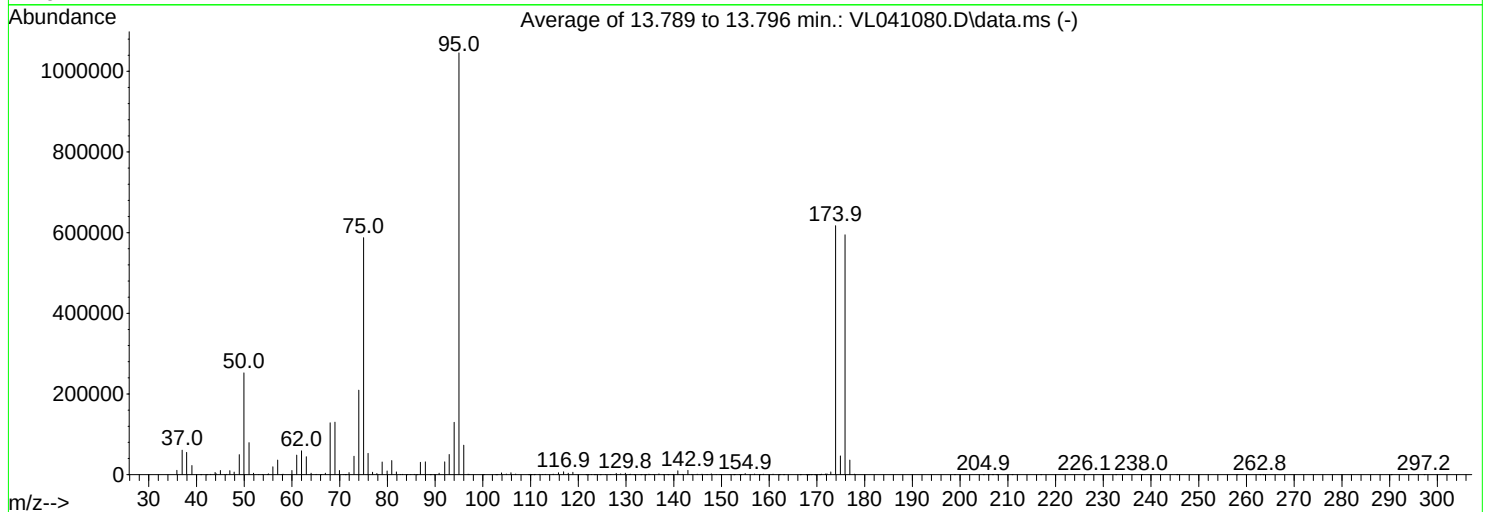


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031124\
Data File : VL041080.D
Acq On : 11 Mar 2024 9:49
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031124AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Mar 12 06:25:15 2024

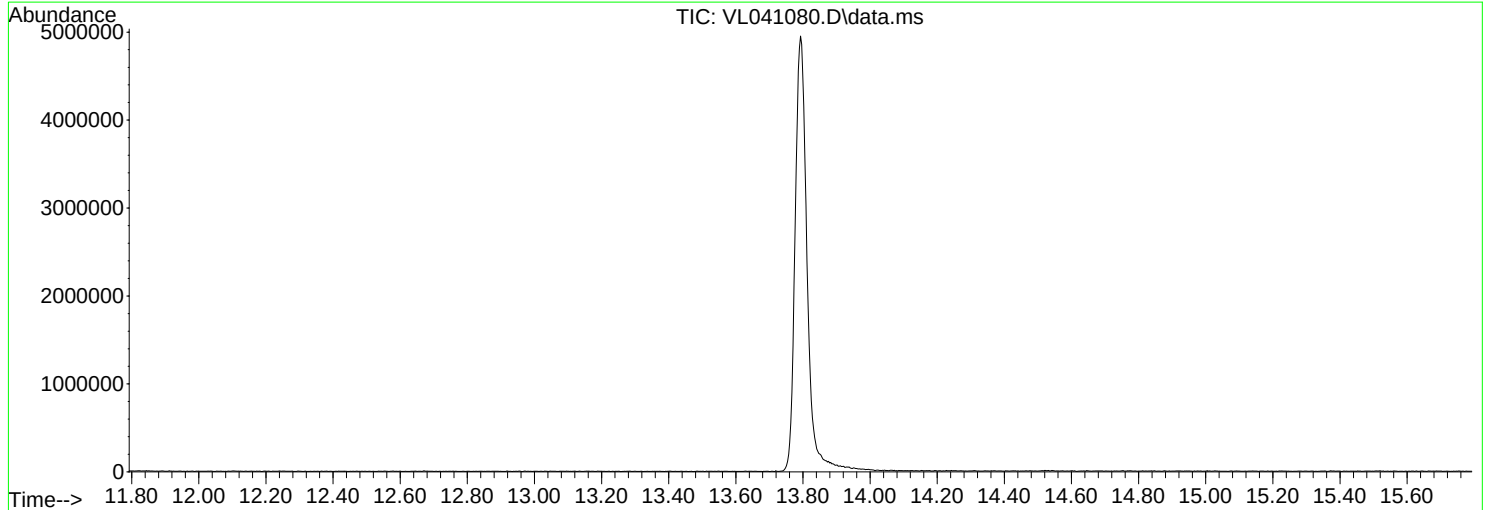

AutoFind: Scans 3479, 3480, 3481; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	252160	PASS
75	95	30	66	56.2	587477	PASS
95	95	100	100	100.0	1045845	PASS
96	95	5	9	7.0	72939	PASS
173	174	0.00	2	1.1	6910	PASS
174	95	50	120	59.0	617408	PASS
175	174	4	9	7.6	46651	PASS
176	174	93	101	96.4	594880	PASS
177	176	5	9	6.1	36165	PASS

Average of 13.789 to 13.796 min.: VL041080.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	10616	45.90	267	55.10	1974	65.95	170
37.00	60677	46.25	701	56.00	19315	67.00	379
37.95	55340	47.00	9880	57.00	35999	68.00	12864
39.05	22541	47.90	6374	57.90	543	69.00	13006
40.00	439	48.95	49409	58.10	1314	69.95	10482
40.90	127	49.95	252160	60.00	10360	70.90	573
42.10	223	51.00	79235	61.00	48579	71.20	116
42.95	795	51.95	3778	62.00	59043	71.95	5258
43.90	5415	53.05	337	63.00	44467	73.00	45840
44.10	2569	53.80	306	64.00	3753	74.00	209536
45.00	10353	54.90	871	65.05	861	75.00	587477

Average of 13.789 to 13.796 min.: VL041080.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.95	52960	85.65	698	96.00	72939	109.90	703
76.90	5903	86.10	231	96.90	1367	110.10	139
77.80	2799	86.90	30523	97.10	830	110.70	208
78.90	31523	87.95	31824	100.10	60	110.90	698
79.95	9209	89.00	101	102.70	154	111.80	938
80.90	34784	89.80	161	102.95	214	112.55	400
81.90	6739	90.85	3595	103.90	4374	113.05	847
82.75	454	92.00	31597	104.90	1792	114.75	1098
83.15	755	92.95	49955	105.90	4791	115.85	4675
84.00	51	94.00	129877	106.90	1589	116.90	7158
84.90	325	95.00	1.04585e+006	109.60	120	117.90	3642

Average of 13.789 to 13.796 min.: VL041080.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.85	5874	129.85	3633	137.80	121	145.90	1285
121.65	221	130.70	302	138.10	286	146.80	362
122.00	51	130.90	1159	138.60	313	147.05	405
122.75	449	131.70	93	138.80	199	147.85	1923
123.40	159	133.10	58	139.80	353	148.90	566
123.90	539	133.90	248	139.95	819	149.70	406
124.60	151	134.10	229	140.85	9353	149.95	634
125.75	277	134.80	1258	141.85	914	151.80	635
126.80	603	135.00	736	142.95	10725	152.60	134
127.95	3378	135.70	261	143.80	1004	152.85	531
128.90	2134	136.90	1884	144.90	1096	153.80	544

Average of 13.789 to 13.796 min.: VL041080.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.00	119	168.10	97	172.90	6910	210.90	98
154.95	2677	168.30	182	173.90	617408	216.90	53
156.00	497	168.70	201	174.90	46651	226.10	145
156.95	1755	169.10	434	175.90	594880	232.60	76
158.00	109	169.50	161	176.90	36165	238.00	176
158.75	1143	169.70	153	177.90	1368	245.40	53
160.80	1039	170.15	397	198.80	62	258.00	62
162.10	65	170.60	238	204.90	140	262.80	212
163.00	58	170.95	1067	205.90	52	263.50	54
166.50	59	171.80	1613	206.80	50	290.30	62
167.80	149	172.10	2219	207.70	119	297.20	87