


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL031219\
Data File : VL033271.D
Acq On : 12 Mar 2019 1:40
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031219AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Mar 13 07:17:55 2019
Last Update : Wed Mar 13 07:17:55 2019

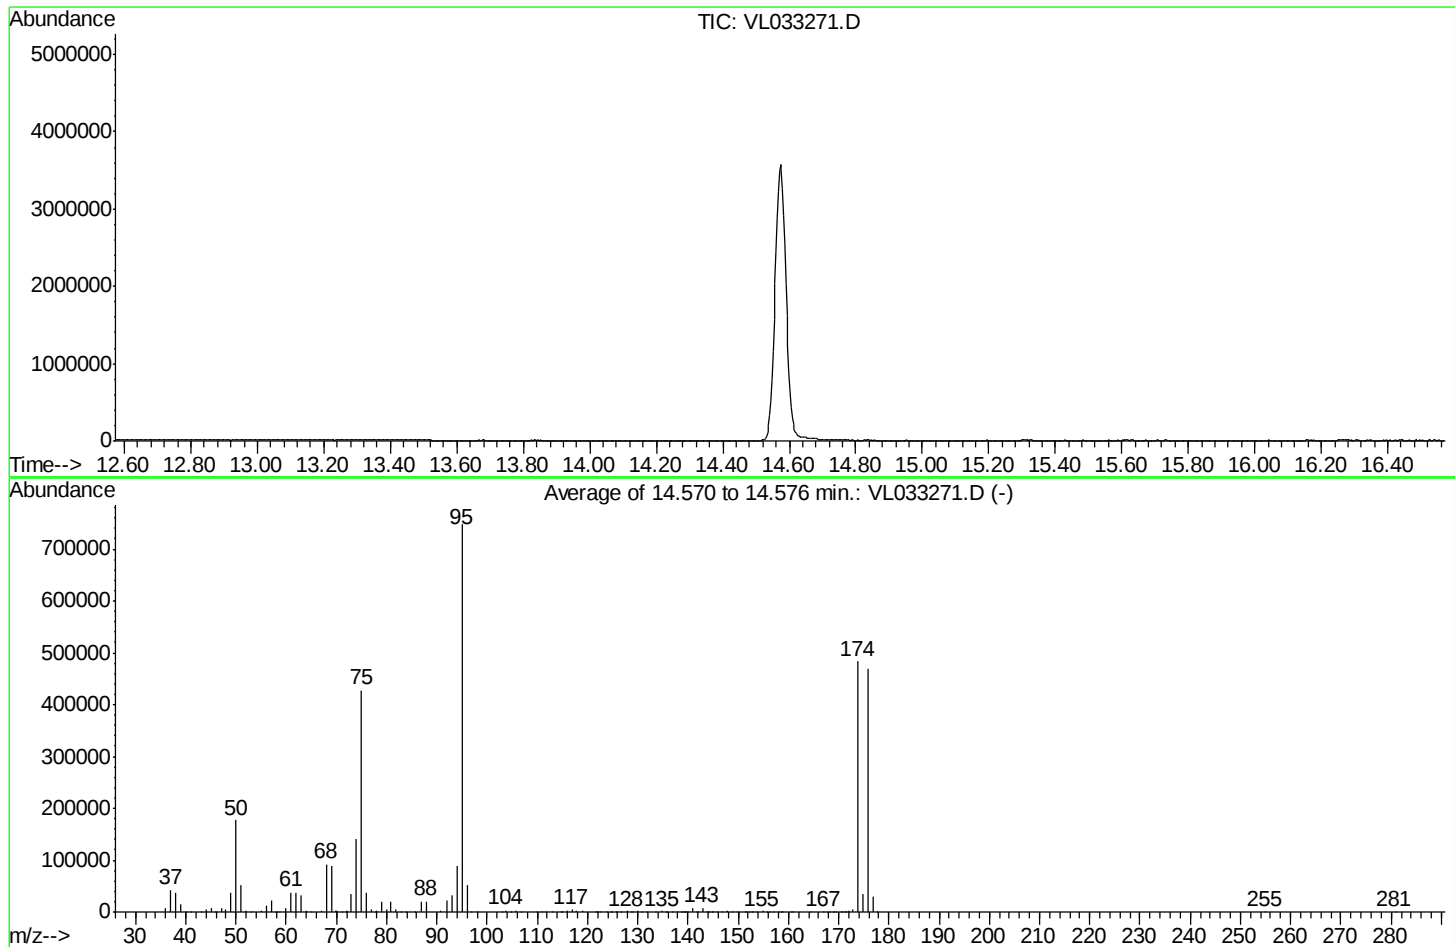

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	176938	PASS
75	95	30	66	57.1	427221	PASS
95	95	100	100	100.0	747797	PASS
96	95	5	9	6.8	50930	PASS
173	174	0.00	2	1.0	4870	PASS
174	95	50	120	64.6	483072	PASS
175	174	4	9	7.2	35008	PASS
176	174	93	101	97.0	468586	PASS
177	176	5	9	6.4	29890	PASS