
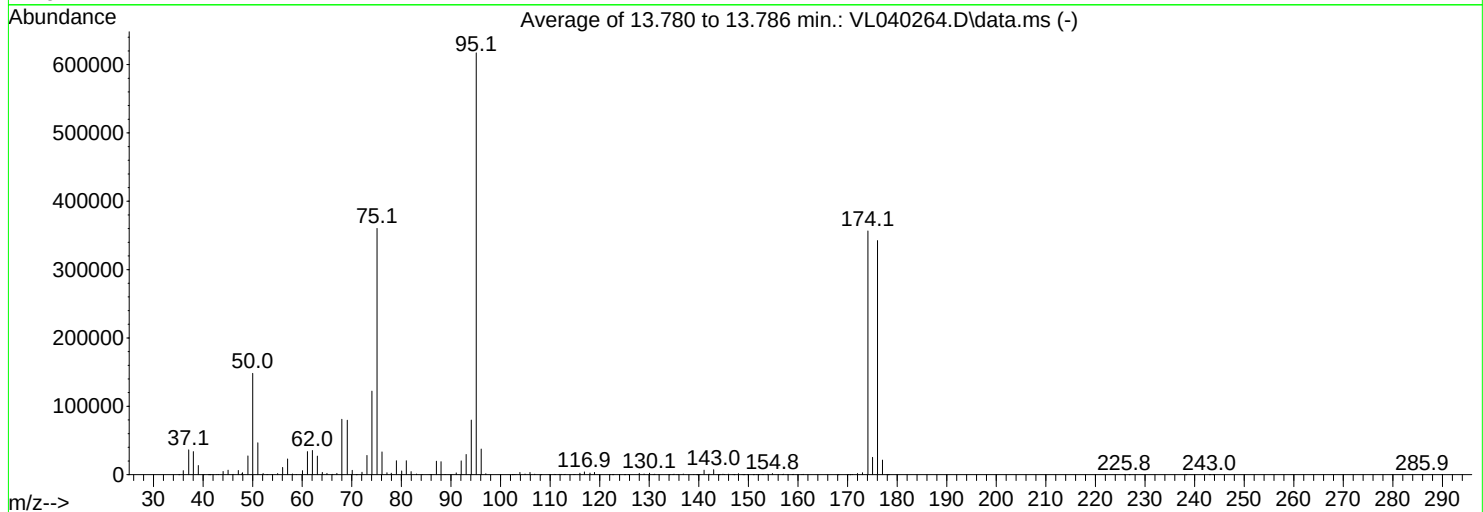


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031323\
 Data File : VL040264.D
 Acq On : 13 Mar 2023 11:49
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Mar 14 04:52:39 2023

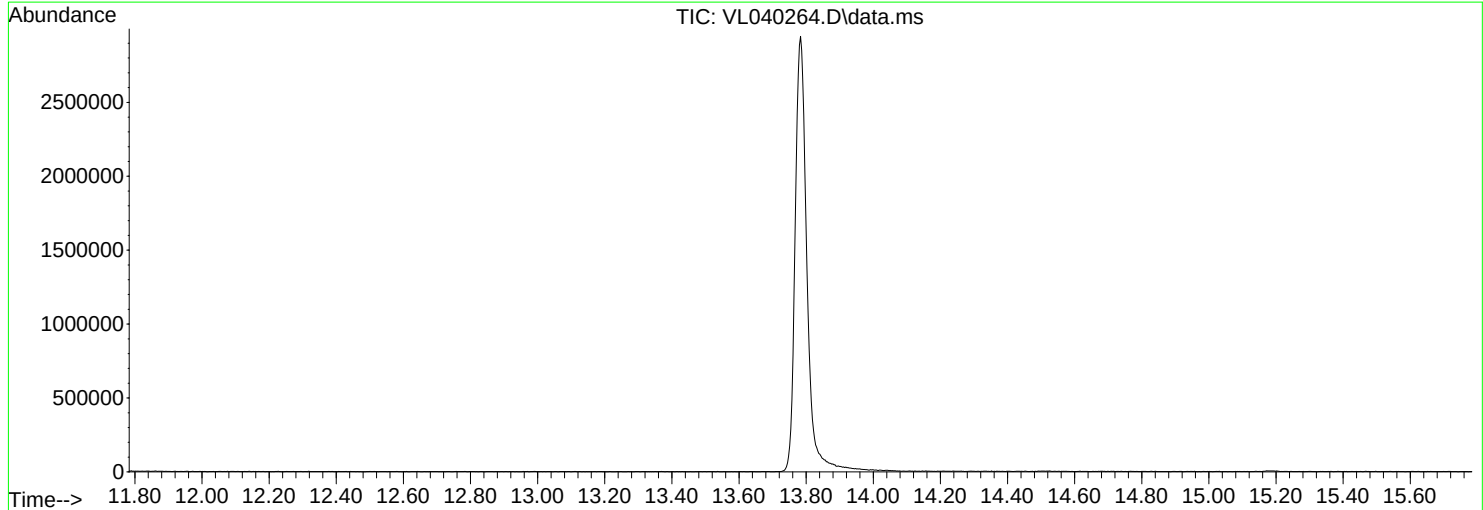

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	148288	PASS
75	95	30	66	58.4	360341	PASS
95	95	100	100	100.0	617195	PASS
96	95	5	9	6.1	37395	PASS
173	174	0.00	2	0.8	2796	PASS
174	95	50	120	57.8	356565	PASS
175	174	4	9	7.1	25368	PASS
176	174	93	101	96.1	342571	PASS
177	176	5	9	6.3	21429	PASS

Average of 13.780 to 13.786 min.: VL040264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	56	44.05	4758	53.05	182	64.05	332
36.00	5909	45.05	6556	53.95	218	65.00	195
37.10	36243	46.05	601	55.05	1603	66.15	57
38.05	33685	47.10	6098	56.05	10666	67.00	195
39.05	13389	47.80	909	57.05	22867	68.00	81067
40.00	113	47.95	2770	58.05	917	69.10	79709
41.10	117	49.05	27435	58.80	131	70.10	6395
41.40	59	50.00	148288	60.05	5861	70.90	59
42.00	144	51.05	46635	61.05	33795	72.05	3637
42.80	329	52.10	1700	62.05	35344	73.05	28133
43.10	235	52.90	192	63.05	27216	74.05	122157

Average of 13.780 to 13.786 min.: VL040264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	360341	86.05	219	102.40	66	111.10	195
76.10	33163	87.05	19675	102.80	319	111.80	528
77.10	2943	88.00	19045	103.10	158	112.20	428
77.95	2198	88.80	200	103.90	3292	112.80	203
79.00	20403	91.05	2615	104.95	1009	113.00	444
80.05	5377	92.05	20221	105.95	3230	114.80	367
81.00	20365	93.05	29435	106.90	707	115.00	304
81.95	4481	94.10	79747	108.10	60	116.00	2192
83.05	1003	95.10	617195	109.80	131	116.90	4125
84.20	172	96.10	37395	110.05	241	118.05	2296
85.80	192	97.05	1501	110.80	498	118.95	3205

Average of 13.780 to 13.786 min.: VL040264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
120.00	138	131.10	740	140.20	145	148.00	1498
122.10	162	131.95	134	141.05	6684	148.75	244
122.60	59	134.00	62	142.05	795	149.00	123
122.85	151	134.80	322	143.00	7208	149.30	137
124.00	275	135.00	815	143.90	275	149.80	358
125.00	104	135.60	147	144.10	54	150.00	306
125.85	232	135.90	248	144.85	731	151.00	68
128.00	2005	136.85	945	145.20	250	151.70	131
128.95	1047	139.00	346	146.00	789	152.00	92
130.05	2144	139.60	54	146.90	382	152.80	154
130.80	269	140.00	176	147.10	68	153.10	347

Average of 13.780 to 13.786 min.: VL040264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.90	409	170.15	259	225.80	73		
154.85	1618	170.50	94	226.80	53		
156.10	140	171.00	228	238.20	57		
156.90	310	172.00	1747	243.00	71		
157.05	678	173.00	2796	243.80	60		
157.95	139	174.10	356565	285.90	88		
158.90	158	175.05	25368				
159.05	577	176.05	342571				
160.80	174	177.05	21429				
161.05	549	178.00	206				
168.10	97	178.20	105				

Instrument :

MSVOA_L

ClientSampleId :

BFB