
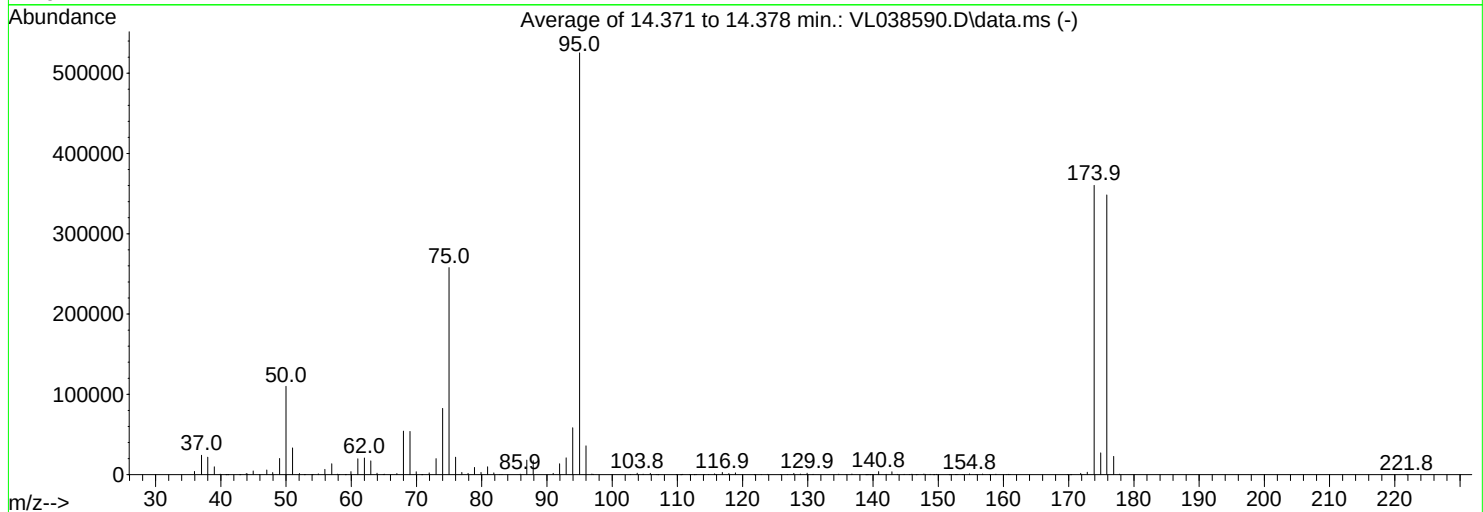


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031422\
 Data File : VL038590.D
 Acq On : 14 Mar 2022 8:57
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030822AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 08 21:18:44 2022
 Last Update : Tue Mar 08 21:18:44 2022

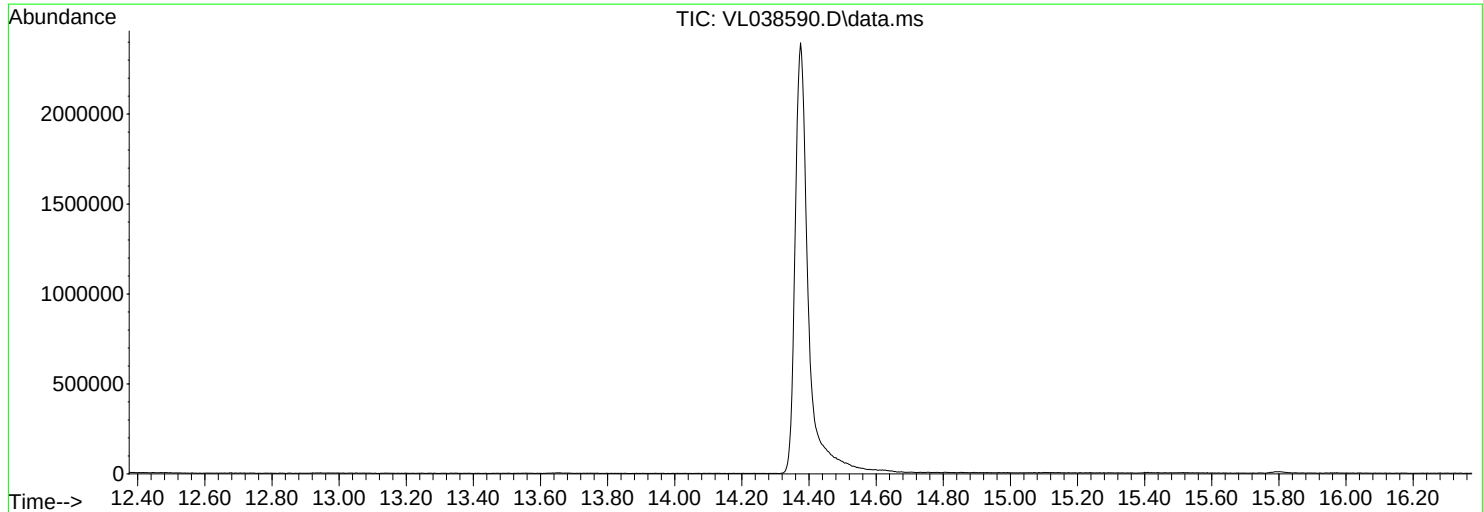

AutoFind: Scans 3603, 3604, 3605; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.9	110005	PASS
75	95	30	66	49.1	257835	PASS
95	95	100	100	100.0	525333	PASS
96	95	5	9	6.8	35941	PASS
173	174	0.00	2	0.8	2924	PASS
174	95	50	120	68.6	360384	PASS
175	174	4	9	7.5	27195	PASS
176	174	93	101	96.7	348331	PASS
177	176	5	9	6.6	22829	PASS

Average of 14.371 to 14.378 min.: VL038590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	3995	45.95	280	57.00	13564	67.00	140
37.05	24221	47.05	5830	57.90	600	68.00	5421
38.00	21683	47.95	2647	58.20	219	69.00	5377
39.00	9818	49.00	20139	59.10	65	69.95	370
39.90	587	50.00	110005	59.95	3892	70.80	107
40.80	57	51.00	33288	61.00	19693	70.95	283
41.05	120	52.05	1389	62.00	20829	71.95	2271
42.90	58	52.80	69	63.00	17083	73.00	19904
43.90	1421	54.00	62	63.95	1756	74.00	82461
44.10	920	54.95	985	64.90	295	75.00	257835
44.95	4587	55.95	6579	65.05	570	76.00	21725

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 14.371 to 14.378 min.: VL038590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	2874	90.95	1577	105.85	1636	115.70	1091
77.90	1597	91.95	13626	106.75	305	115.90	447
78.90	8961	92.95	20931	107.00	100	116.90	2798
79.90	2883	93.95	58355	109.85	141	117.90	1373
80.90	9870	95.00	525333	110.50	86	118.90	2232
81.85	2133	96.00	35941	110.80	345	121.80	58
82.80	205	96.90	799	111.90	222	122.85	224
83.10	204	97.10	337	112.60	79	123.85	359
85.90	519	102.80	143	112.95	168	125.80	130
86.90	18096	103.85	1746	114.00	53	126.85	157
87.90	17276	104.75	616	114.80	284	127.85	1509

Average of 14.371 to 14.378 min.: VL038590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.85	741	142.00	466	149.30	58	155.80	142
129.90	1757	142.90	3549	149.75	378	156.80	829
130.80	496	143.75	351	150.00	161	157.85	196
134.75	522	144.75	471	151.70	75	158.85	546
135.90	184	145.60	222	152.00	186	160.50	128
136.75	816	145.95	634	152.65	172	160.75	480
138.90	96	146.60	94	152.80	141	161.00	130
139.15	118	146.90	315	153.00	151	169.80	130
139.50	84	147.80	755	153.70	212	170.30	54
139.90	154	148.00	367	153.90	191	171.85	1537
140.85	3723	148.75	344	154.80	1017	172.85	2924

Average of 14.371 to 14.378 min.: VL038590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.90	360384						
174.90	27195						
175.85	348331						
176.90	22829						
177.80	676						
221.80	52						