


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031425\
 Data File : VL042140.D
 Acq On : 14 Mar 2025 07:56
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Feb 26 01:08:36 2025

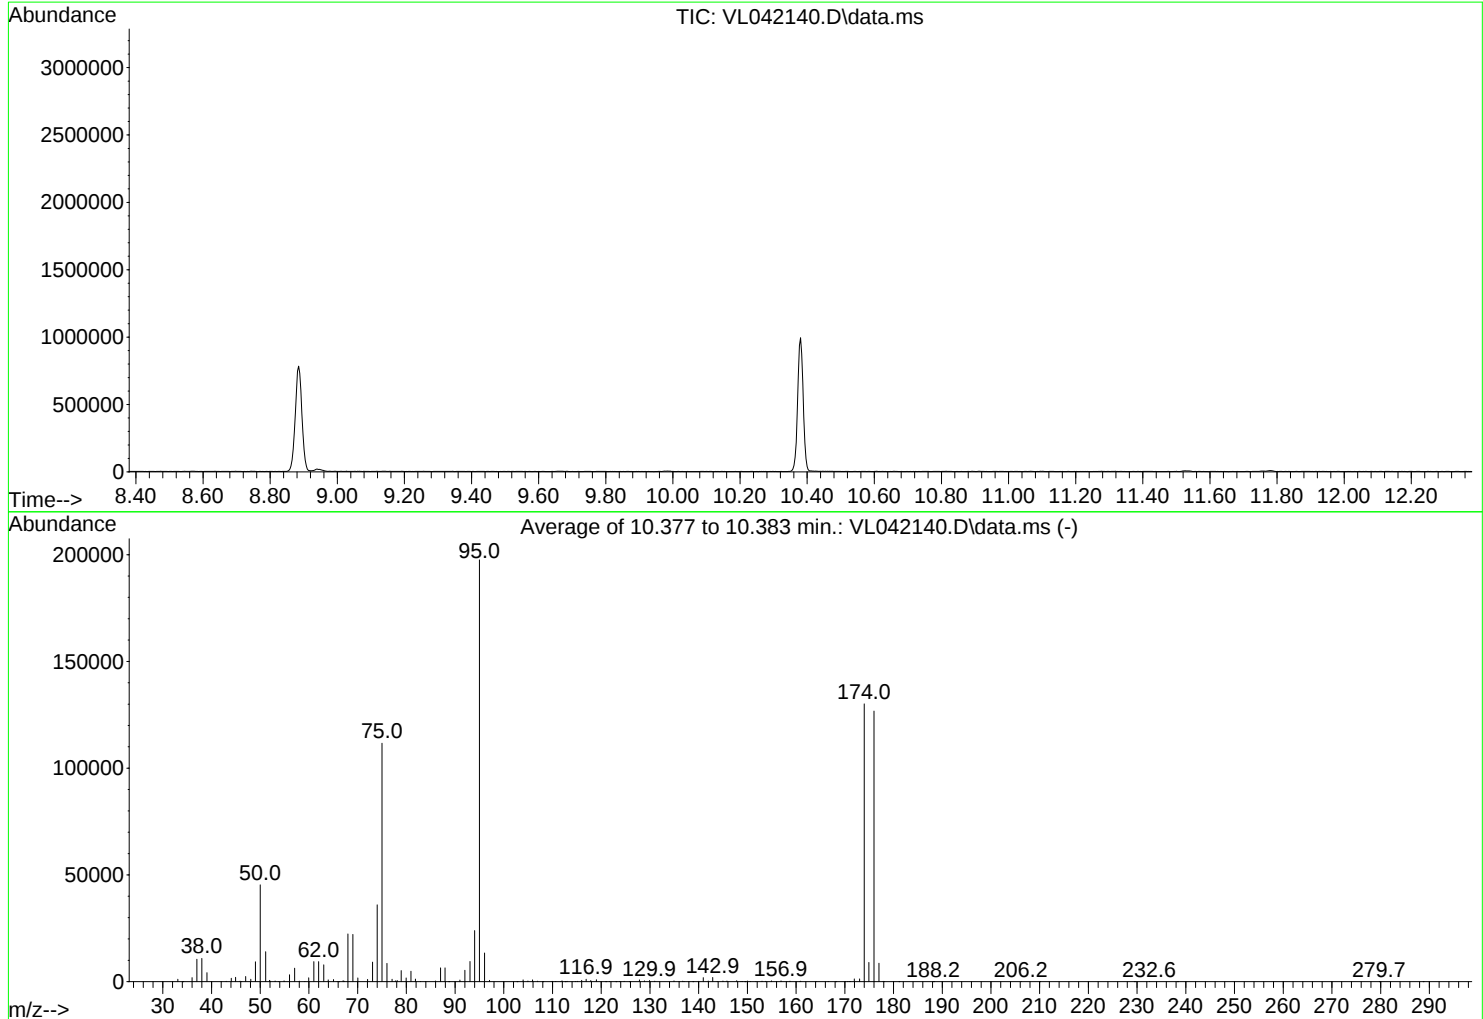

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	45333	PASS
75	95	30	66	56.5	111685	PASS
95	95	100	100	100.0	197589	PASS
96	95	5	9	6.8	13388	PASS
173	174	0.00	2	1.0	1315	PASS
174	95	50	120	65.9	130120	PASS
175	174	4	9	6.9	8967	PASS
176	174	93	101	97.4	126715	PASS
177	176	5	9	6.8	8618	PASS

Average of 10.377 to 10.383 min.: VL042140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1104	46.20	67	56.00	3248	66.10	11
34.10	19	47.00	2436	57.05	6313	67.00	45
36.00	1874	48.05	1145	58.00	206	67.20	20
37.00	10525	49.00	9275	59.15	62	68.00	2232
38.00	10902	50.00	45333	59.95	1827	69.00	22126
39.05	4186	51.10	14027	61.00	9356	70.05	1756
42.00	67	51.90	609	62.00	9338	72.05	1083
43.00	170	52.10	192	63.05	7890	73.05	9177
44.05	1570	53.05	284	63.95	795	74.00	35971
44.95	2053	53.80	82	65.05	952	75.00	111685
45.85	207	54.90	379	65.80	57	76.00	8550

Average of 10.377 to 10.383 min.: VL042140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	1129	87.95	6443	104.95	312	115.10	171
77.75	360	88.70	39	105.90	868	116.00	613
78.10	565	91.00	766	106.95	224	116.90	1125
78.95	5166	92.00	5349	108.00	38	117.85	560
79.95	1751	93.05	9434	109.90	123	119.00	943
80.95	4903	94.00	23939	110.65	57	120.90	27
81.85	1216	95.00	197589	111.70	55	121.70	84
82.90	108	96.05	13388	111.95	366	123.00	25
83.95	56	97.05	573	112.60	19	123.75	84
85.95	342	102.70	35	113.00	187	124.00	117
87.00	6416	103.95	854	114.70	116	124.70	152

Average of 10.377 to 10.383 min.: VL042140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.80	29	138.80	27	149.50	27	160.80	58
126.05	65	140.00	148	150.00	295	160.95	204
127.85	793	140.95	1898	150.60	50	164.10	40
128.85	349	141.95	289	151.75	60	166.60	41
129.90	556	142.90	1947	153.00	218	168.10	25
131.00	250	143.80	104	153.75	139	170.10	95
134.95	382	145.00	280	154.95	362	170.60	70
136.00	56	145.80	284	155.95	98	170.90	112
136.75	213	147.80	429	156.90	381	171.10	52
137.00	41	148.70	95	158.10	69	171.95	1308
138.00	50	148.95	114	158.75	257	173.05	1315

Average of 10.377 to 10.383 min.: VL042140.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	130120	232.55	44				
174.95	8967	238.30	25				
176.00	126715	279.70	32				
177.00	8618	288.70	30				
177.85	180						
178.10	67						
181.10	38						
188.20	28						
206.20	40						
210.00	23						
229.45	35						