

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL031519\
 Data File : VL033347.D
 Acq On : 16 Mar 2019 1:44
 Operator : SY/AP
 Sample : K1827-02
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Mar 16 04:01:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL031519AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
 QLast Update : Fri Mar 15 14:52:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	794975	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.29	114	1794141	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.25	117	1738192	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.58	95	1302146	10.11	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.10%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.08	85	32931	0.236	ppbv	99
3) Chlorodifluoromethane	2.99	51	258822	2.837	ppbv #	74
4) Chloromethane	3.17	50	24988	0.506	ppbv	95
9) Propene	3.24	41	431345	10.590	ppbv	93
10) Heptane	8.25	43	174216	1.724	ppbv	100
11) Trichlorofluoromethane	4.01	101	32390	0.233	ppbv	95
12) 1,1,2-Trichlorotrifluoroet	4.55	101	3012	0.033	ppbv #	14
13) Ethanol	3.66	45	1986274	102.291	ppbv	98
15) Acetone	3.90	43	977261	7.908	ppbv	94
16) 1,3-Butadiene	3.34	39	4602	0.115	ppbv #	2
17) tert-Butyl alcohol	4.37	59	8913	0.513	ppbv #	74
19) Isopropyl Alcohol	4.04	45	619416	10.537	ppbv #	99
20) Methylene Chloride	4.41	84	89587	2.223	ppbv	98
21) Allyl Chloride	4.42	41	1374	0.023	ppbv #	46
23) Vinyl Acetate	5.15	43	36465	0.255	ppbv #	45
25) Ethyl Acetate	5.77	43	266661	1.484	ppbv #	96
26) Hexane	5.78	57	163426	2.035	ppbv #	75
27) Carbon Disulfide	4.63	76	4682	0.051	ppbv #	32
29) Chloroform	5.84	83	2760	0.021	ppbv	90
30) Cyclohexane	7.25	84	7022	0.109	ppbv #	32
31) cis-1,2-Dichloroethene	5.76	61	6703	0.083	ppbv #	28
34) 2-Butanone	5.34	43	88970	0.755	ppbv	99
36) Benzene	7.00	78	27875	0.174	ppbv	94
37) 1,2-Dichloroethane	6.41	62	4399	0.043	ppbv	99
39) 1,2-Dichloropropane	7.29	63	487910	8.114	ppbv #	24
41) Tetrahydrofuran	6.16	42	1479	0.024	ppbv #	1
43) Methyl Methacrylate	8.13	69	2861	0.046	ppbv #	1
44) 2,2,4-Trimethylpentane	7.99	57	38284	0.144	ppbv #	48
52) Tetrachloroethene	11.37	164	1951	0.029	ppbv #	70
53) Toluene	9.95	91	3369824	18.470	ppbv	100
58) Ethyl Benzene	12.87	91	98298	0.400	ppbv	96
59) m/p-Xylene	13.12	91	111854	0.529	ppbv #	100
60) o-Xylene	13.86	91	17931	0.087	ppbv #	31
61) Styrene	13.70	104	5794	0.040	ppbv #	27

(#) = qualifier out of range (m) = manual integration (+) = signals summed

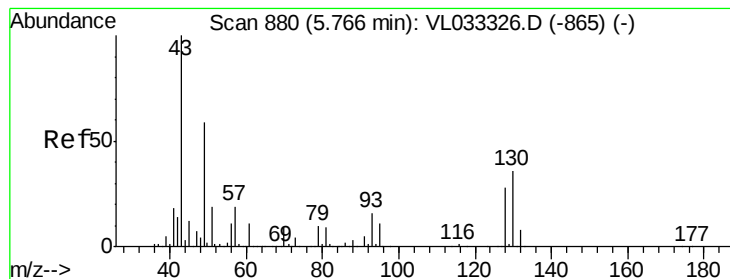

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 879

Delta R.T. -0.00 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L

ClientSampled :


Tot Ion: 49 Resp: 794975

Ion Ratio Lower Upper

49 100

128 46.4 23.5 70.6




130 58.6 30.1 90.3



Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

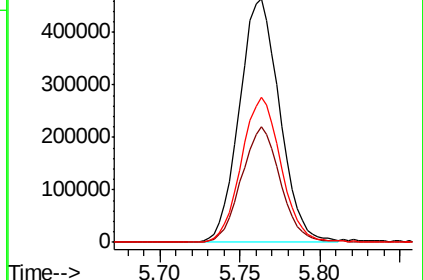

#2

Dichlorodifluoromethane

Concen: 0.236 ppbv

RT: 3.08 min Scan# 44

Delta R.T. -0.00 min

Lab File: VL033347.D


Acq: 16 Mar 2019 1:44

Tgt Ion: 85 Resp: 32931

Ion Ratio Lower Upper



85 100


87 34.1 26.9 40.3



Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

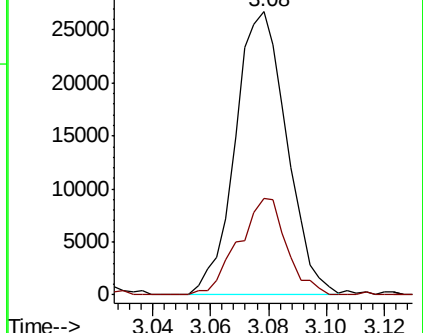



#3

Chlorodifluoromethane

Concen: 2.837 ppbv

RT: 2.99 min Scan# 16

Delta R.T. -0.03 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 51 Resp: 258822

Ion Ratio Lower Upper

51 100

67 7.2 14.9 22.3#

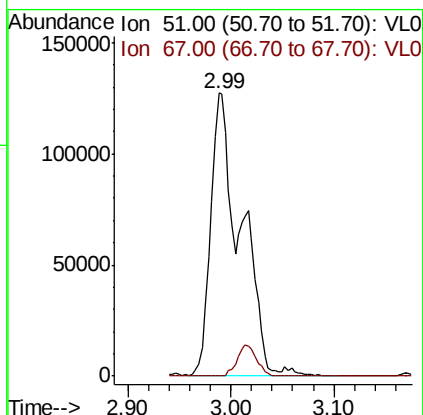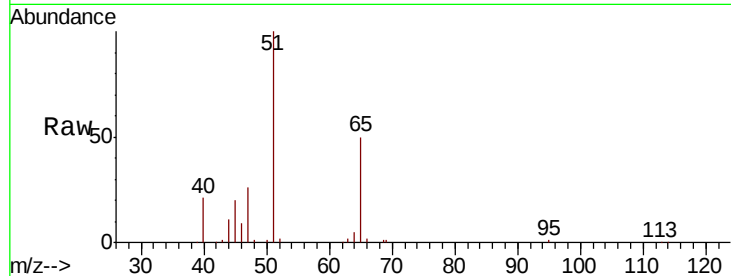

#4

Chloromethane

Concen: 0.506 ppbv

RT: 3.17 min Scan# 73

Delta R.T. -0.00 min

Lab File: VL033347.D




Acq: 16 Mar 2019 1:44


Tgt Ion: 50 Resp: 24988

Ion Ratio Lower Upper

50 100

52 28.7 25.0 37.6

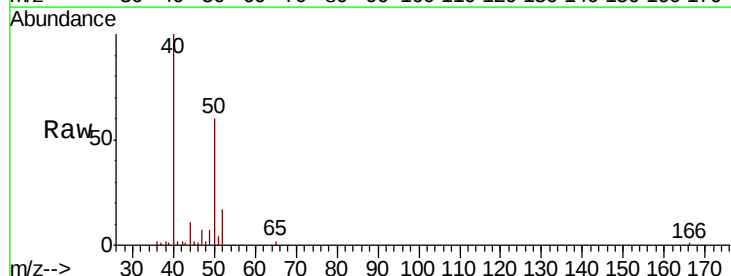



#9

Propene

Concen: 10.590 ppbv

RT: 3.24 min Scan# 94

Delta R.T. 0.20 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 41 Resp: 431345

Ion Ratio Lower Upper

41 100

42 63.5 55.2 82.8

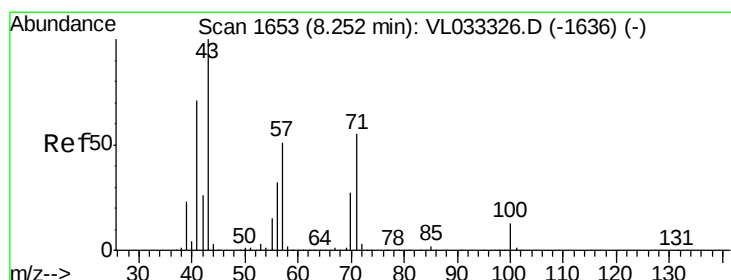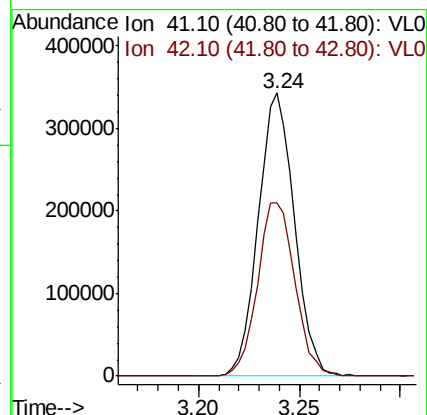

#10

Heptane

Concen: 1.724 ppbv

RT: 8.25 min Scan# 1652

Delta R.T. -0.00 min

Lab File: VL033347.D




Acq: 16 Mar 2019 1:44


Tgt Ion: 43 Resp: 174216

Ion Ratio Lower Upper

43 100

57 50.5 40.4 60.6


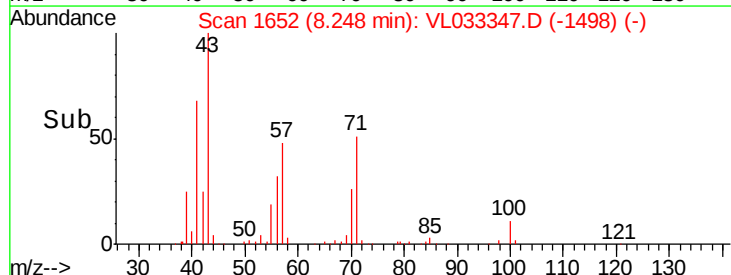
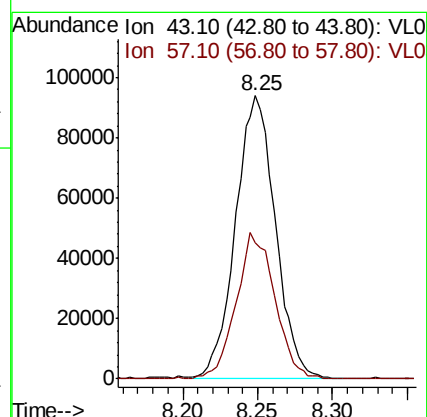



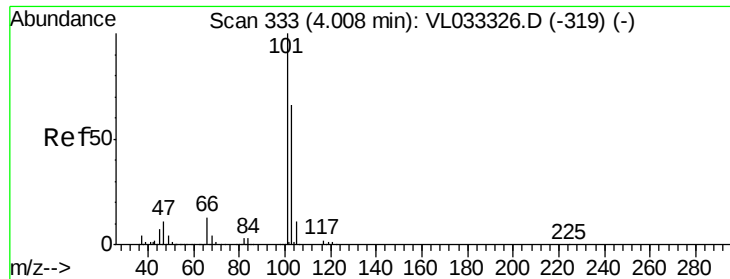

#11
 Trichlorofluoromethane
 Concen: 0.233 ppbv
 RT: 4.01 min Scan# 333
 Delta R.T. -0.00 min
 Lab File: VL033347.D
 Acq: 16 Mar 2019 1:44




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion:101 Resp: 32390
 Ion Ratio Lower Upper
 101 100
 103 61.8 52.9 79.3

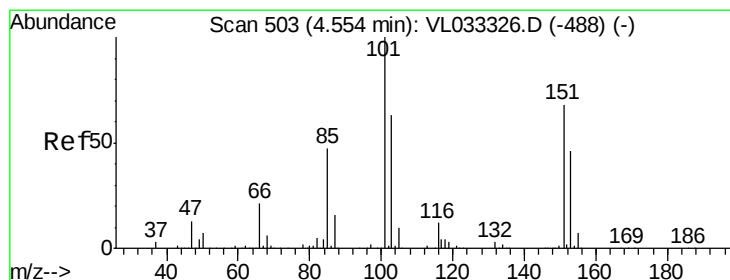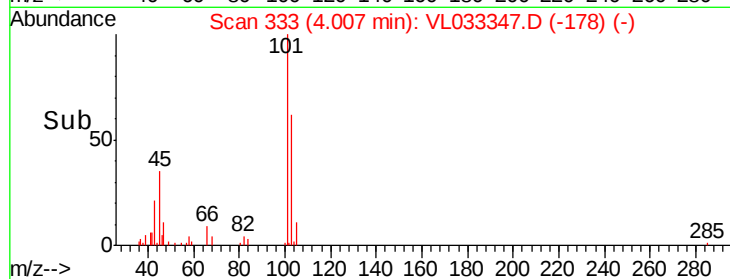

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.033 ppbv
 RT: 4.55 min Scan# 502
 Delta R.T. -0.00 min
 Lab File: VL033347.D
 Acq: 16 Mar 2019 1:44

Tgt Ion:101 Resp: 3012
 Ion Ratio Lower Upper
 101 100
 151 0.0 56.3 84.5#







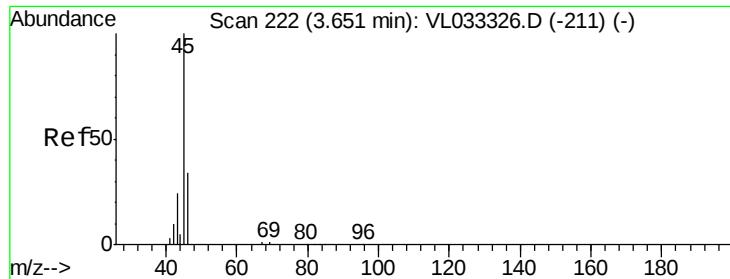

#13
Ethanol
Concen: 102.291 ppbv
RT: 3.66 min Scan# 224
Delta R.T. 0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampled :


Tot Ion: 45 Resp: 1986274
Ion Ratio Lower Upper
45 100
46 35.9 14.9 59.7

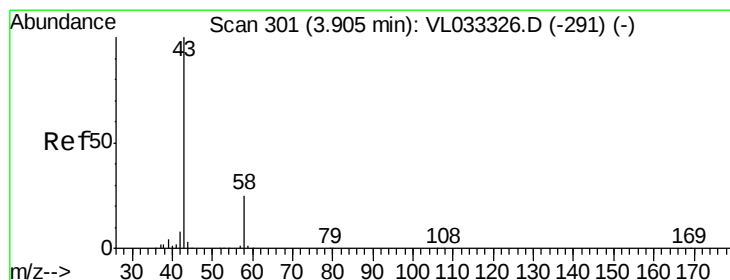

#15
Acetone
Concen: 7.908 ppbv
RT: 3.90 min Scan# 299
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 43 Resp: 977261
Ion Ratio Lower Upper
43 100
58 22.7 20.4 30.6

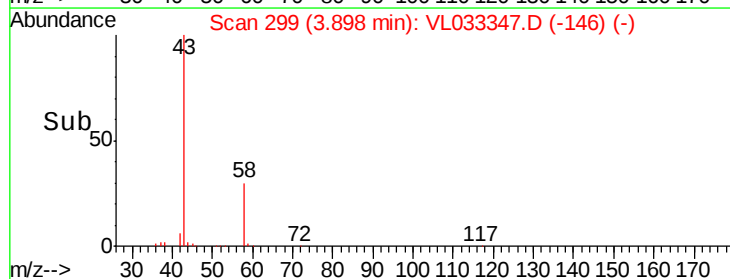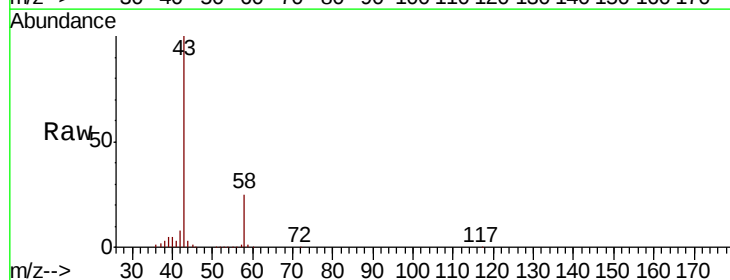



#16

1,3-Butadiene

Concen: 0.115 ppbv

RT: 3.34 min Scan# 126

Delta R.T. -0.02 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 39 Resp: 4602

Ion Ratio Lower Upper

39 100

54 0.0 76.8 115.2#

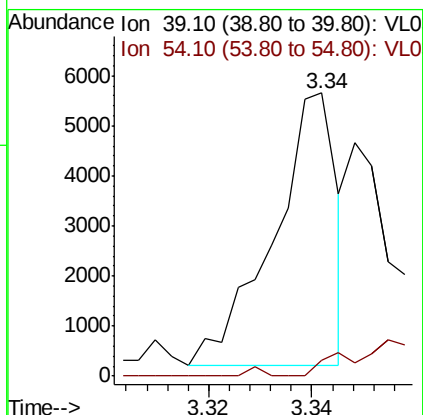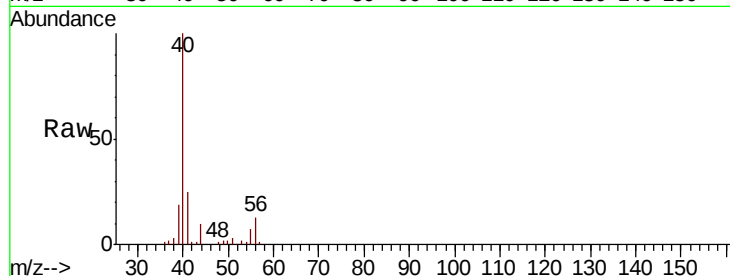

#17

tert-Butyl alcohol

Concen: 0.513 ppbv

RT: 4.37 min Scan# 447

Delta R.T. 0.02 min

Lab File: VL033347.D




Acq: 16 Mar 2019 1:44


Tgt Ion: 59 Resp: 8913

Ion Ratio Lower Upper

59 100

57 0.0 7.7 11.5#


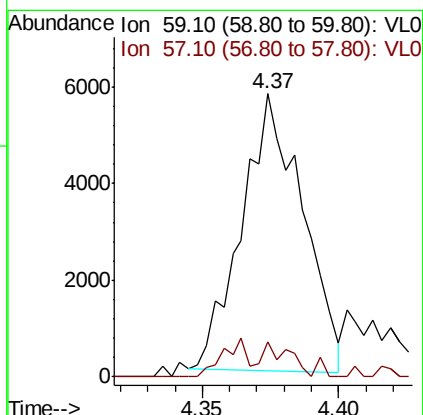




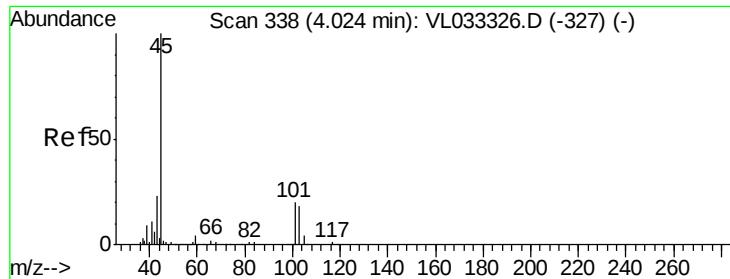

#19
Isopropyl Alcohol
Concen: 10.537 ppbv
RT: 4.04 min Scan# 342
Delta R.T. 0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 45 Resp: 619416
Ion Ratio Lower Upper
45 100
58 2.3 1.5 2.3#

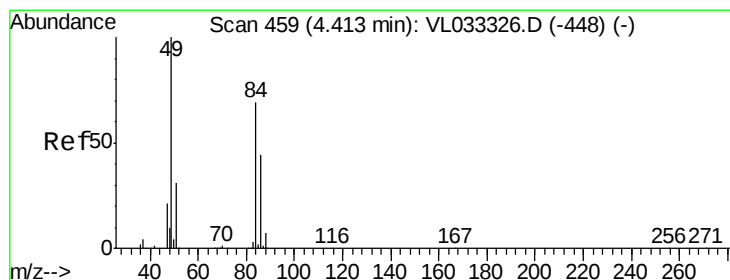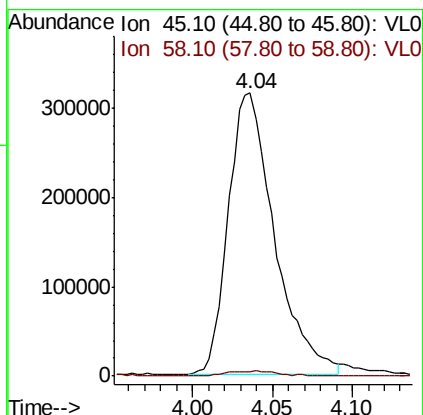

#20
Methylene Chloride
Concen: 2.223 ppbv
RT: 4.41 min Scan# 459
Delta R.T. -0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 84 Resp: 89587
Ion Ratio Lower Upper
84 100
49 144.3 115.4 173.0
51 39.7 35.8 53.6
86 65.9 50.6 75.8



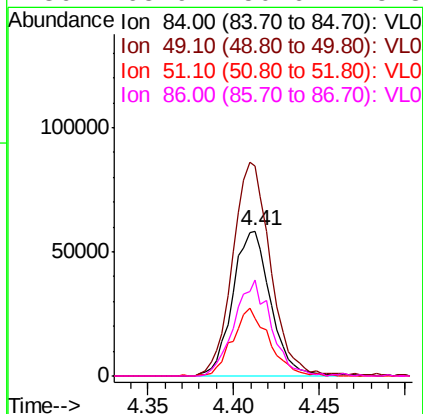



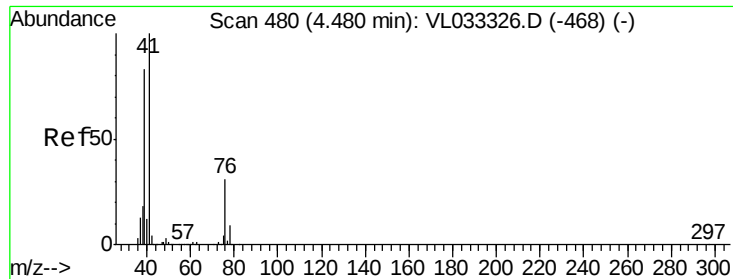

#21
Allvl Chloride
Concen: 0.023 ppbv
RT: 4.42 min Scan# 462
Delta R.T. -0.06 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 41 Resp: 1374
Ion Ratio Lower Upper
41 100
76 0.0 25.0 37.4#
39 129.5 65.9 98.9#

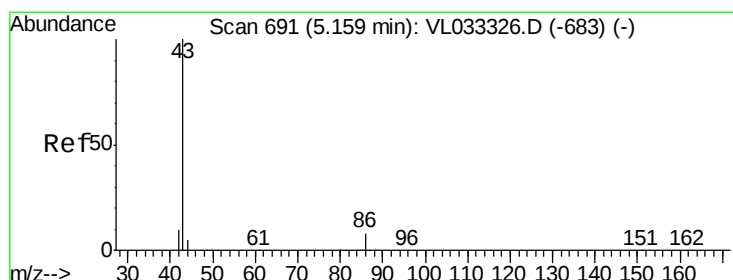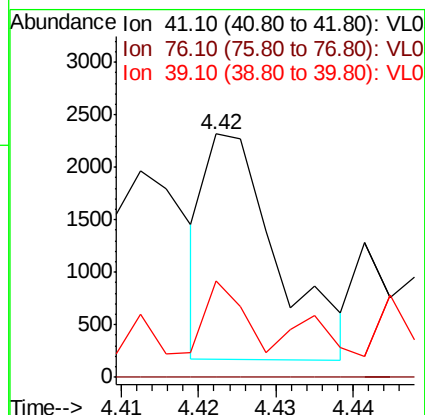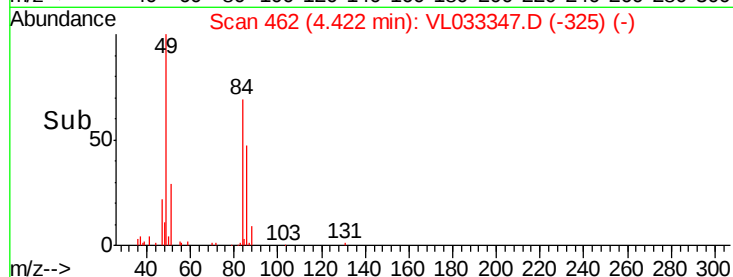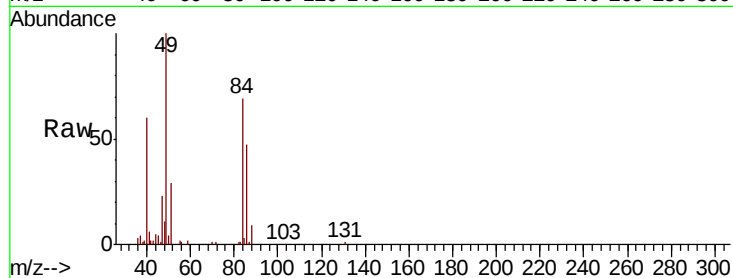

#23
Vinyl Acetate
Concen: 0.255 ppbv
RT: 5.15 min Scan# 687
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 43 Resp: 36465
Ion Ratio Lower Upper
43 100
86 9.2 6.2 9.2
42 54.1 8.1 12.1#
44 7.0 4.1 6.1#


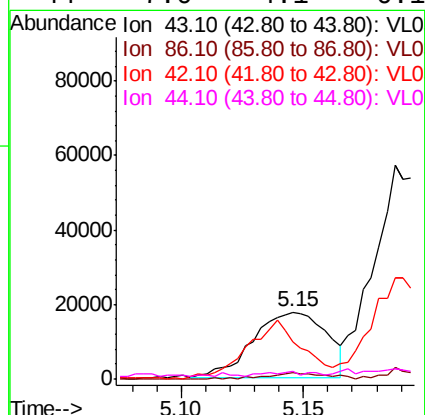
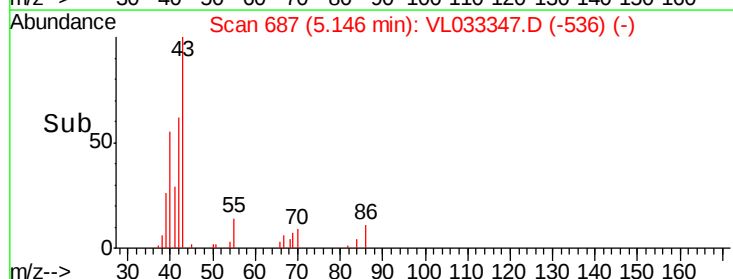
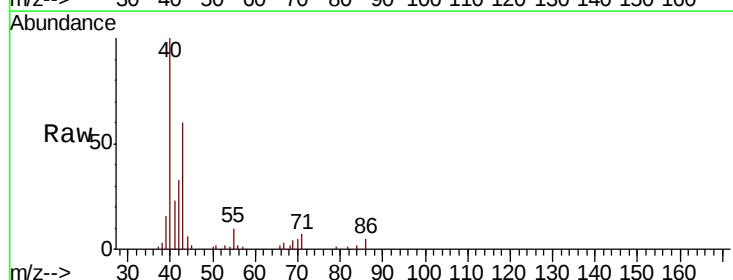




#25
Ethyl Acetate
Concen: 1.484 ppbv
RT: 5.77 min Scan# 882
Delta R.T. 0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion:	43	Resp:	266661
Ion	Ratio	Lower	Upper
43	100		
45	9.1	7.9	11.9
61	6.9	7.4	11.2#
70	6.1	5.7	8.5

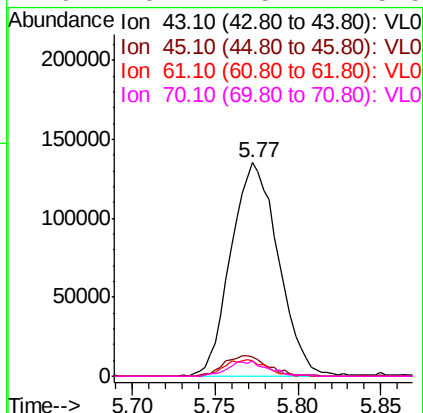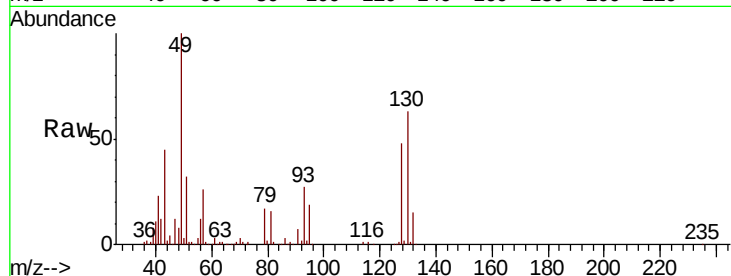

#26
Hexane
Concen: 2.035 ppbv
RT: 5.78 min Scan# 884
Delta R.T. -0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion:	57	Resp:	163426
Ion	Ratio	Lower	Upper
57	100		
41	95.2	70.5	105.7
43	165.2	181.8	272.8#
56	53.7	42.2	63.2

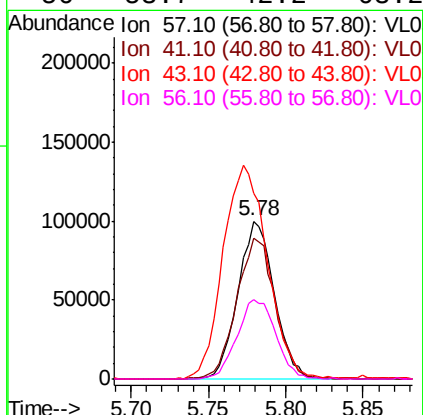



#27

Carbon Disulfide

Concen: 0.051 ppbv

RT: 4.63 min Scan# 526

Delta R.T. 0.01 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L

ClientSampleId :





Tot Ion: 76 Resp: 4682

Ion Ratio Lower Upper

76 100

44 61.4 15.2 22.8#

78 13.6 7.2 10.8#

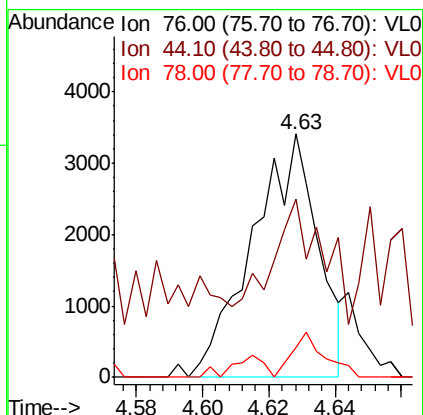

#29

Chloroform

Concen: 0.021 ppbv

RT: 5.84 min Scan# 904

Delta R.T. -0.01 min

Lab File: VL033347.D




Acq: 16 Mar 2019 1:44


Tgt Ion: 83 Resp: 2760

Ion Ratio Lower Upper

83 100

85 57.4 52.0 78.0


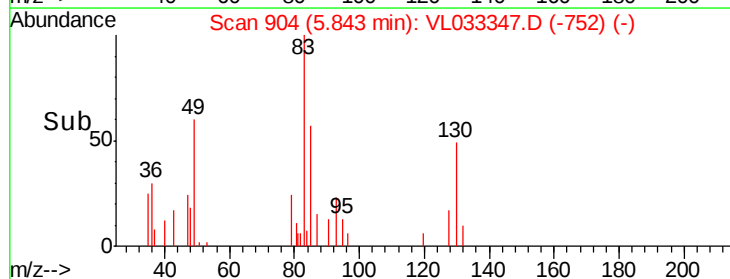






#30
Cyclohexane
Concen: 0.109 ppbv
RT: 7.25 min Scan# 1343
Delta R.T. 0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 84 Resp: 7022
Ion Ratio Lower Upper
84 100
56 201.6 111.3 166.9#
41 174.9 69.6 104.4#

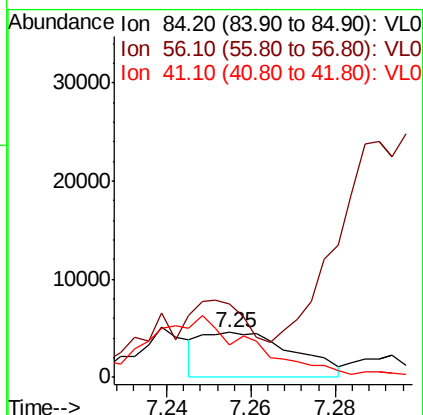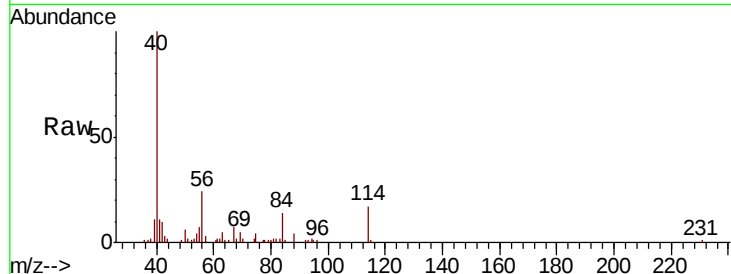

#31
cis-1,2-Dichloroethene
Concen: 0.083 ppbv
RT: 5.76 min Scan# 878
Delta R.T. 0.12 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 61 Resp: 6703
Ion Ratio Lower Upper
61 100
96 3.8 50.3 75.5#
98 0.0 31.5 47.3#



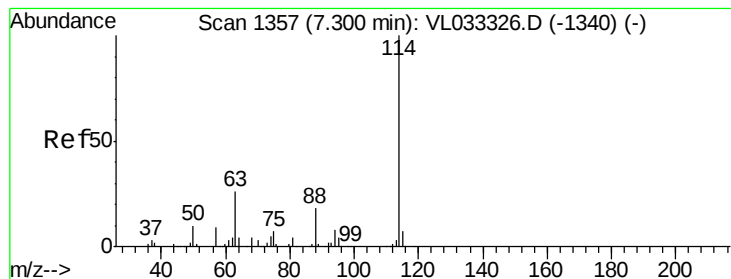

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.29 min Scan# 1355

Delta R.T. -0.01 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L

ClientSampleId :


Tot Ion:114 Resp: 1794141

Ion Ratio Lower Upper




114 100

63 27.4 21.4 32.2

88 18.3 14.5 21.7



Abundance Ion 114.10 (113.80 to 114.80): VL0
Ion 63.10 (62.80 to 63.80): VL0
Ion 88.10 (87.80 to 88.80): VL0

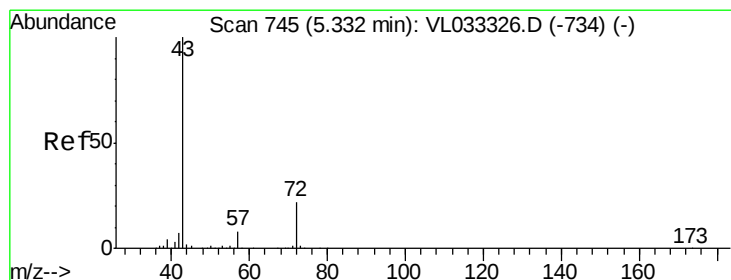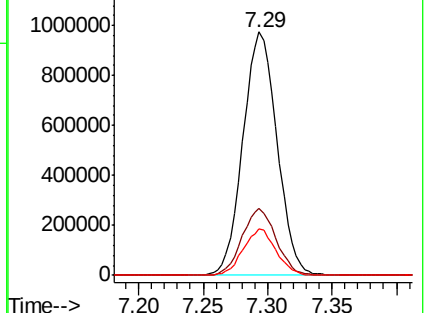

#34

2-Butanone

Concen: 0.755 ppbv

RT: 5.34 min Scan# 746

Delta R.T. 0.00 min

Lab File: VL033347.D


Acq: 16 Mar 2019 1:44

Tgt Ion: 43 Resp: 88970



Ion Ratio Lower Upper


43 100

72 21.8 17.7 26.5



Abundance Ion 43.10 (42.80 to 43.80): VL0
Ion 72.10 (71.80 to 72.80): VL0



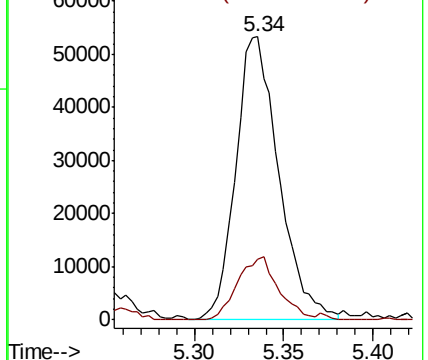





#36
Benzene
Concen: 0.174 ppbv
RT: 7.00 min Scan# 1265
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampled :


Tot Ion: 78 Resp: 27875
Ion Ratio Lower Upper
78 100
77 19.9 18.1 27.1
50 21.7 15.2 22.8

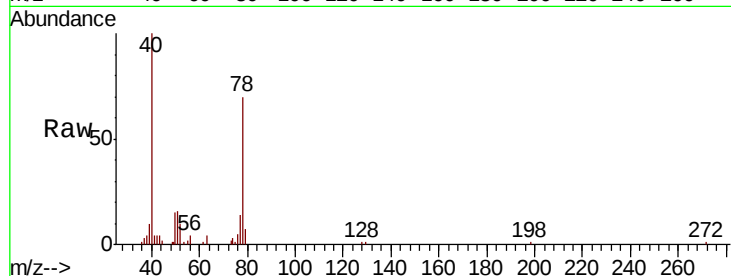

#37
1,2-Dichloroethane
Concen: 0.043 ppbv
RT: 6.41 min Scan# 1081
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 62 Resp: 4399
Ion Ratio Lower Upper
62 100
98 5.8 4.5 6.7







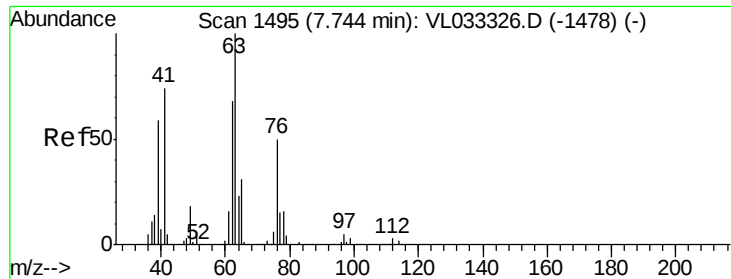

#39
 1,2-Dichloropropane
 Concen: 8.114 ppbv
 RT: 7.29 min Scan# 1355
 Delta R.T. -0.45 min
 Lab File: VL033347.D
 Acq: 16 Mar 2019 1:44




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
63	100		
41	0.0	59.5	89.3#
62	17.1	54.7	82.1#

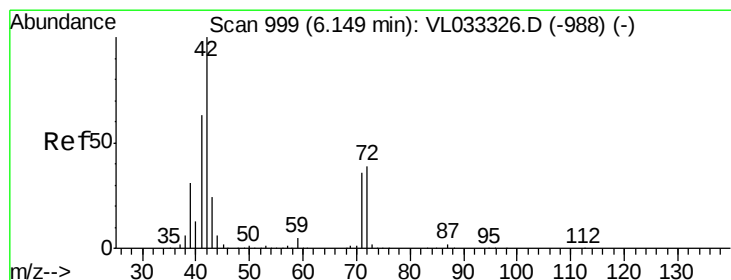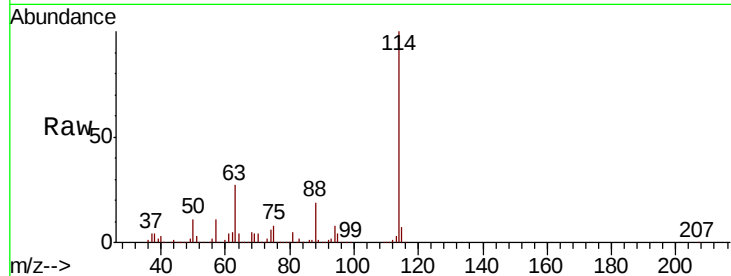

#41
 Tetrahydrofuran
 Concen: 0.024 ppbv
 RT: 6.16 min Scan# 1002
 Delta R.T. 0.01 min
 Lab File: VL033347.D
 Acq: 16 Mar 2019 1:44

Tgt Ion	Ratio	Lower	Upper
42	100		
72	101.8	31.6	47.4#
71	125.0	29.9	44.9#









#43
Methvl Methacrvlate
Concen: 0.046 ppbv
RT: 8.13 min Scan# 1616
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 69 Resp: 2861
Ion Ratio Lower Upper
69 100
41 0.0 119.5 179.3#
100 0.0 24.4 36.6#

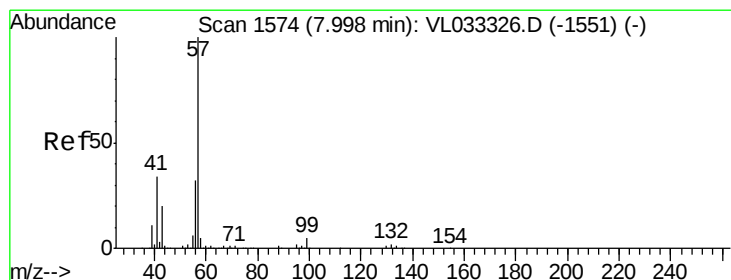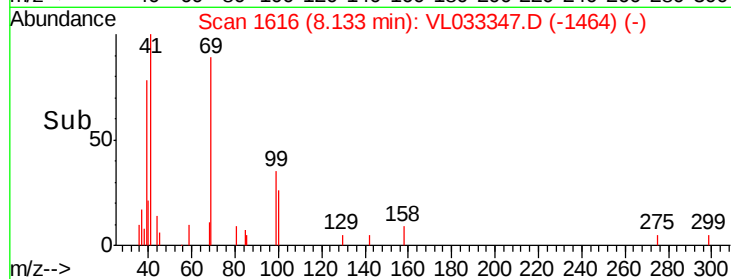

#44
2,2,4-Trimethylpentane
Concen: 0.144 ppbv
RT: 7.99 min Scan# 1572
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 57 Resp: 38284
Ion Ratio Lower Upper
57 100
41 62.8 26.0 39.0#
56 57.8 24.6 36.8#

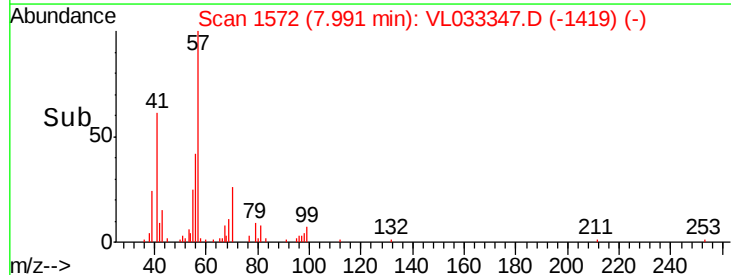

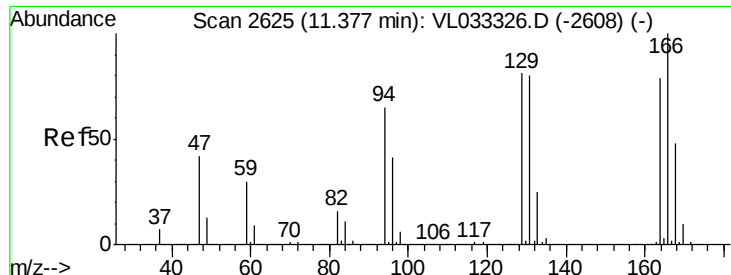

#52

Tetrachloroethene

Concen: 0.029 ppbv

RT: 11.37 min Scan# 2622

Delta R.T. -0.01 min

Lab File: VL033347.D

Acq: 16 Mar 2019 1:44

Instrument :

MSVOA_L

ClientSampleId :

Tot Ion:164 Resp: 1951


Ion Ratio Lower Upper

164 100

166 67.7 101.5 152.3#

129 93.3 82.2 123.2

131 76.3 81.1 121.7#



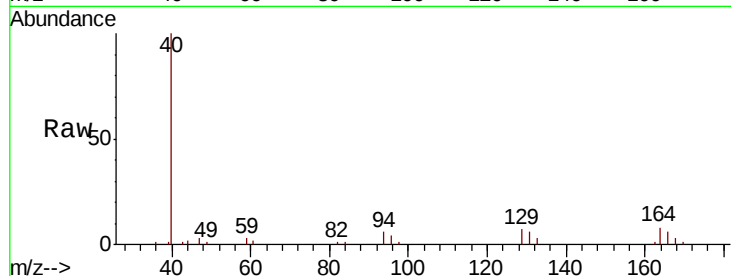


Abundance Ion 163.90 (163.60 to 164.60): V

Ion 165.90 (165.60 to 166.60): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

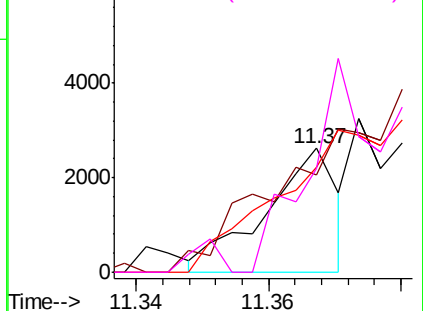

#53

Toluene

Concen: 18.470 ppbv

RT: 9.95 min Scan# 2181

Delta R.T. -0.00 min

Lab File: VL033347.D


Acq: 16 Mar 2019 1:44

Tgt Ion: 91 Resp: 3369824

Ion Ratio Lower Upper



91 100


92 59.4 47.4 71.0



Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 92.10 (91.80 to 92.80): VL0




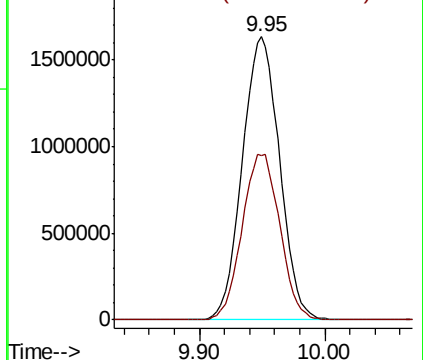




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.25 min Scan# 2895
Delta R.T. -0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion:117 Resp: 1738192
Ion Ratio Lower Upper
117 100
82 68.1 53.4 80.2
119 32.2 27.3 40.9

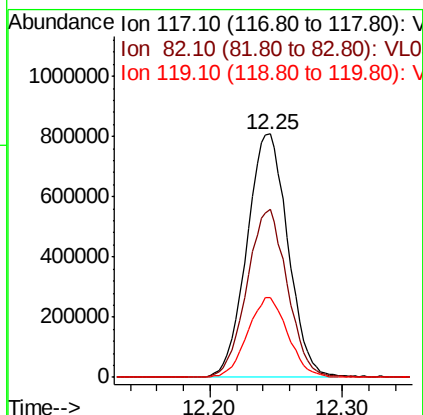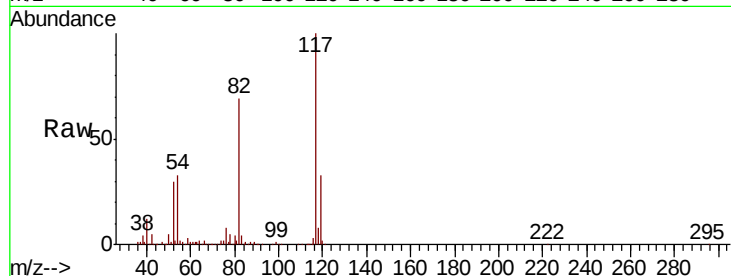

#58
Ethyl Benzene
Concen: 0.400 ppbv
RT: 12.87 min Scan# 3089
Delta R.T. -0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 91 Resp: 98298
Ion Ratio Lower Upper
91 100
106 32.5 24.2 36.2


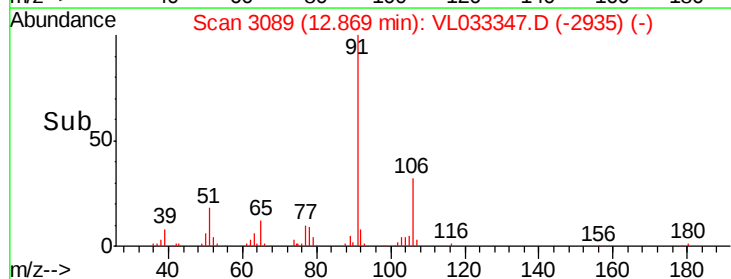




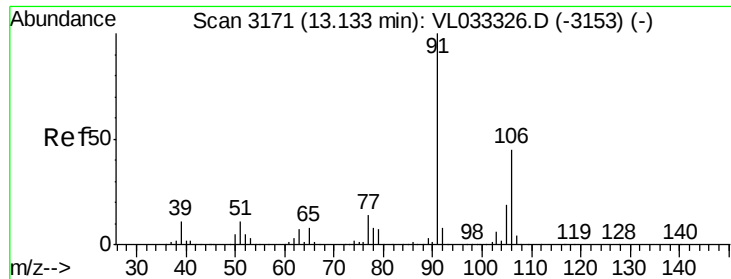

#59
m/p-Xylene
Concen: 0.529 ppbv
RT: 13.12 min Scan# 3168
Delta R.T. -0.01 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 91 Resp: 111854
Ion Ratio Lower Upper
91 100
106 46.4 0.0 0.0#

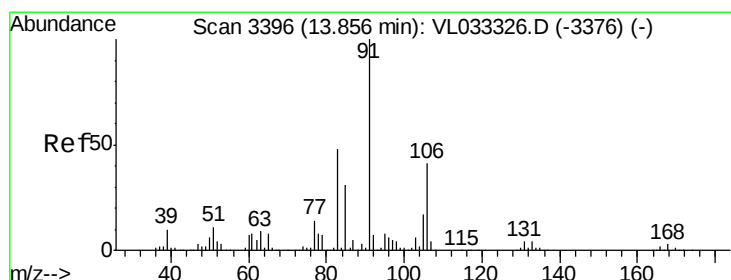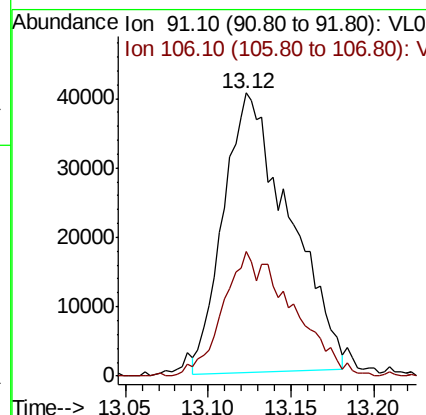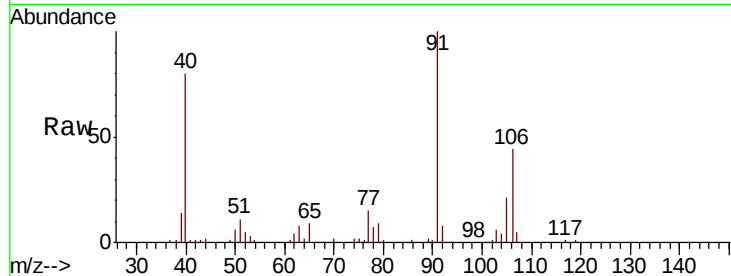

#60
o-Xylene
Concen: 0.087 ppbv
RT: 13.86 min Scan# 3396
Delta R.T. -0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 91 Resp: 17931
Ion Ratio Lower Upper
91 100
106 86.6 21.3 63.9#



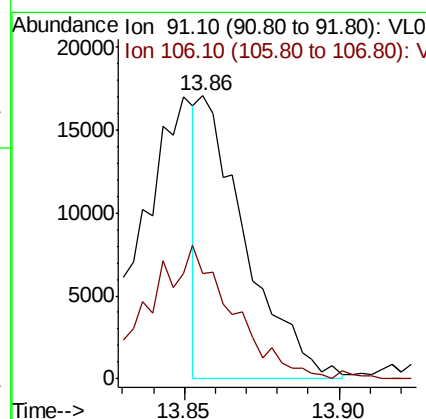





#61
Stvrene
Concen: 0.040 ppbv
RT: 13.70 min Scan# 3346
Delta R.T. 0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Instrument :
MSVOA_L
ClientSampled :

Tot Ion:104 Resp: 5794
Ion Ratio Lower Upper
104 100
78 0.0 42.7 64.1#
103 0.0 38.0 57.0#

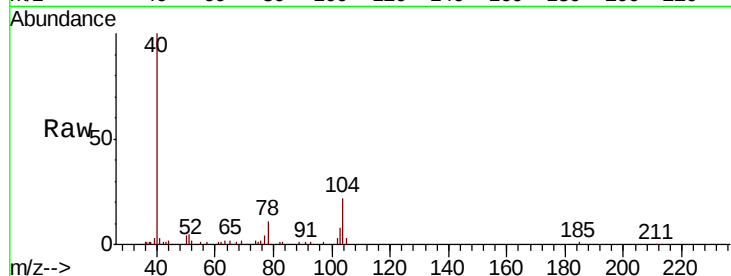

#68
1-Bromo-4-Fluorobenzene
Concen: 10.110 ppbv
RT: 14.58 min Scan# 3621
Delta R.T. -0.00 min
Lab File: VL033347.D
Acq: 16 Mar 2019 1:44

Tgt Ion: 95 Resp: 1302146
Ion Ratio Lower Upper
95 100
174 64.4 51.5 77.3
175 4.6 3.8 5.6

